

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122818\
 Data File : FF003113.D
 Signal(s) : FID2B.ch
 Acq On : 28 Dec 2018 18:15
 Operator : AJ\SJ
 Sample : J6193-17MS 10X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Dec 28 21:04:25 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
 Quant Title :
 QLast Update : Tue Dec 04 16:40:56 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.633	255298	1.966 ug/ml
Target Compounds			
2) N-DECANE	4.360	244370	1.560 ug/ml
3) N-DODECANE	6.380	266409	1.678 ug/ml
4) N-TETRADECANE	8.174	237483	1.482 ug/ml
5) N-HEXADECANE	9.773	270394	1.688 ug/mlm
6) N-OCTADECANE	11.217	270302	1.706 ug/ml
7) N-EICOSANE	12.530	304013	1.971 ug/ml
8) N-DOCOSANE	13.730	305581	2.044 ug/mlm
10) N-TETRACOSANE	14.836	291014	2.014 ug/ml
11) N-HEXACOSANE	15.861	290939	2.084 ug/mlm
12) N-OCTACOSANE	16.811	353222	2.636 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122818\
Data File : FF003113.D
Signal(s) : FID2B.ch
Acq On : 28 Dec 2018 18:15
Operator : AJ\SJ
Sample : J6193-17MS 10X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Dec 28 21:04:25 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120418.M
Quant Title :
QLast Update : Tue Dec 04 16:40:56 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

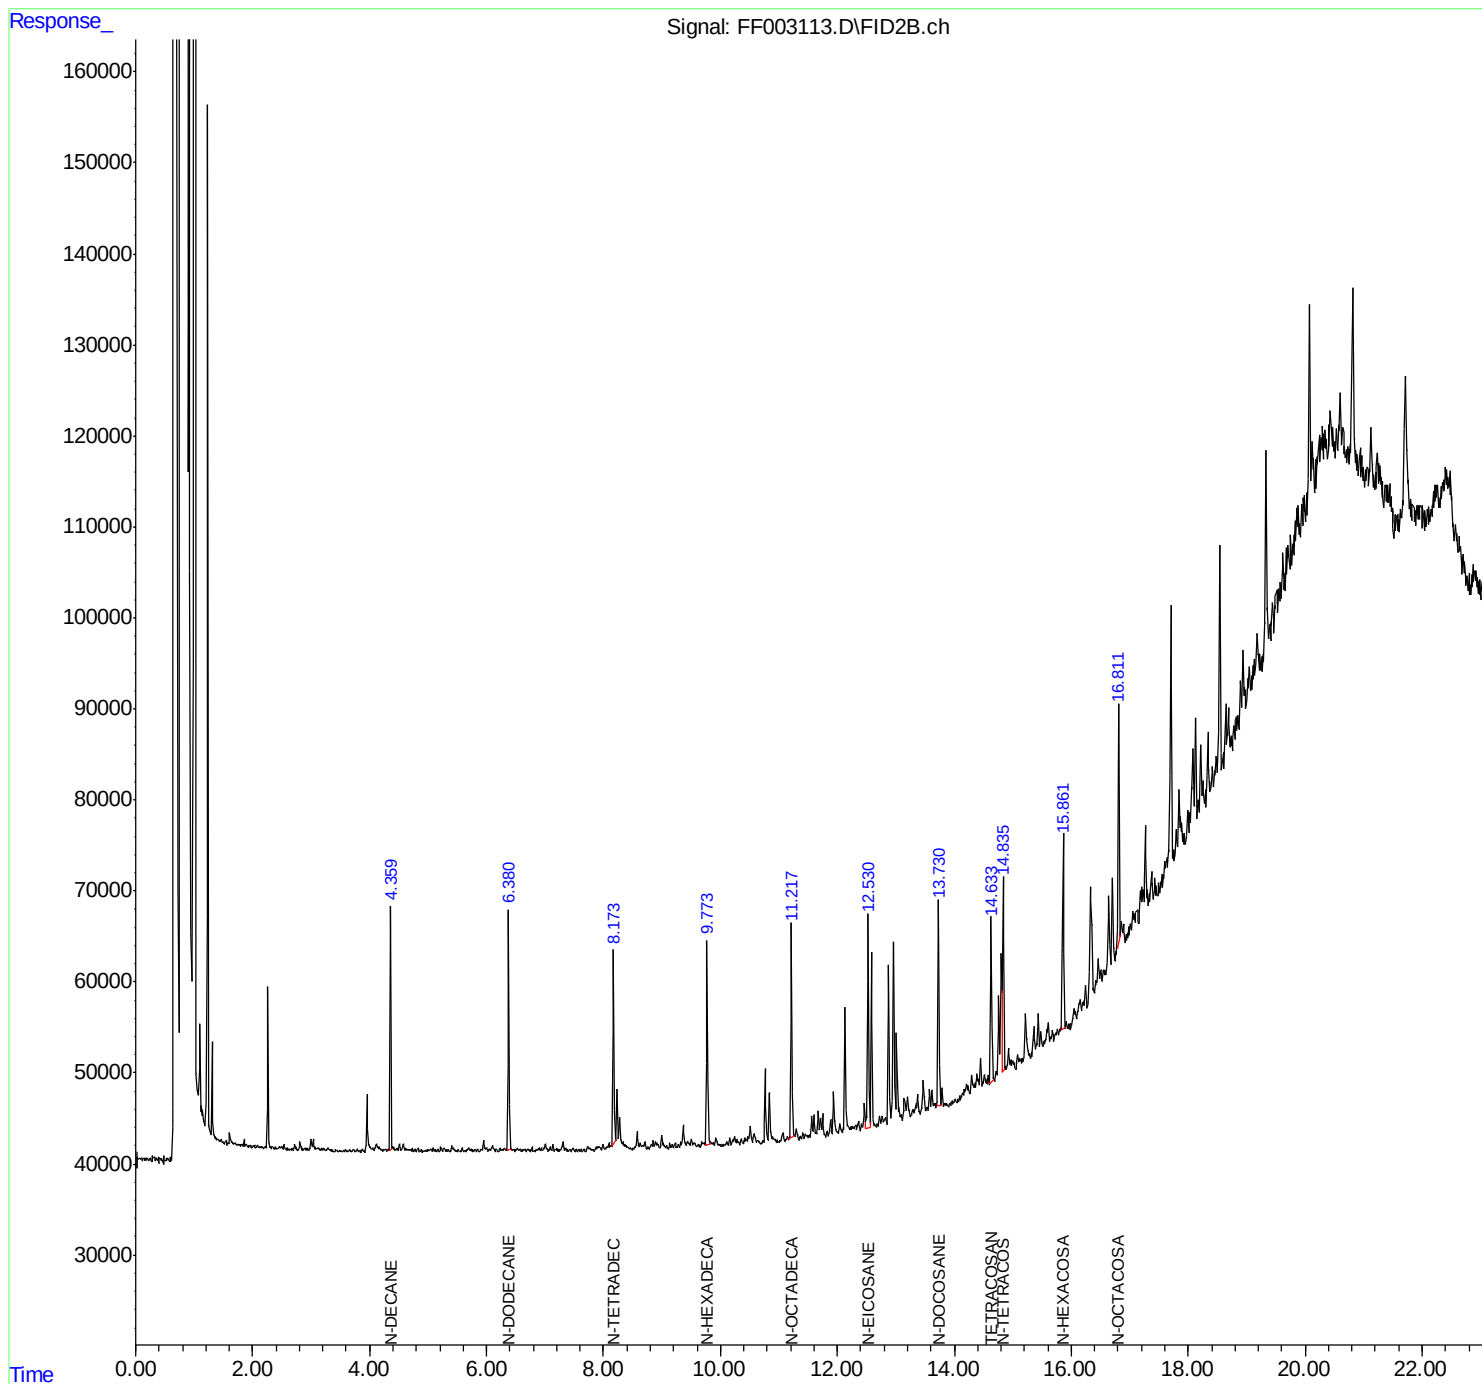

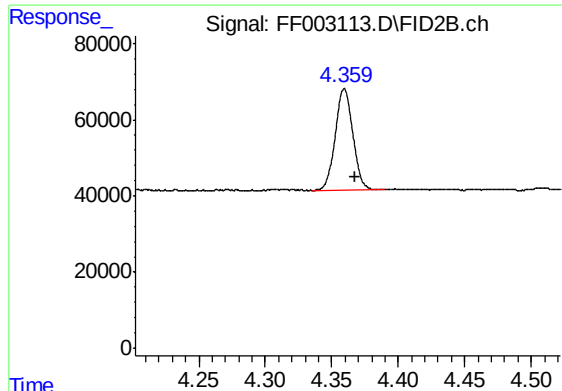


#2 N-DECANE

R.T.: 4.360 min
Delta R.T.: -0.008 min
Response: 244370
Conc: 1.56 ug/ml

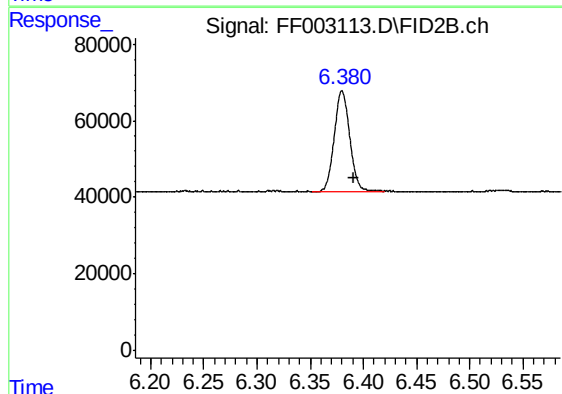


#3 N-DODECANE

R.T.: 6.380 min
Delta R.T.: -0.011 min
Response: 266409
Conc: 1.68 ug/ml

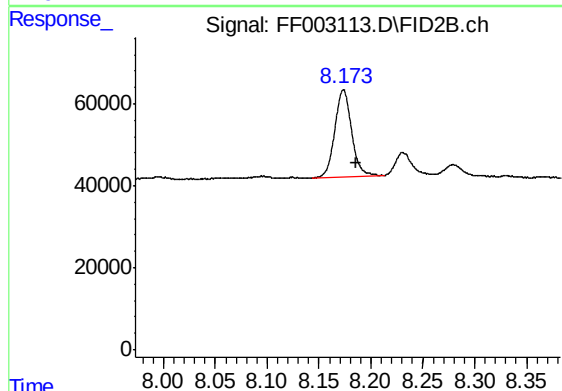


#4 N-TETRADECANE

R.T.: 8.174 min
Delta R.T.: -0.012 min
Response: 237483
Conc: 1.48 ug/ml

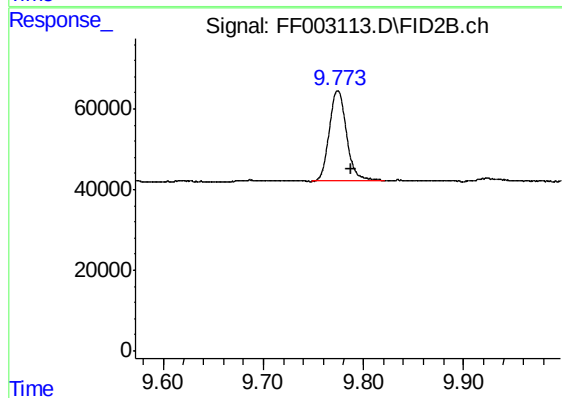


#5 N-HEXADECANE

R.T.: 9.773 min
Delta R.T.: -0.014 min
Response: 270394
Conc: 1.69 ug/ml m

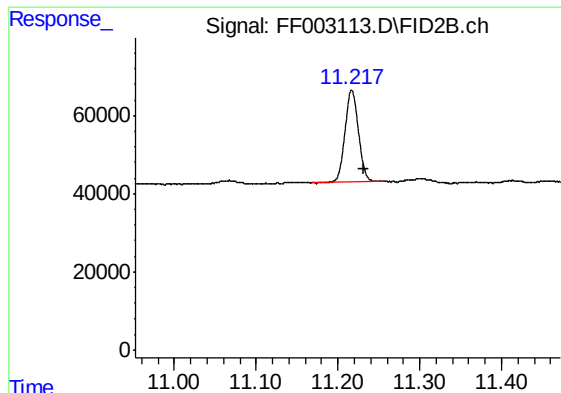


#6 N-OCTADECANE

R.T.: 11.217 min
Delta R.T.: -0.014 min
Response: 270302
Conc: 1.71 ug/ml

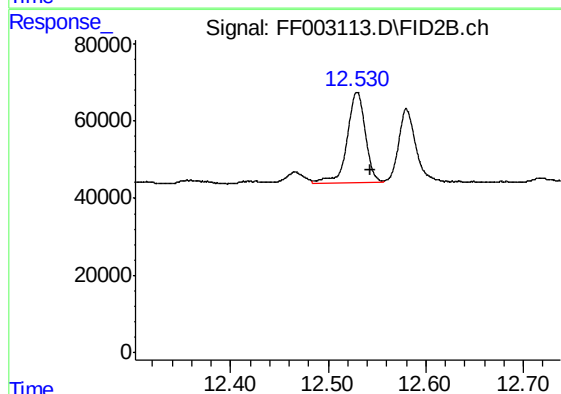


#7 N-EICOSANE

R.T.: 12.530 min
Delta R.T.: -0.014 min
Response: 304013
Conc: 1.97 ug/ml

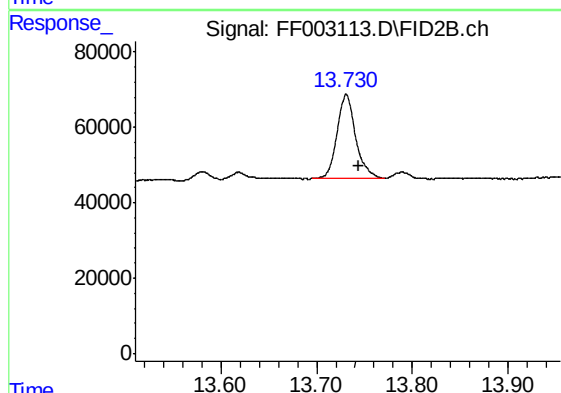


#8 N-DOCOSANE

R.T.: 13.730 min
Delta R.T.: -0.014 min
Response: 305581
Conc: 2.04 ug/ml m

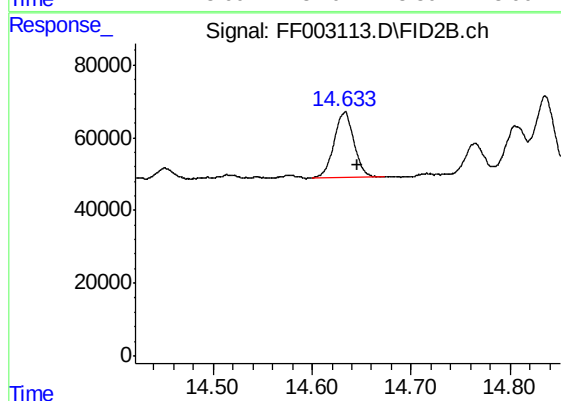


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.633 min
Delta R.T.: -0.012 min
Response: 255298
Conc: 1.97 ug/ml

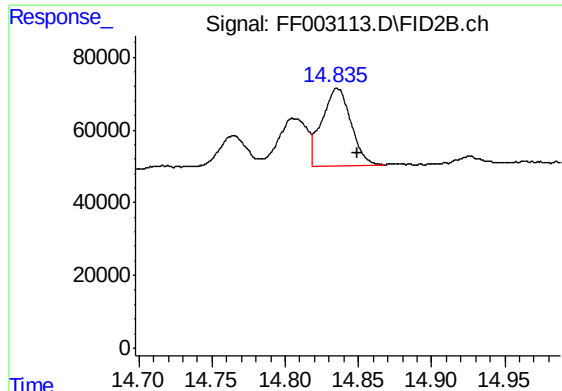


#10 N-TETRACOSANE

R.T.: 14.836 min
Delta R.T.: -0.014 min
Response: 291014
Conc: 2.01 ug/ml

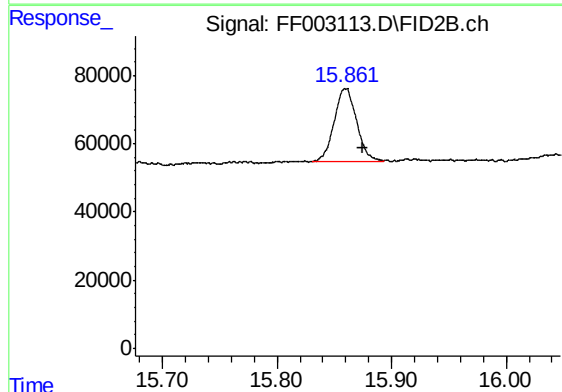

#11 N-HEXACOSANE

R.T.: 15.861 min
Delta R.T.: -0.013 min
Response: 290939
Conc: 2.08 ug/ml m

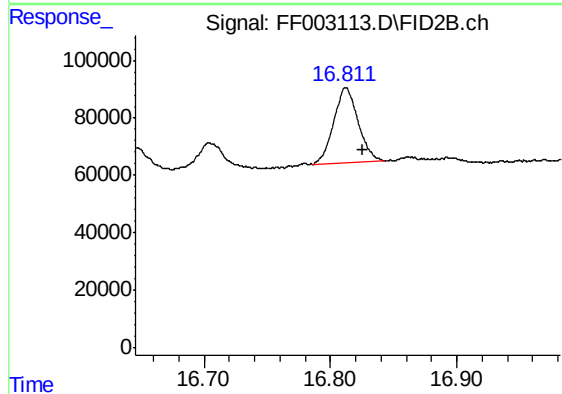

#12 N-OCTACOSANE

R.T.: 16.811 min
Delta R.T.: -0.014 min
Response: 353222
Conc: 2.64 ug/ml m