

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122821\
 Data File : FF009573.D
 Signal(s) : FID2B.ch
 Acq On : 28 Dec 2021 11:20
 Operator : AJ\MA
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Dec 29 00:37:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
 Quant Title :
 QLast Update : Thu Dec 16 03:33:07 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.262	3147934	21.768 ug/ml
4)	N-TETRADECANE	8.047	53267	0.366 ug/ml
5)	N-HEXADECANE	9.640	53622	0.373 ug/ml
6)	N-OCTADECANE	11.075	58967	0.409 ug/ml
7)	N-EICOSANE	12.380	59077	0.417 ug/ml
8)	N-DOCOSANE	13.573	54636	0.401 ug/ml
10)	N-TETRACOSANE	14.670	54001	0.410 ug/ml
11)	N-HEXACOSANE	15.688	55873	0.447 ug/ml
12)	N-OCTACOSANE	16.635	2481302	20.838 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122821\
Data File : FF009573.D
Signal(s) : FID2B.ch
Acq On : 28 Dec 2021 11:20
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 29 00:37:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

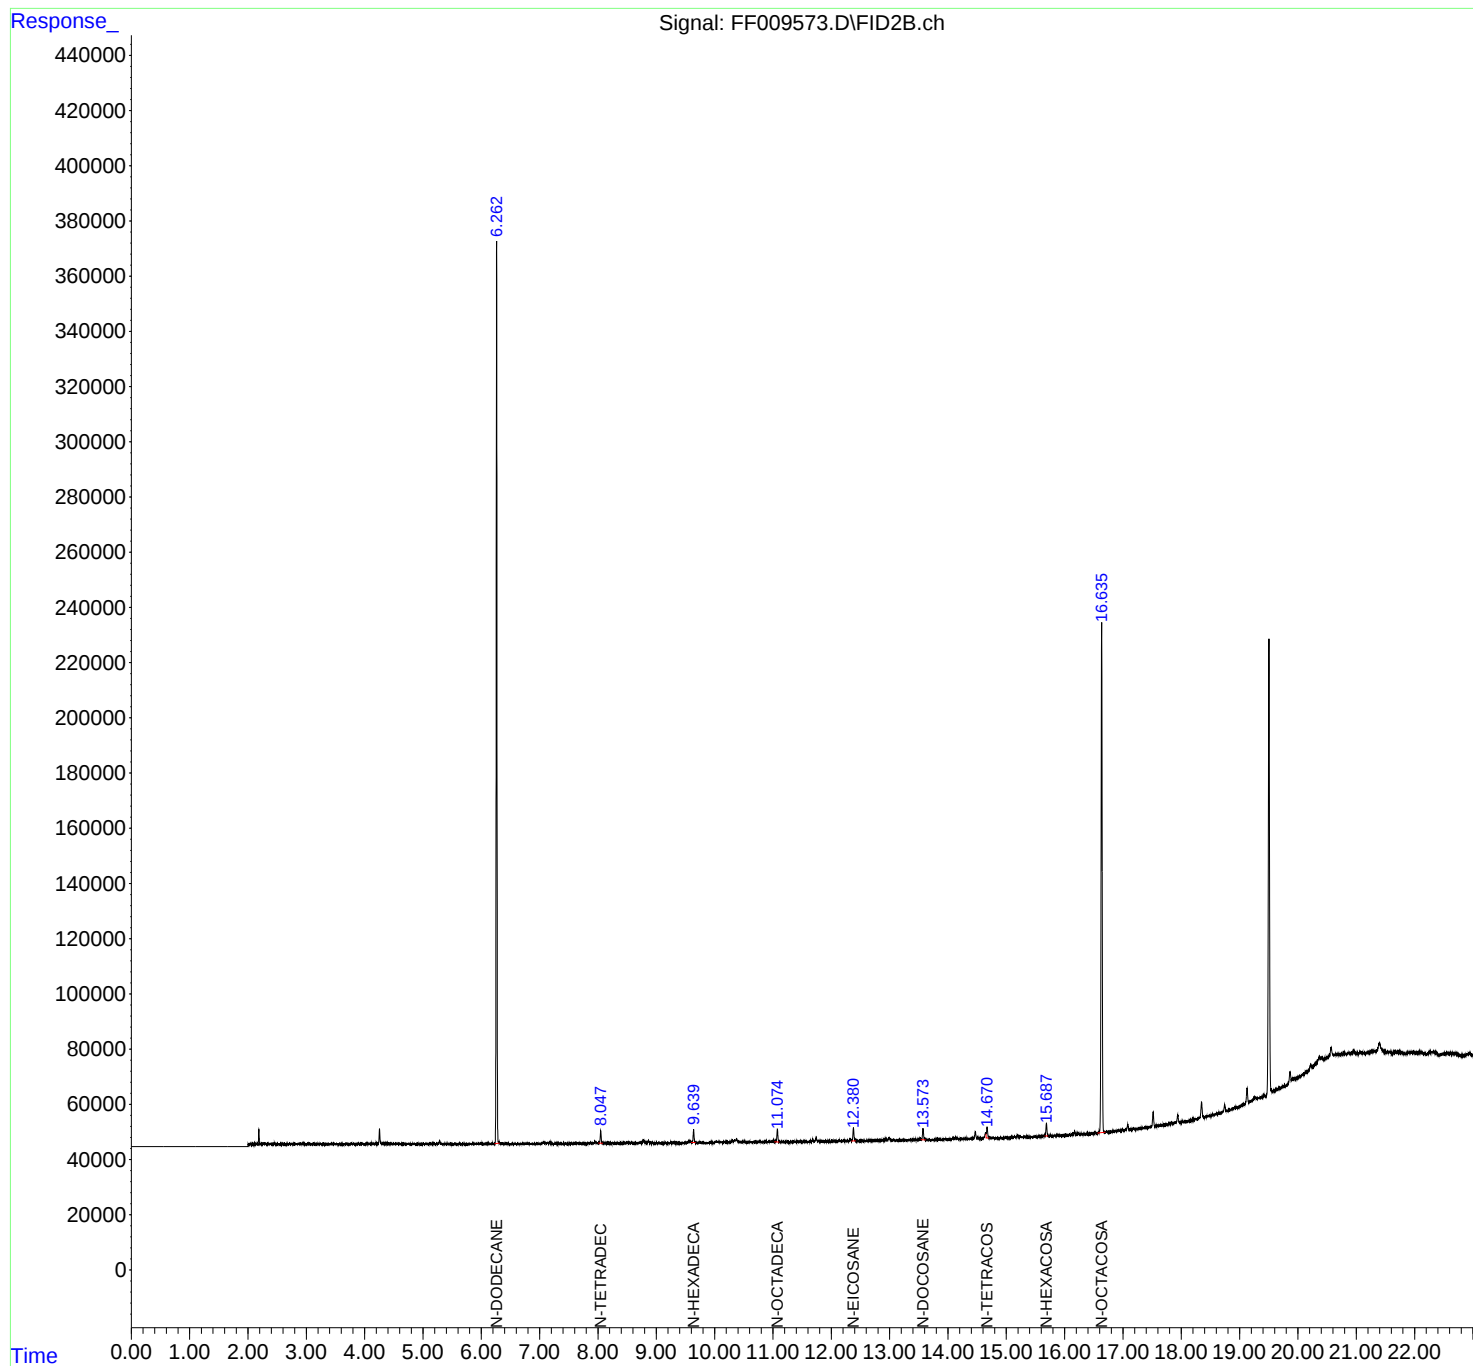


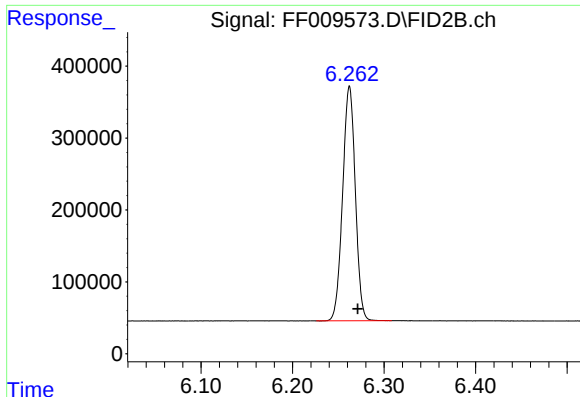

#3 N-DODECANE


R.T.: 6.262 min
Delta R.T.: -0.009 min
Response: 3147934
Conc: 21.77 ug/ml

Instrument :
FID_F
ClientSampleId :

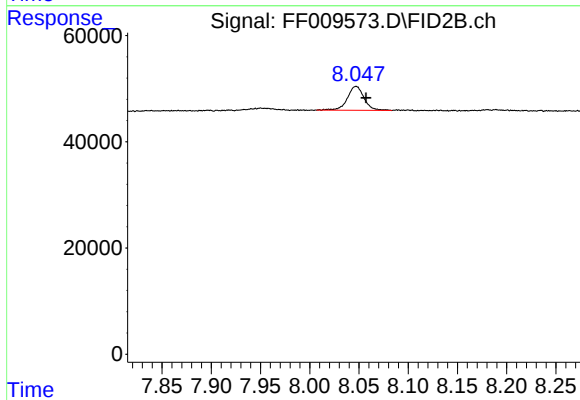


#4 N-TETRADECANE

R.T.: 8.047 min
Delta R.T.: -0.010 min
Response: 53267
Conc: 0.37 ug/ml

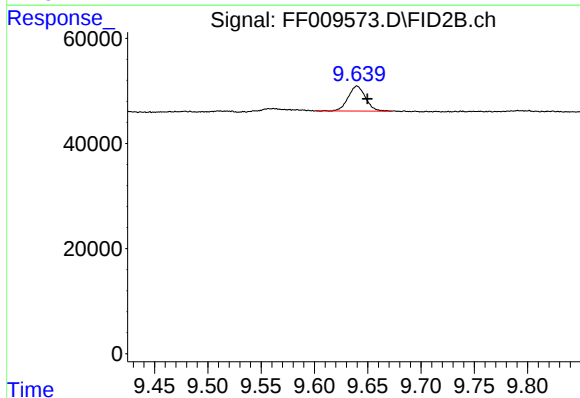


#5 N-HEXADECANE

R.T.: 9.640 min
Delta R.T.: -0.010 min
Response: 53622
Conc: 0.37 ug/ml

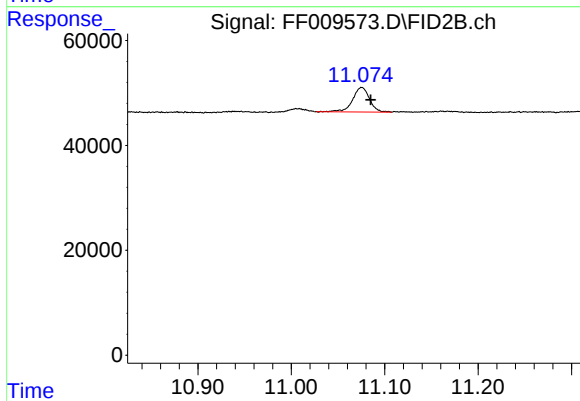

#6 N-OCTADECANE


R.T.: 11.075 min
Delta R.T.: -0.010 min
Response: 58967
Conc: 0.41 ug/ml

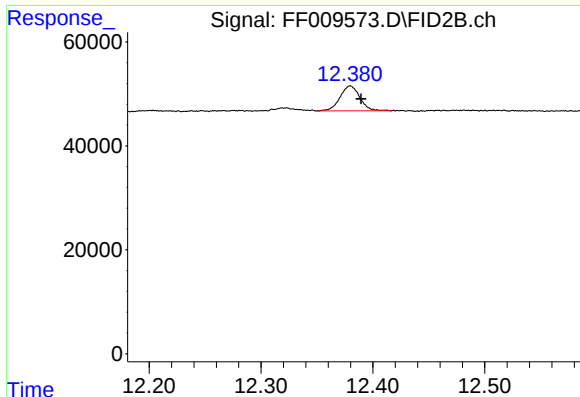

#7 N-EICOSANE


R.T.: 12.380 min
Delta R.T.: -0.009 min
Response: 59077
Conc: 0.42 ug/ml

Instrument :
FID_F
ClientSampleId :

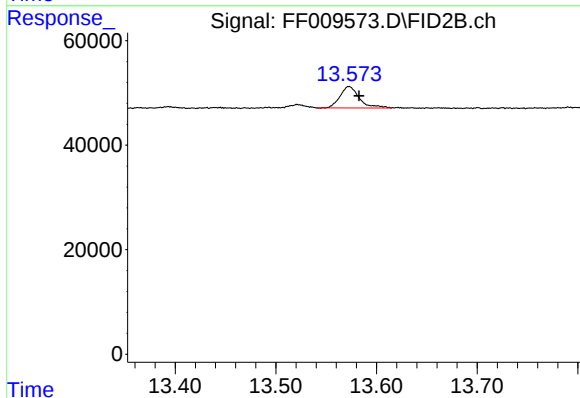


#8 N-DOCOSANE

R.T.: 13.573 min
Delta R.T.: -0.009 min
Response: 54636
Conc: 0.40 ug/ml

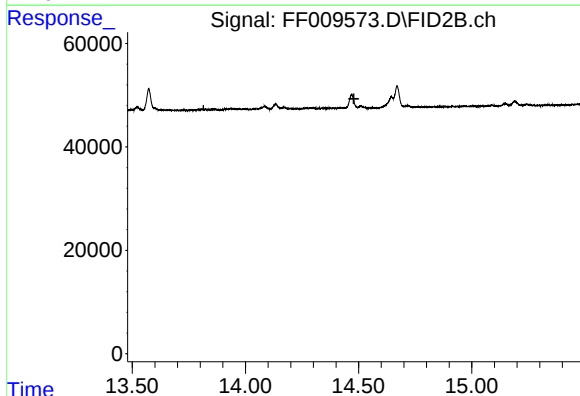


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.479 min
Response: 0
Conc: N.D.

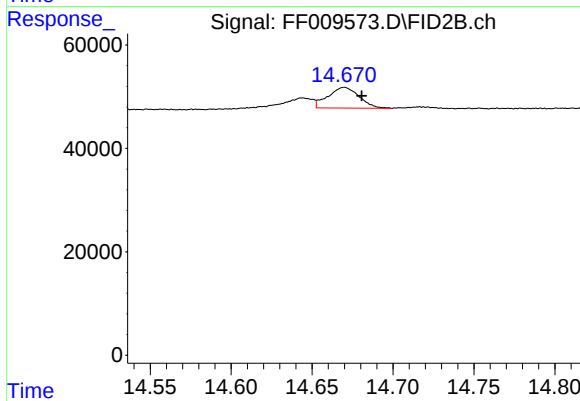

#10 N-TETRACOSANE


R.T.: 14.670 min
Delta R.T.: -0.010 min
Response: 54001
Conc: 0.41 ug/ml

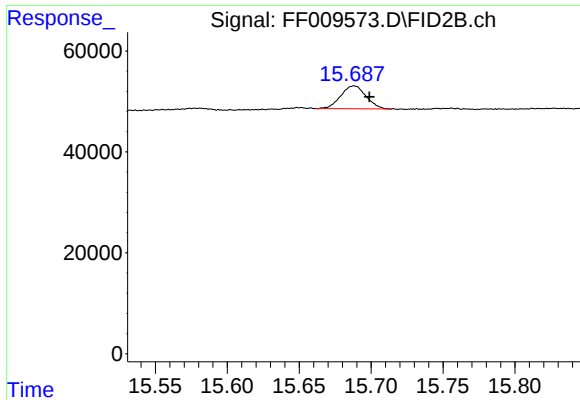

#11 N-HEXACOSANE

R.T.: 15.688 min
Delta R.T.: -0.011 min
Response: 55873
Conc: 0.45 ug/ml

Instrument :
FID_F
ClientSampleId :

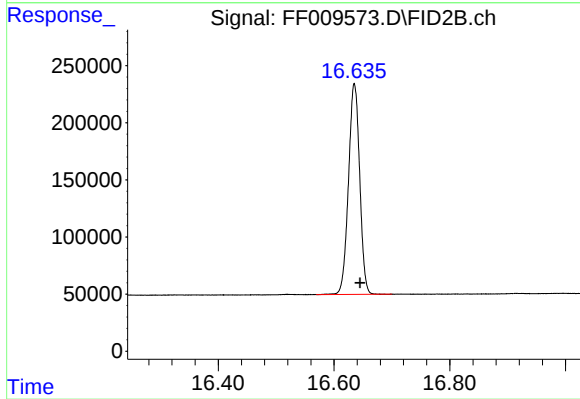

#12 N-OCTACOSANE

R.T.: 16.635 min
Delta R.T.: -0.010 min
Response: 2481302
Conc: 20.84 ug/ml