

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122921\
Data File : FF009589.D
Signal(s) : FID2B.ch
Acq On : 29 Dec 2021 11:05
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 29 12:04:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.260	3501737	24.214 ug/ml
12)	N-OCTACOSANE	16.631	2759042	23.170 ug/ml
13)	N-TRIACONTANE	17.515	102069	0.891 ug/ml
14)	N-DOTRIACONTANE	18.342	134773	1.233 ug/ml
15)	N-TETRATRIACONTANE	19.123	114486	1.081 ug/ml
16)	N-HEXATRIACONTANE	19.861	93668	0.935 ug/ml
17)	N-OCTATRIACONTANE	20.566	347263	3.536 ug/ml
18)	N-TETRACONTANE	21.388	212764	2.107 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF122921\
Data File : FF009589.D
Signal(s) : FID2B.ch
Acq On : 29 Dec 2021 11:05
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Dec 29 12:04:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF121521.M
Quant Title :
QLast Update : Thu Dec 16 03:33:07 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

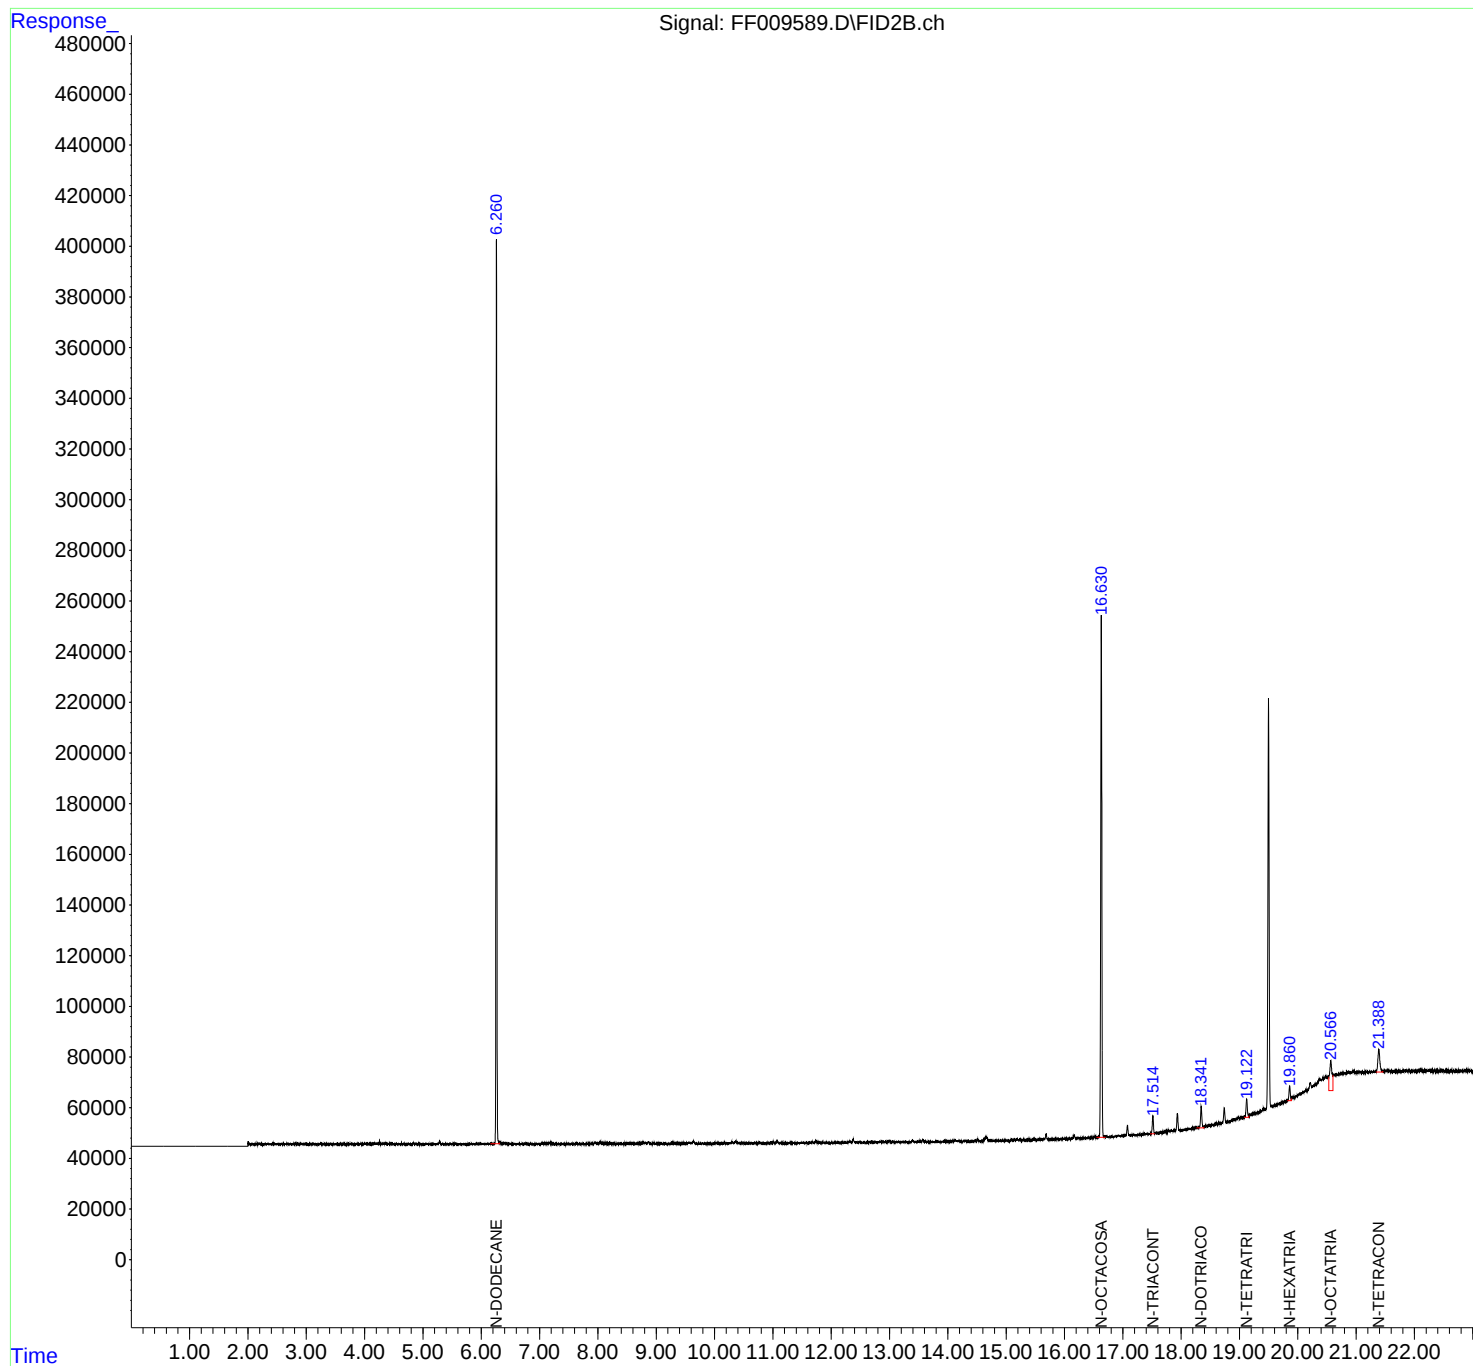


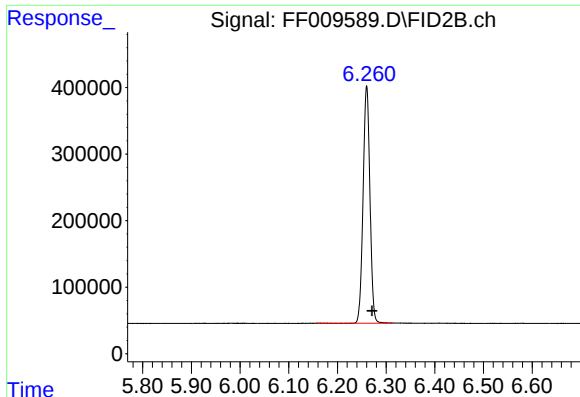

#3 N-DODECANE


R.T.: 6.260 min
Delta R.T.: -0.011 min
Response: 3501737
Conc: 24.21 ug/ml

Instrument :
FID_F
ClientSampleId :

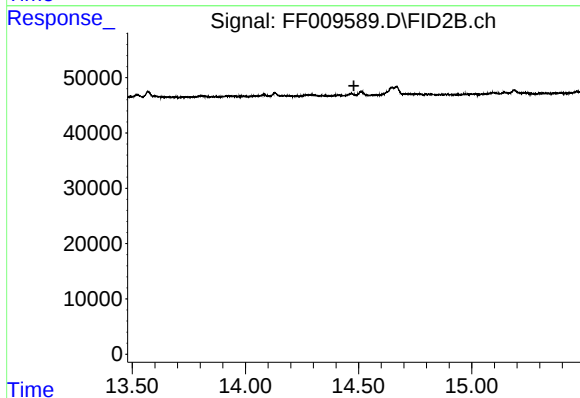


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.479 min
Response: 0
Conc: N.D.

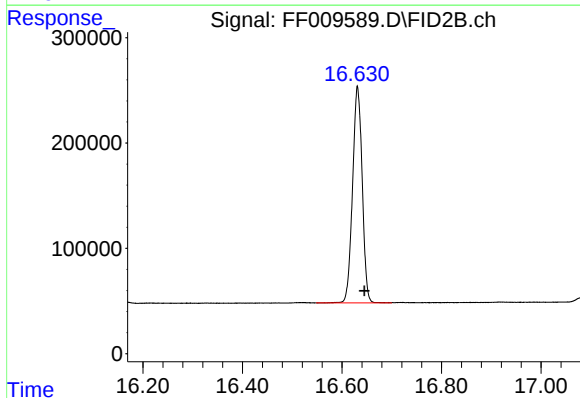


#12 N-OCTACOSANE

R.T.: 16.631 min
Delta R.T.: -0.014 min
Response: 2759042
Conc: 23.17 ug/ml

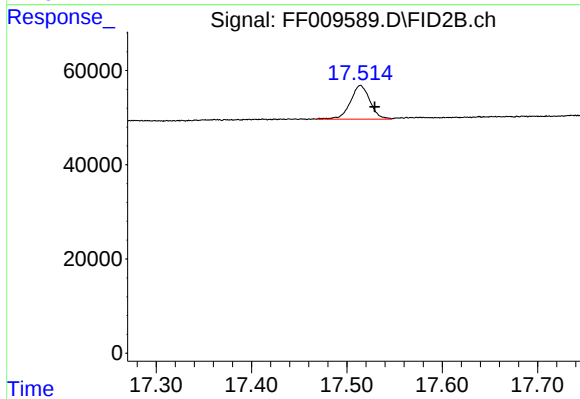

#13 N-TRIACONTANE


R.T.: 17.515 min
Delta R.T.: -0.015 min
Response: 102069
Conc: 0.89 ug/ml

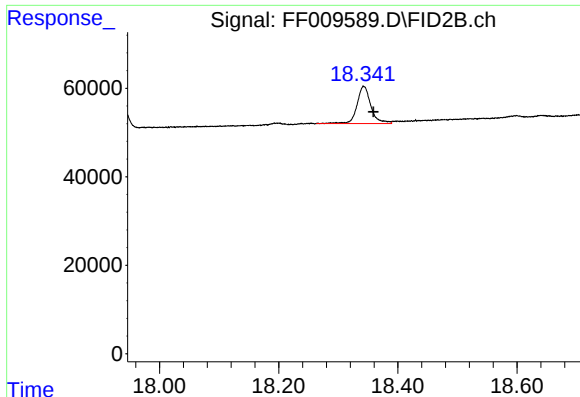

#14 N-DOTRIACONTANE


R.T.: 18.342 min
Delta R.T.: -0.017 min
Response: 134773
Conc: 1.23 ug/ml

Instrument :
FID_F
ClientSampleId :

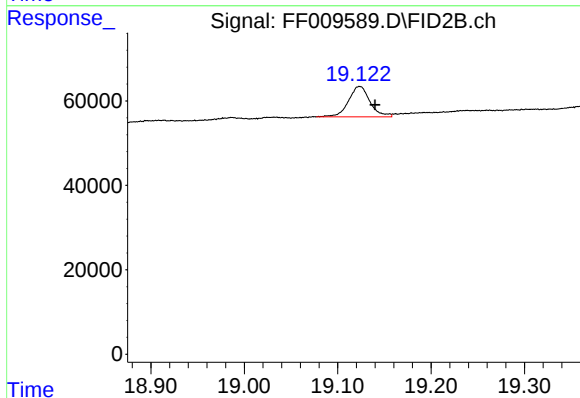


#15 N-TETRATRIACONTANE

R.T.: 19.123 min
Delta R.T.: -0.017 min
Response: 114486
Conc: 1.08 ug/ml

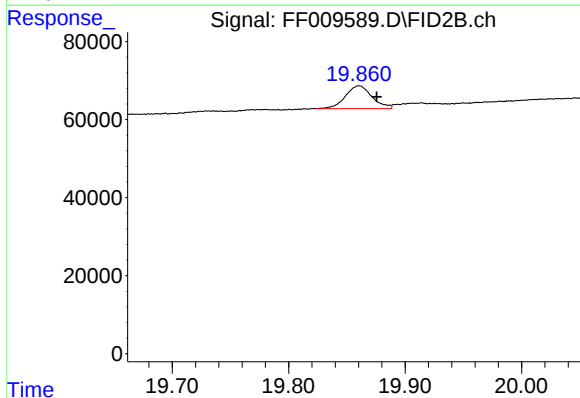


#16 N-HEXATRIACONTANE

R.T.: 19.861 min
Delta R.T.: -0.015 min
Response: 93668
Conc: 0.94 ug/ml

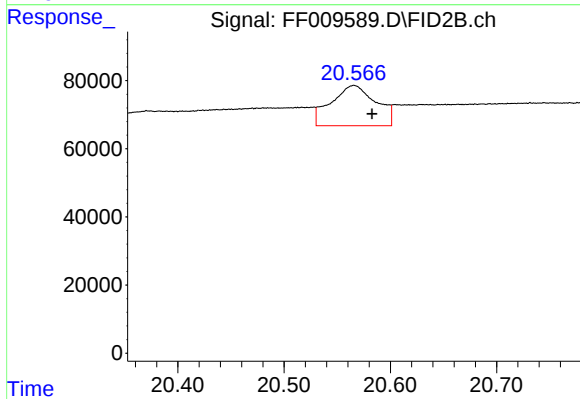

#17 N-OCTATRIACONTANE

R.T.: 20.566 min
Delta R.T.: -0.017 min
Response: 347263
Conc: 3.54 ug/ml

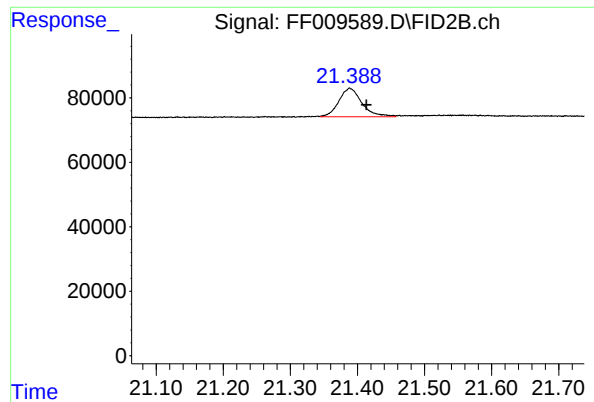

#18 N-TETRACONTANE

R.T.: 21.388 min
Delta R.T.: -0.025 min
Response: 212764
Conc: 2.11 ug/ml

Instrument :

FID_F

ClientSampleId :