

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF123019\
Data File : FF006113.D
Signal(s) : FID2B.ch
Acq On : 30 Dec 2019 11:23
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 30 15:26:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.412	2641775	15.716 ug/ml
12) N-OCTACOSANE	16.804	2398894	15.638 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF123019\
Data File : FF006113.D
Signal(s) : FID2B.ch
Acq On : 30 Dec 2019 11:23
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Dec 30 15:26:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

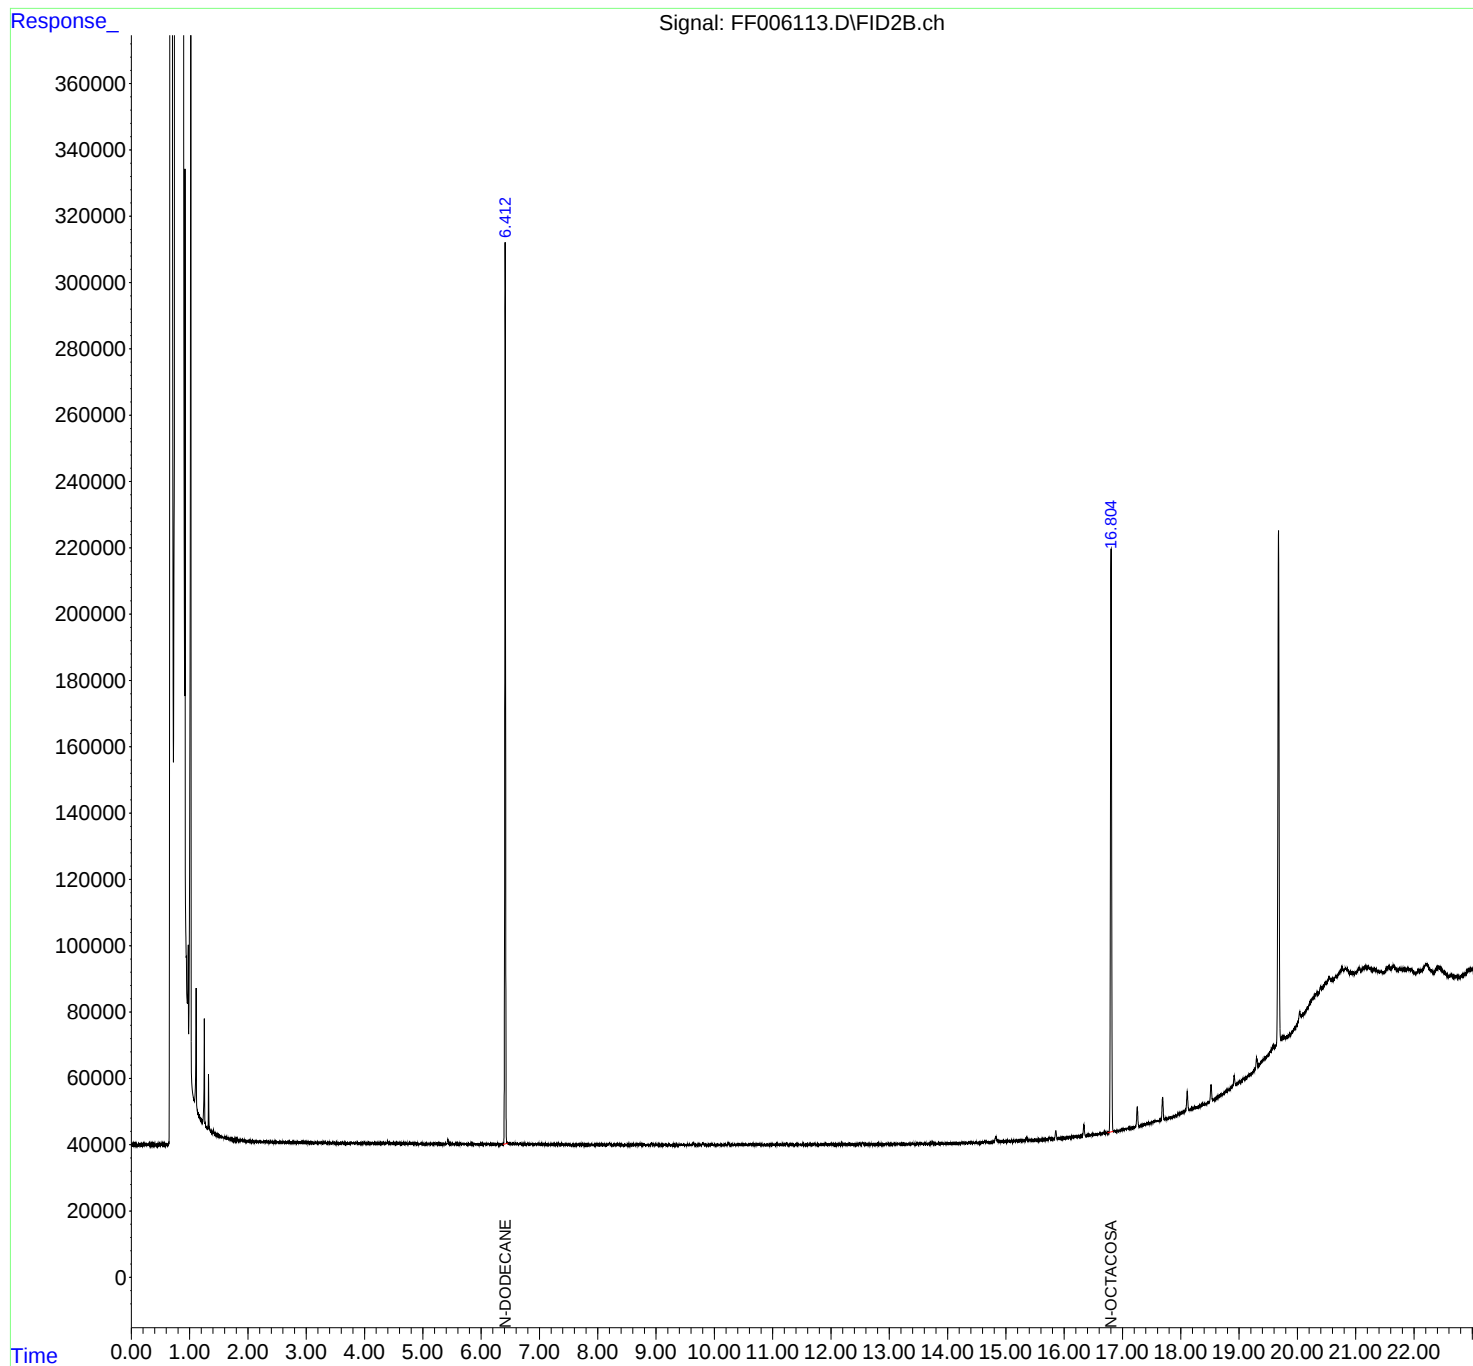


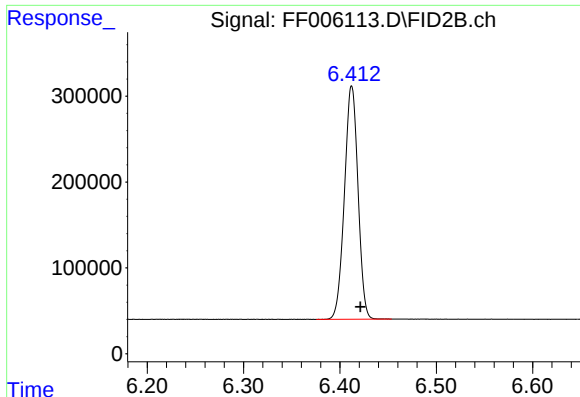

#3 N-DODECANE


R.T.: 6.412 min
Delta R.T.: -0.009 min
Response: 2641775
Conc: 15.72 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

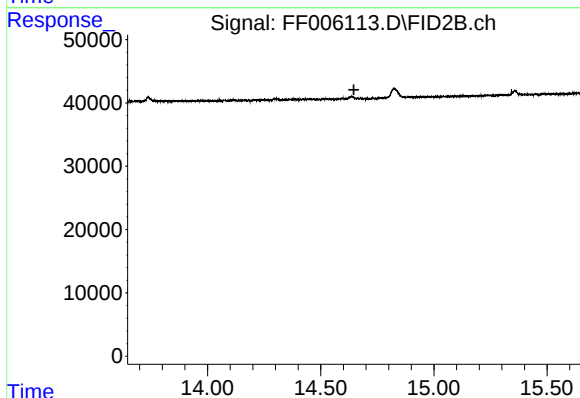

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.646 min
Response: 0
Conc: N.D.

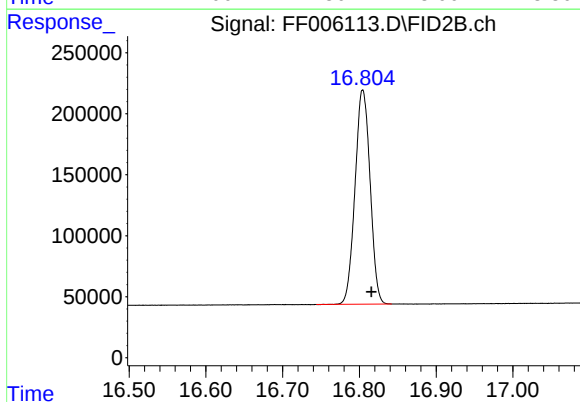

#12 N-OCTACOSANE

R.T.: 16.804 min
Delta R.T.: -0.011 min
Response: 2398894
Conc: 15.64 ug/ml