

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF123019\
Data File : FF006115.D
Signal(s) : FID2B.ch
Acq On : 30 Dec 2019 12:25
Operator : DD\AJ
Sample : K6437-07 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
GP-5-(5-6)

Integration File: autoint1.e
Quant Time: Dec 30 15:26:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	165282	1.138 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF123019\
Data File : FF006115.D
Signal(s) : FID2B.ch
Acq On : 30 Dec 2019 12:25
Operator : DD\AJ
Sample : K6437-07 10X
Misc :
ALS Vial : 56 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
GP-5-(5-6)

Integration File: autoint1.e
Quant Time: Dec 30 15:26:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF120719.M
Quant Title :
QLast Update : Fri Dec 06 13:20:24 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

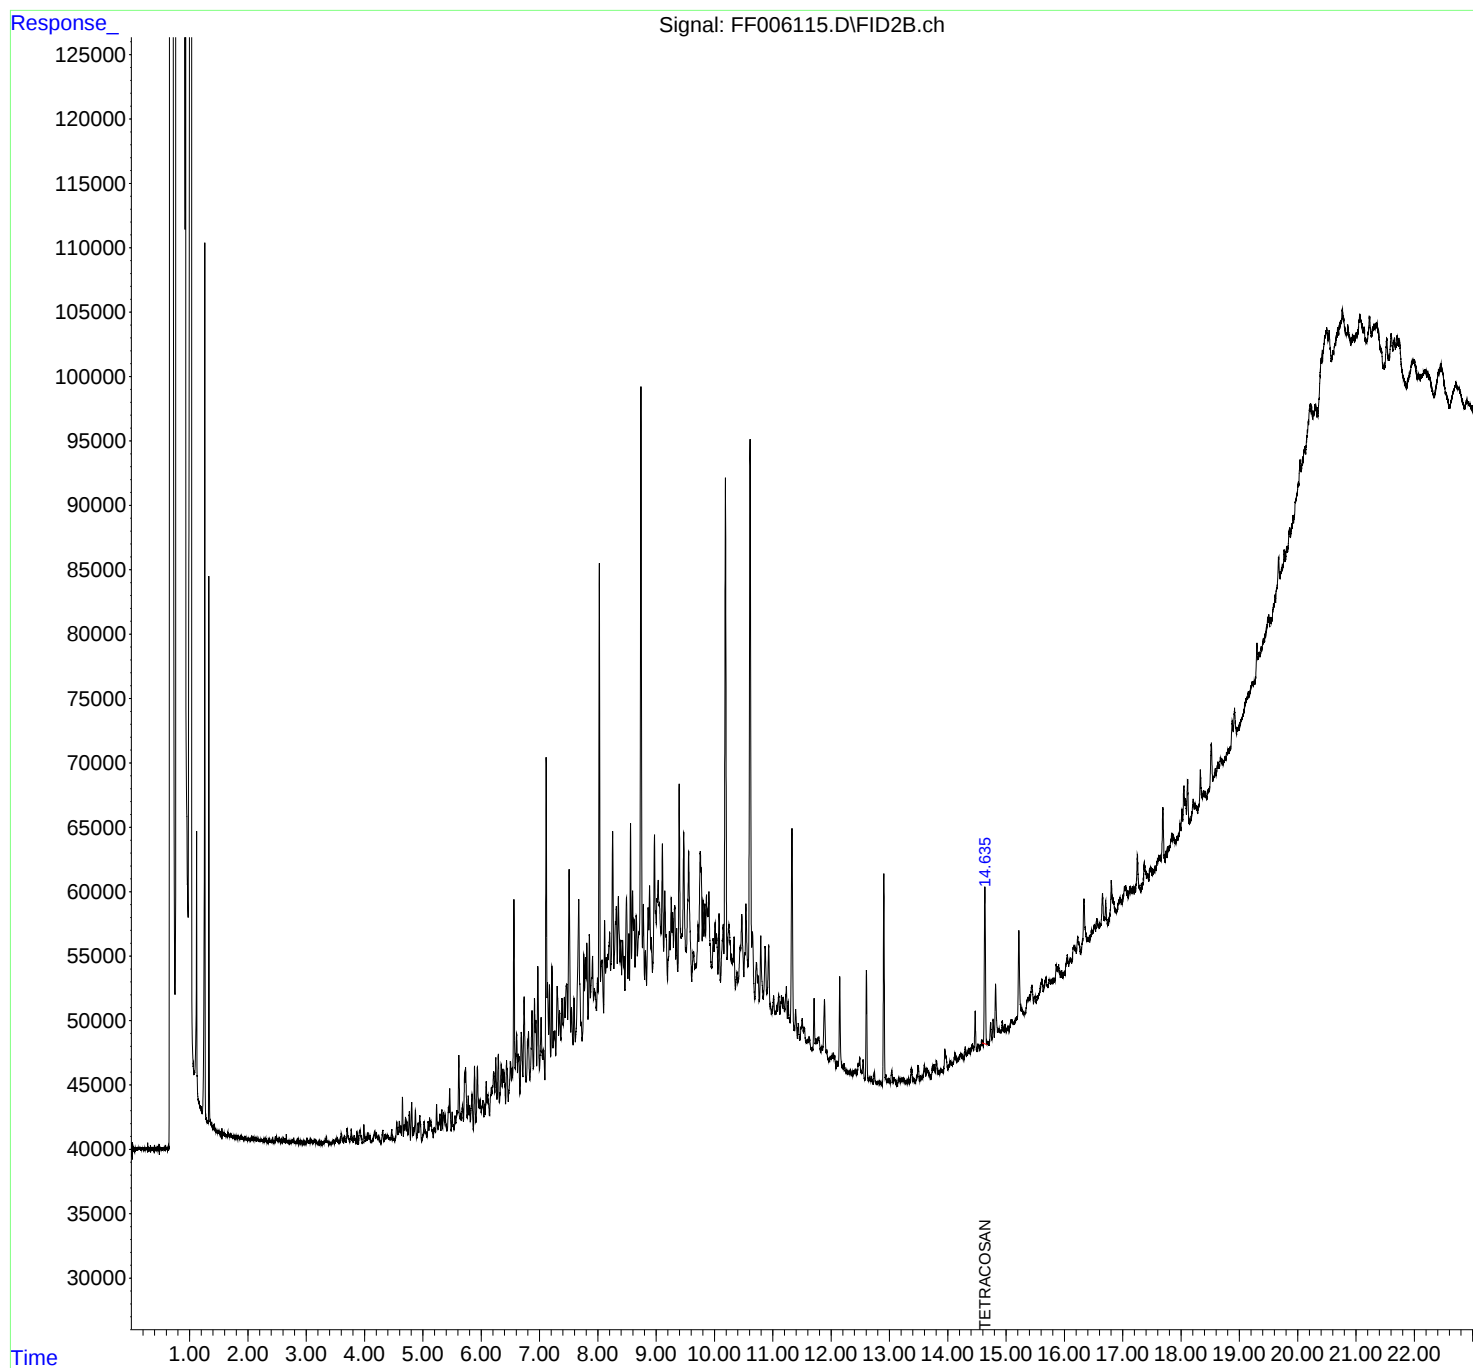

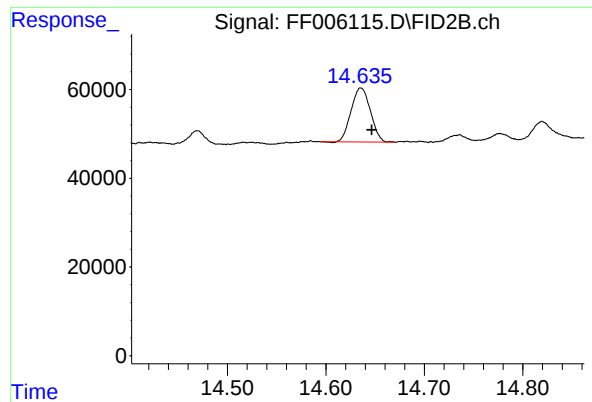

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: -0.011 min
Response: 165282
Conc: 1.14 ug/ml

Instrument :
FID_F
ClientSampleId :
GP-5-(5-6)