

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF123022\
Data File : FF011838.D
Signal(s) : FID2B.ch
Acq On : 30 Dec 2022 13:33
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 02 03:36:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) N-TRIACONTANE	18.106	59787	0.357 ug/ml
14) N-DOTRIACONTANE	18.938	109182	0.674 ug/ml
15) N-TETRATRIACONTANE	19.719	56782	0.381 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF123022\
Data File : FF011838.D
Signal(s) : FID2B.ch
Acq On : 30 Dec 2022 13:33
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jan 02 03:36:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF123022.M
Quant Title :
QLast Update : Mon Jan 02 03:26:15 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

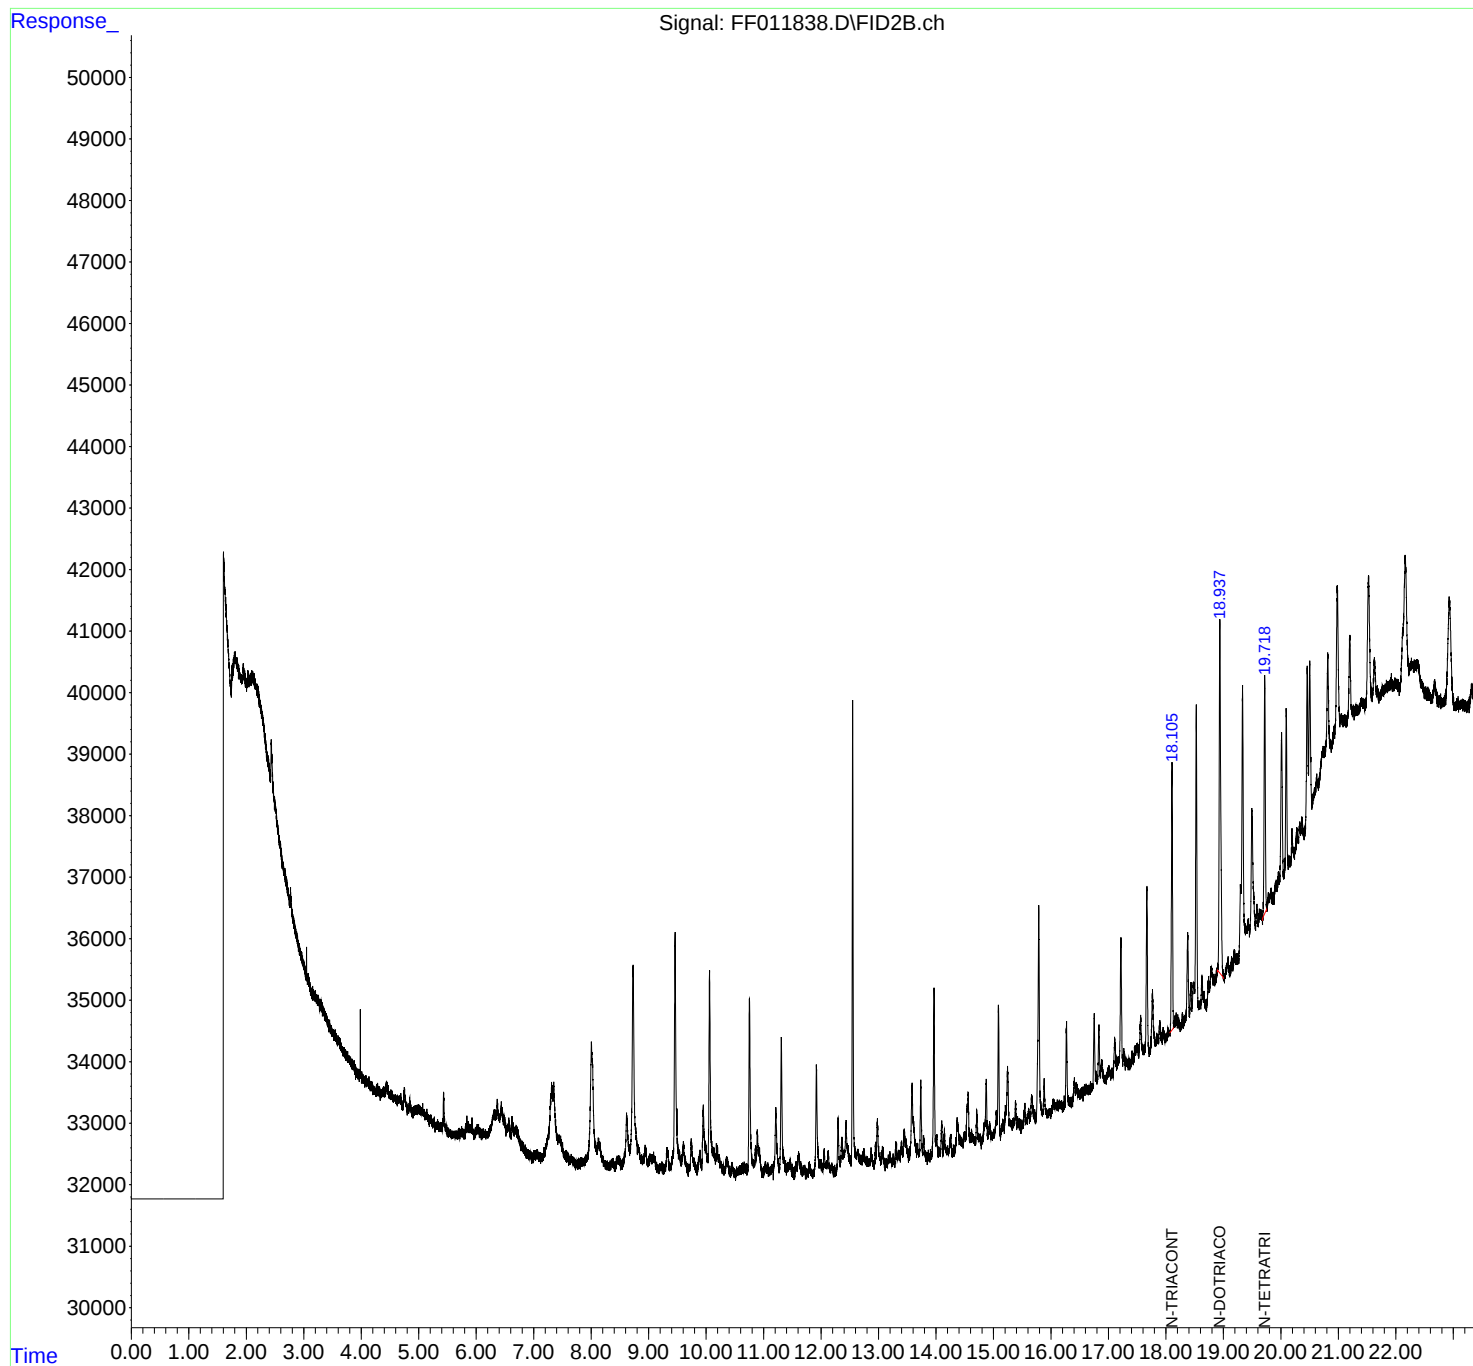


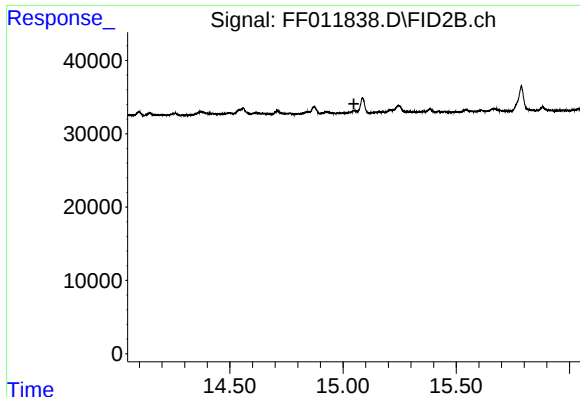

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.048 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

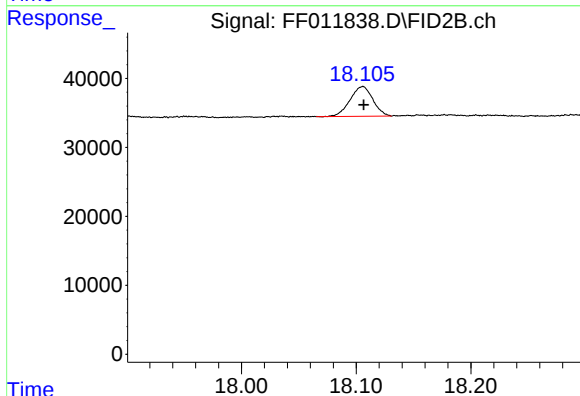


#13 N-TRIACONTANE

R.T.: 18.106 min
Delta R.T.: 0.000 min
Response: 59787
Conc: 0.36 ug/ml

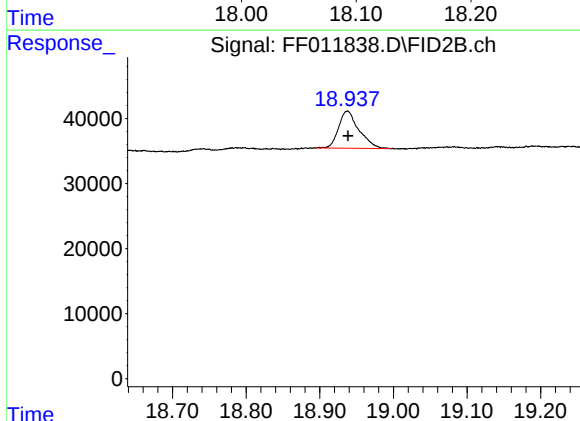

#14 N-DOTRIACONTANE

R.T.: 18.938 min
Delta R.T.: 0.000 min
Response: 109182
Conc: 0.67 ug/ml

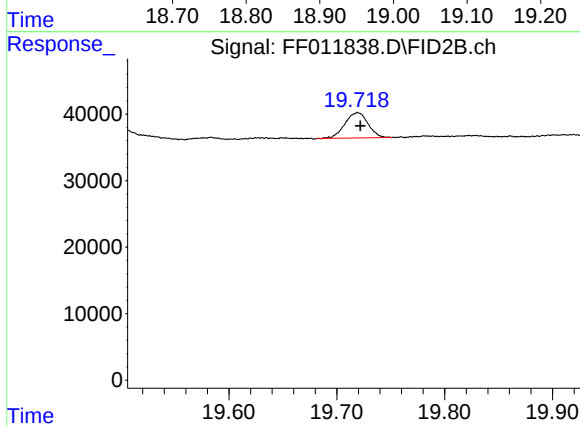

#15 N-TETRATRIACONTANE

R.T.: 19.719 min
Delta R.T.: -0.002 min
Response: 56782
Conc: 0.38 ug/ml