

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
 Data File : FF003948.D
 Signal(s) : FID2B.ch
 Acq On : 22 Mar 2019 09:42
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 22 22:56:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.579	2163327	15.538 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.648	141823	0.964 ug/ml
14) N-DOTRIACONTANE	18.484	201774	1.419 ug/ml
15) N-TETRATRIACONTANE	19.268	102737	0.767 ug/ml
16) N-HEXATRIACONTANE	20.050	363033	2.782 ug/ml
18) N-TETRACONTANE	21.647	298476	2.399 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
Data File : FF003948.D
Signal(s) : FID2B.ch
Acq On : 22 Mar 2019 09:42
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 22 22:56:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

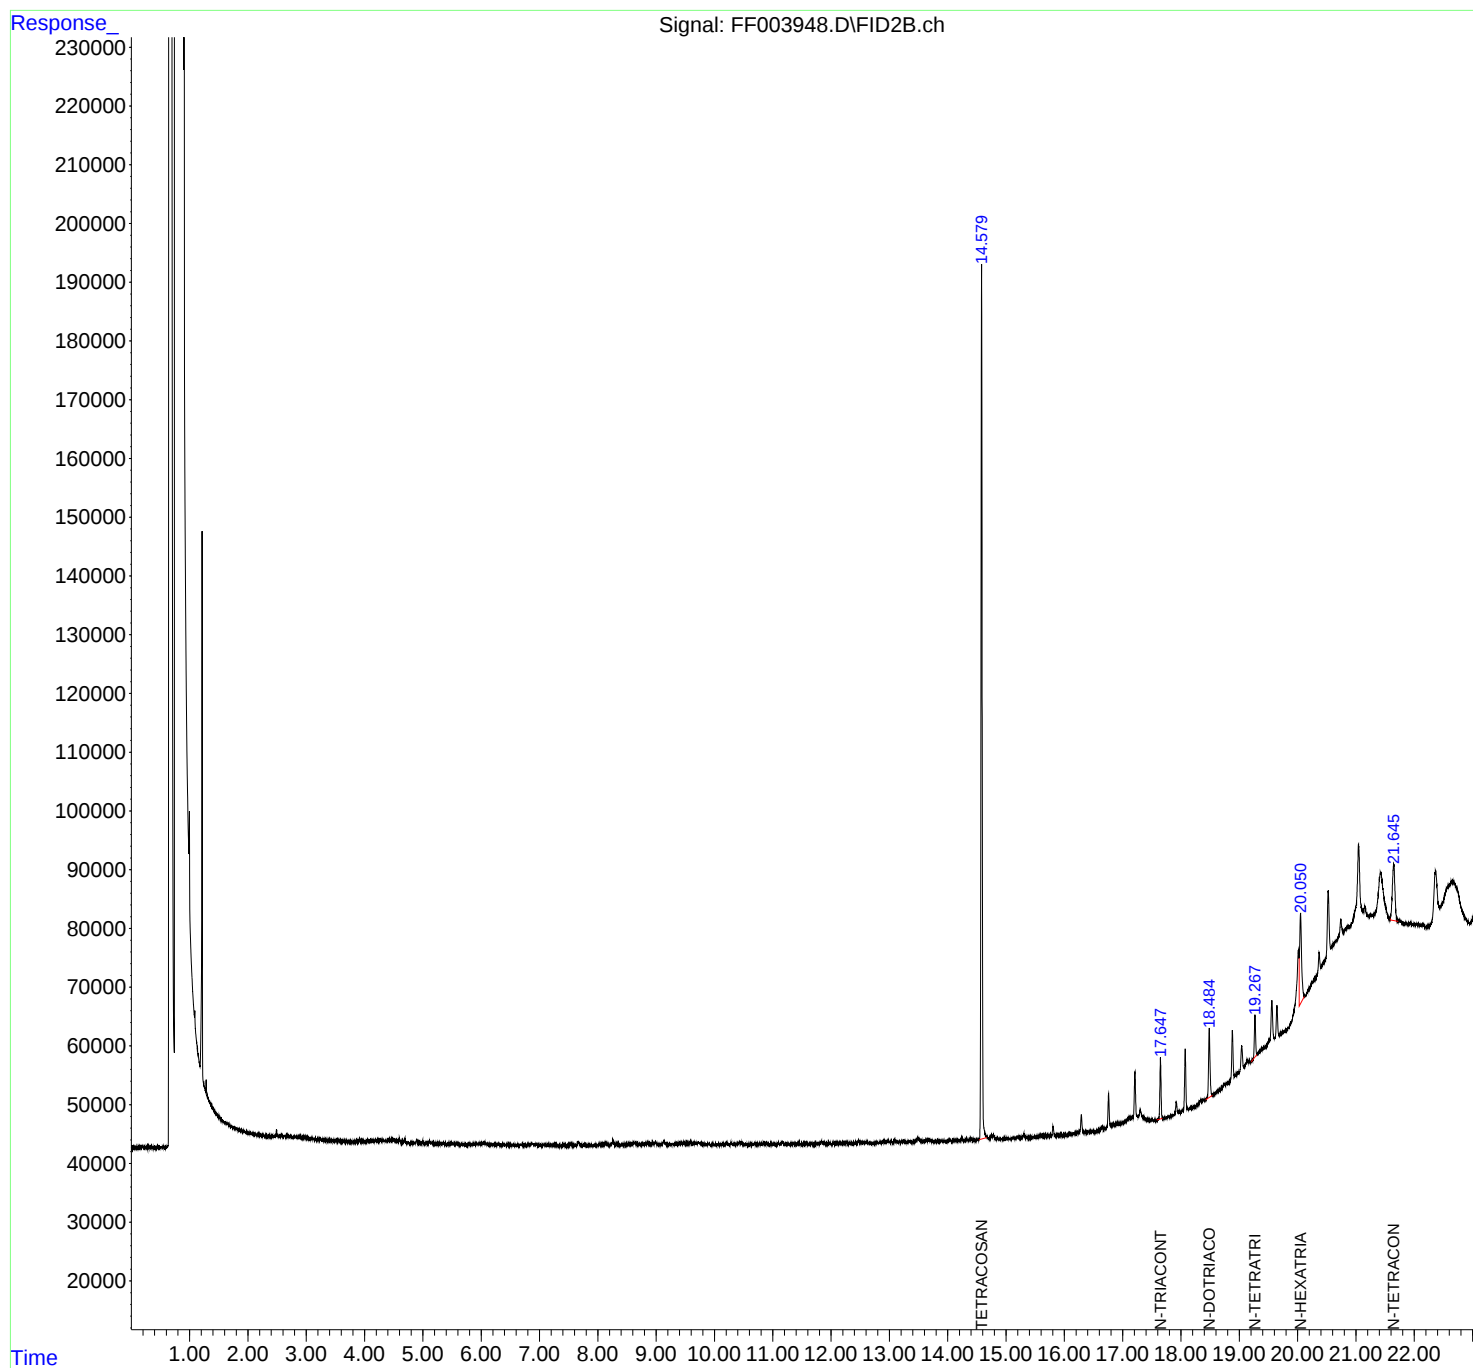


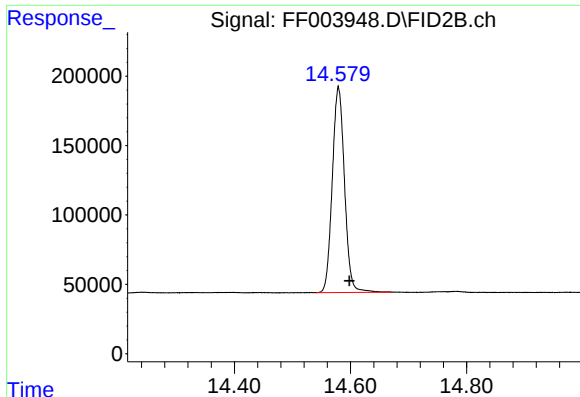

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.579 min
Delta R.T.: -0.019 min
Response: 2163327
Conc: 15.54 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

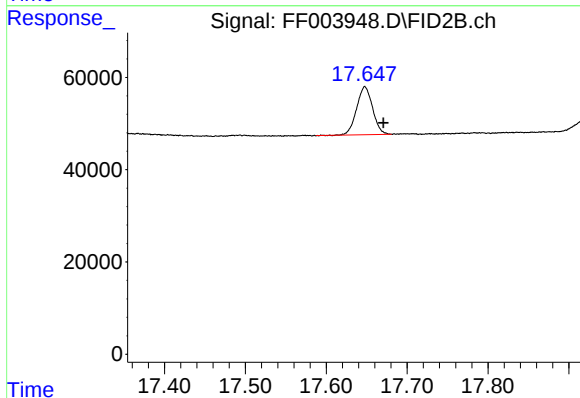


#13 N-TRIACONTANE

R.T.: 17.648 min
Delta R.T.: -0.023 min
Response: 141823
Conc: 0.96 ug/ml

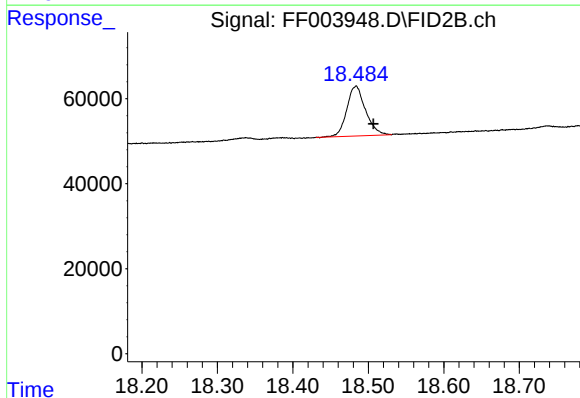


#14 N-DOTRIACONTANE

R.T.: 18.484 min
Delta R.T.: -0.023 min
Response: 201774
Conc: 1.42 ug/ml

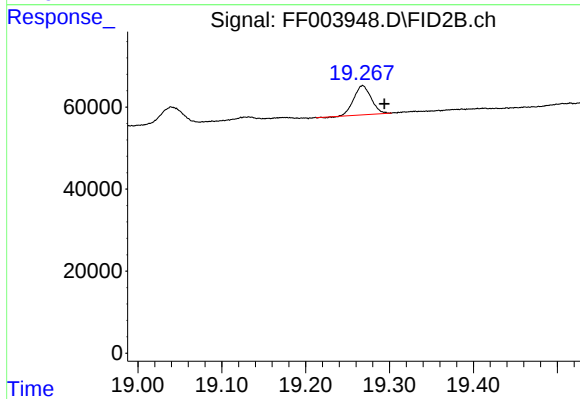

#15 N-TETRATRIACONTANE


R.T.: 19.268 min
Delta R.T.: -0.026 min
Response: 102737
Conc: 0.77 ug/ml

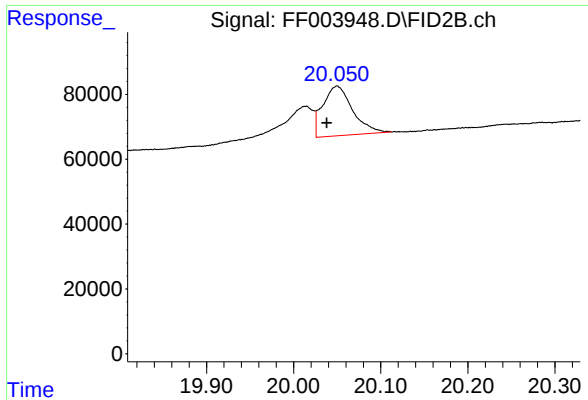

#16 N-HEXATRIACONTANE

R.T.: 20.050 min
Delta R.T.: 0.012 min
Response: 363033
Conc: 2.78 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

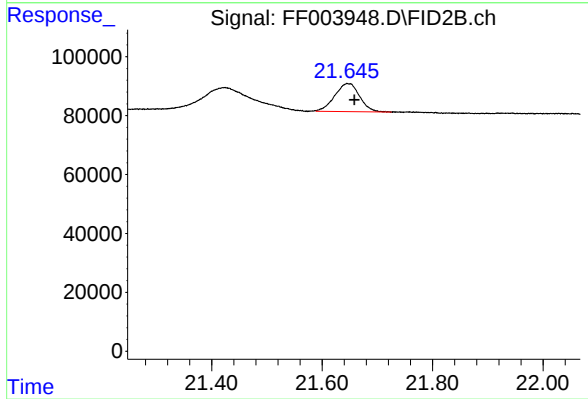

#18 N-TETRACONTANE

R.T.: 21.647 min
Delta R.T.: -0.012 min
Response: 298476
Conc: 2.40 ug/ml