

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
Data File : FF003950.D
Signal(s) : FID2B.ch
Acq On : 22 Mar 2019 10:47
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 22 22:57:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.329	3354053	21.492 ug/ml
12) N-OCTACOSANE	16.758	3218102	21.296 ug/ml
13) N-TRIACONTANE	17.647	429406	2.919 ug/ml
14) N-DOTRIACONTANE	18.482	485849	3.416 ug/ml
15) N-TETRATRIACONTANE	19.269	322159	2.406 ug/ml
16) N-HEXATRIACONTANE	20.053	259457	1.988 ug/ml
17) N-OCTATRIACONTANE	20.743	124662	1.080 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
Data File : FF003950.D
Signal(s) : FID2B.ch
Acq On : 22 Mar 2019 10:47
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 22 22:57:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

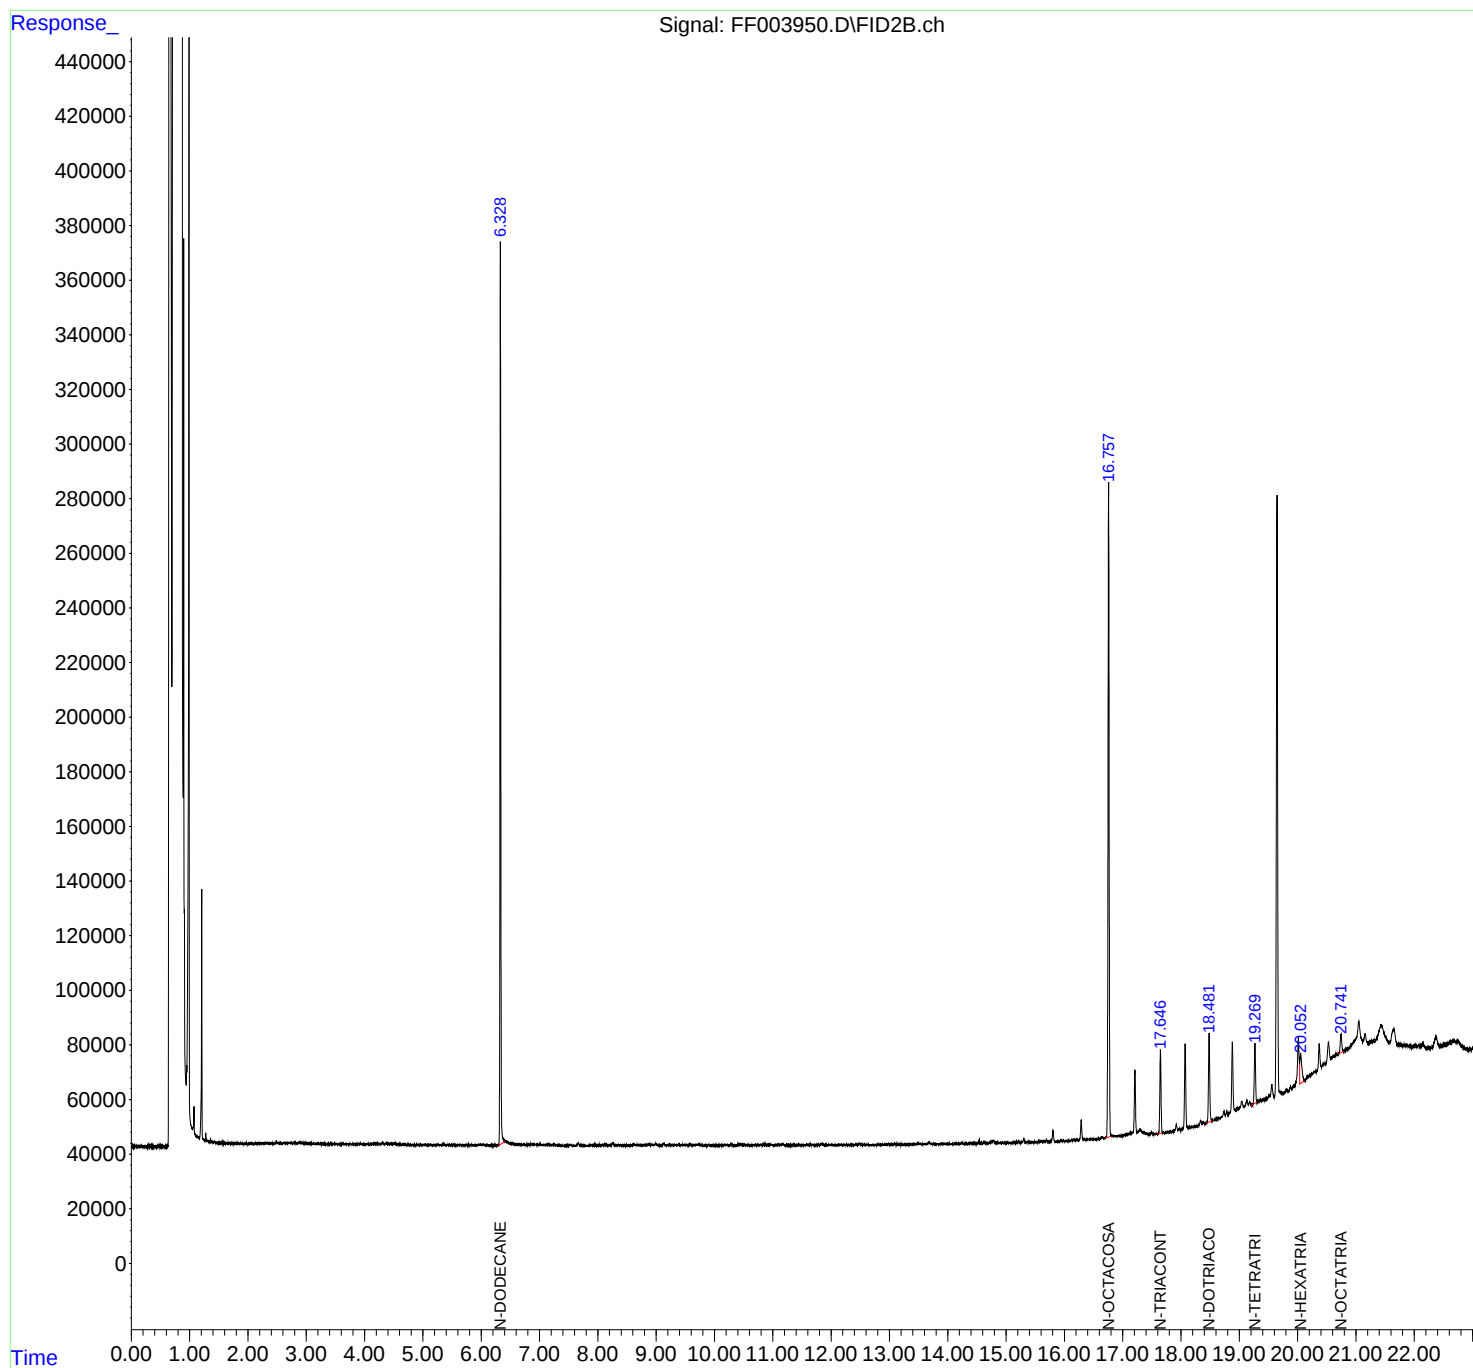


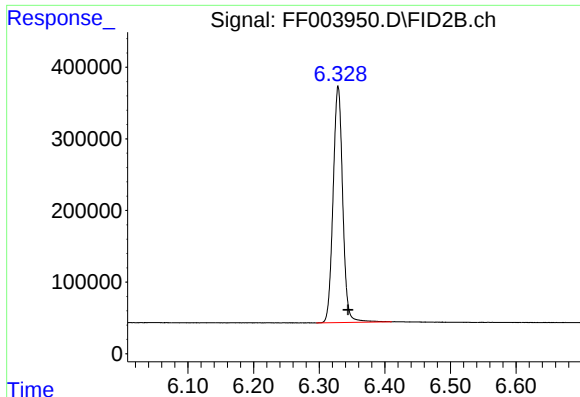

#3 N-DODECANE


R.T.: 6.329 min
Delta R.T.: -0.015 min
Response: 3354053
Conc: 21.49 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

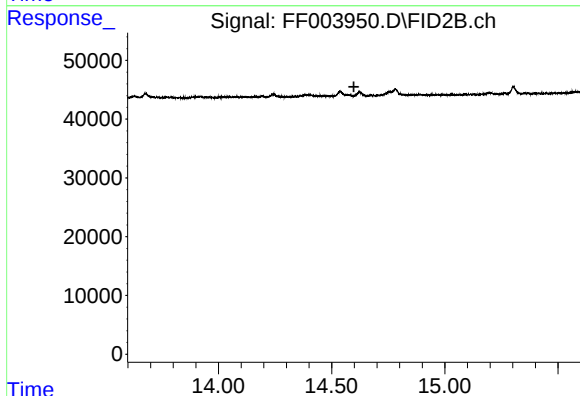


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

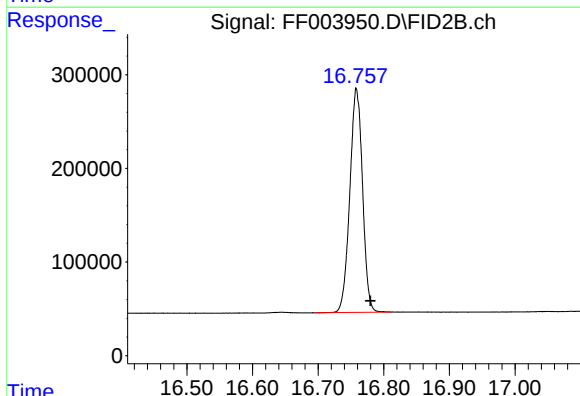


#12 N-OCTACOSANE

R.T.: 16.758 min
Delta R.T.: -0.021 min
Response: 3218102
Conc: 21.30 ug/ml

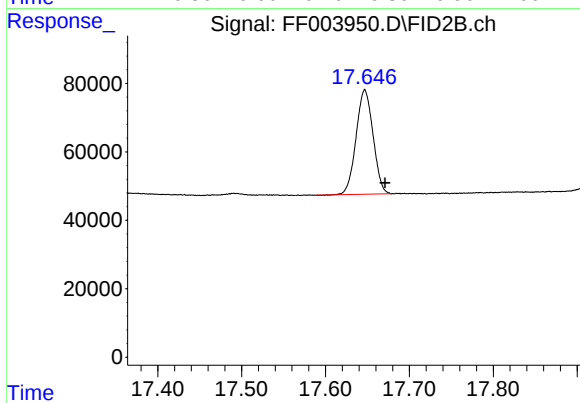

#13 N-TRIACONTANE


R.T.: 17.647 min
Delta R.T.: -0.024 min
Response: 429406
Conc: 2.92 ug/ml

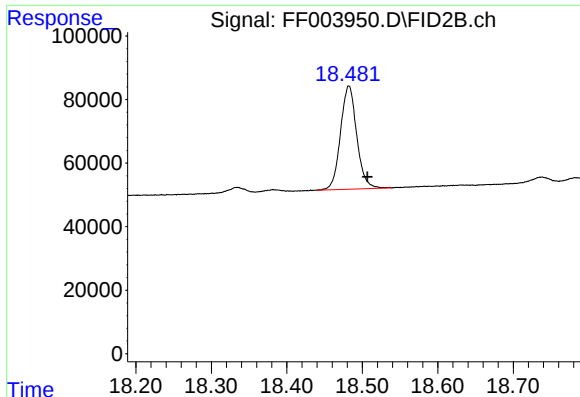

#14 N-DOTRIACONTANE


R.T.: 18.482 min
Delta R.T.: -0.024 min
Response: 485849
Conc: 3.42 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

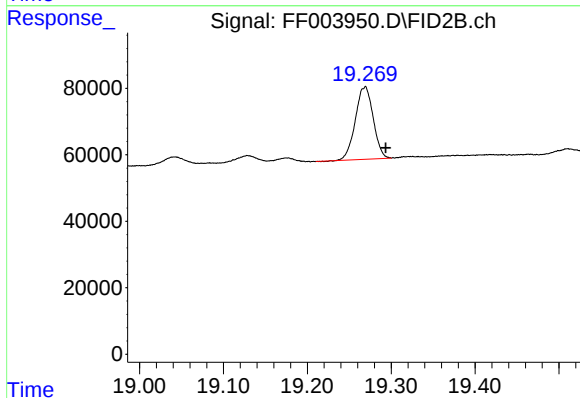


#15 N-TETRATRIACONTANE

R.T.: 19.269 min
Delta R.T.: -0.025 min
Response: 322159
Conc: 2.41 ug/ml

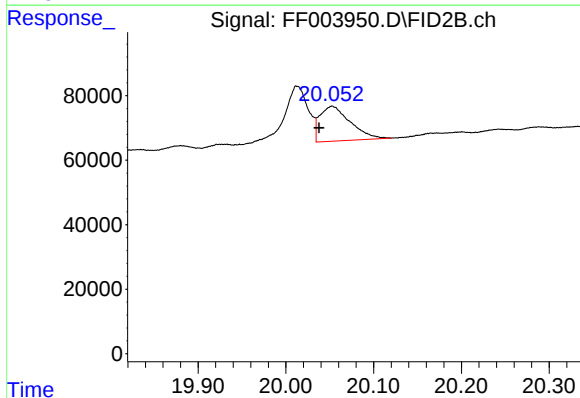

#16 N-HEXATRIACONTANE

R.T.: 20.053 min
Delta R.T.: 0.015 min
Response: 259457
Conc: 1.99 ug/ml

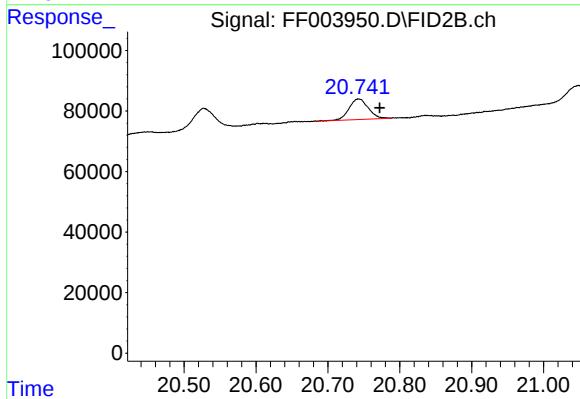

#17 N-OCTATRIACONTANE

R.T.: 20.743 min
Delta R.T.: -0.030 min
Response: 124662
Conc: 1.08 ug/ml