

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
 Data File : FF003952.D
 Signal(s) : FID2B.ch
 Acq On : 22 Mar 2019 11:48
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 22 22:57:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.579	2214889	15.908 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.758	93515	0.619 ug/ml
13) N-TRIACONTANE	17.646	175453	1.193 ug/ml
14) N-DOTRIACONTANE	18.483	218718	1.538 ug/ml
15) N-TETRATRIACONTANE	19.269	123765	0.924 ug/ml
16) N-HEXATRIACONTANE	20.050	425442	3.261 ug/ml
18) N-TETRACONTANE	21.649	277045	2.227 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
Data File : FF003952.D
Signal(s) : FID2B.ch
Acq On : 22 Mar 2019 11:48
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 22 22:57:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

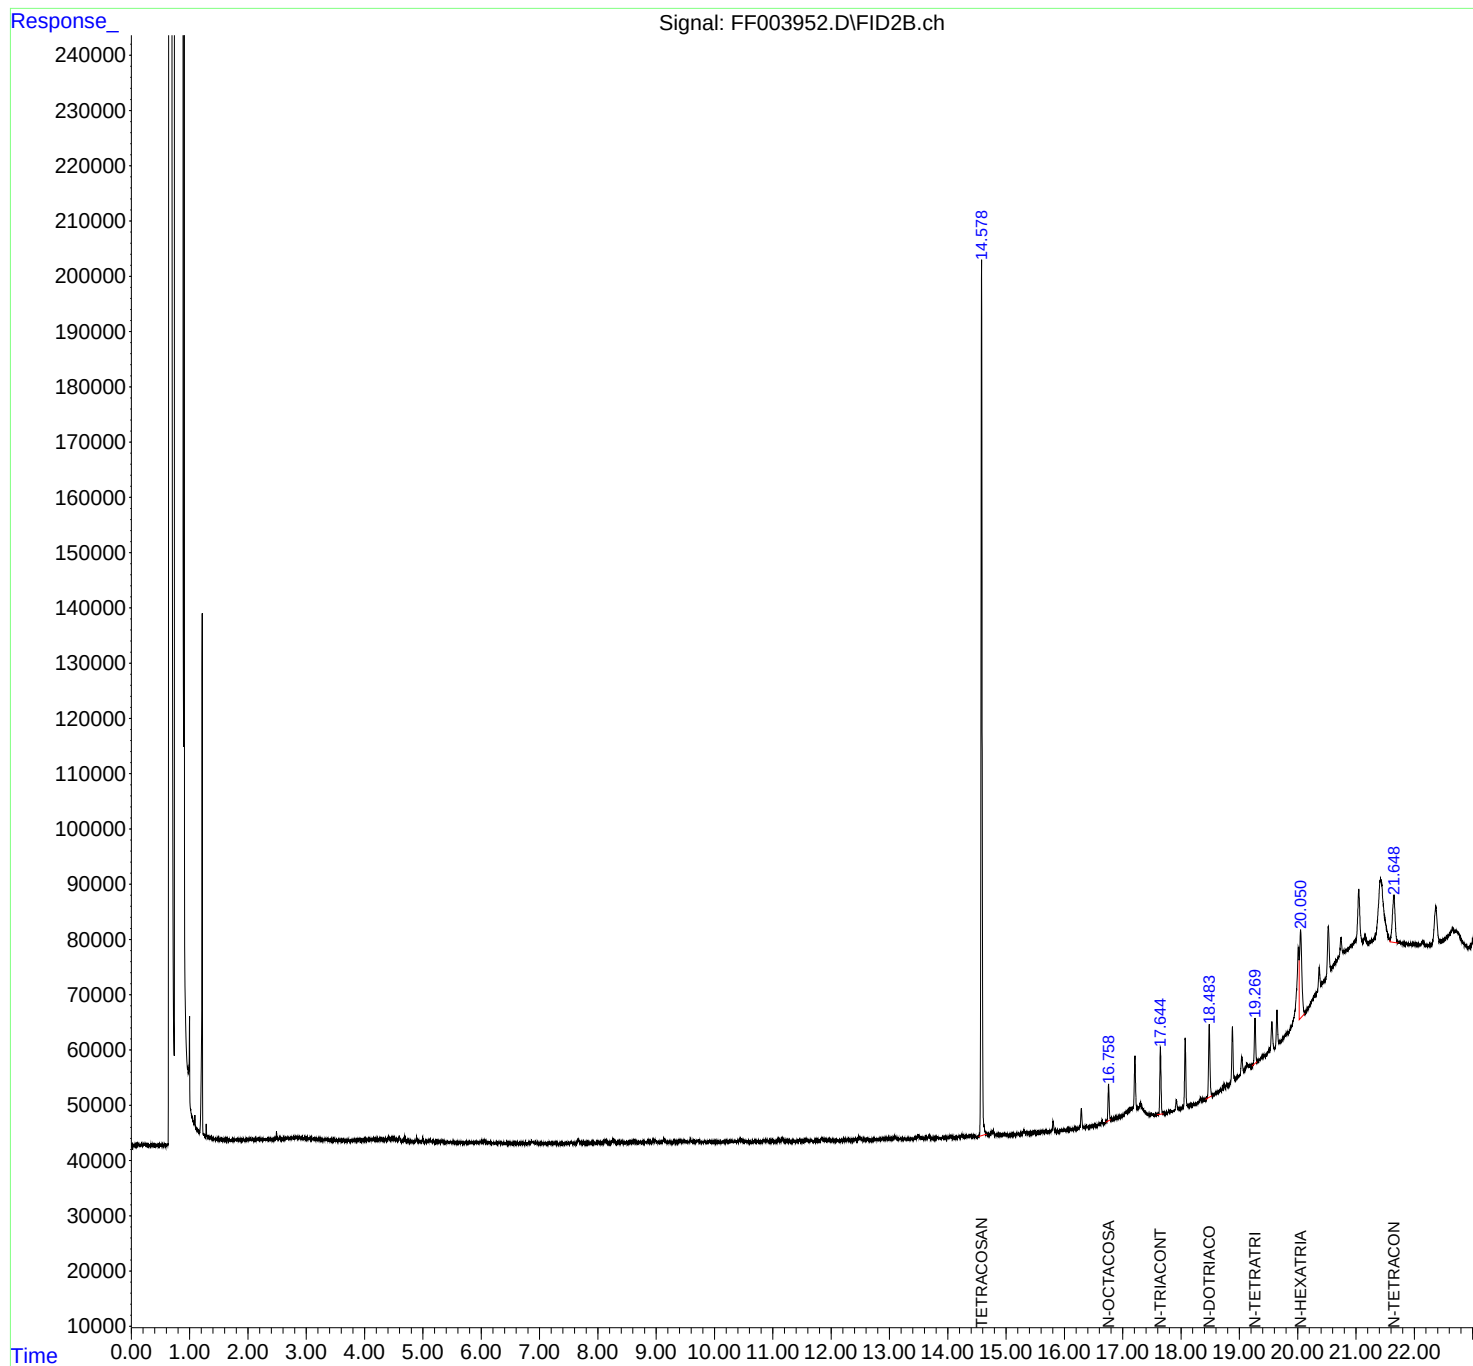


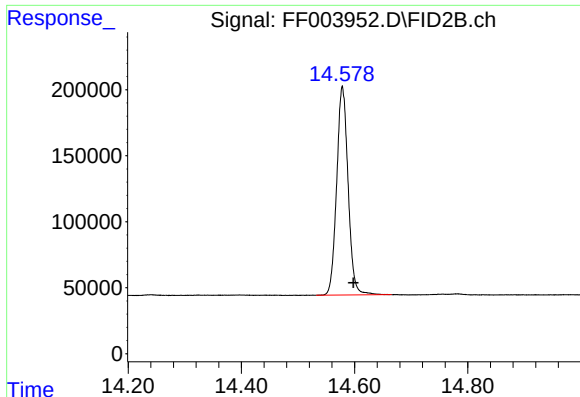

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.579 min
Delta R.T.: -0.020 min
Response: 2214889
Conc: 15.91 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

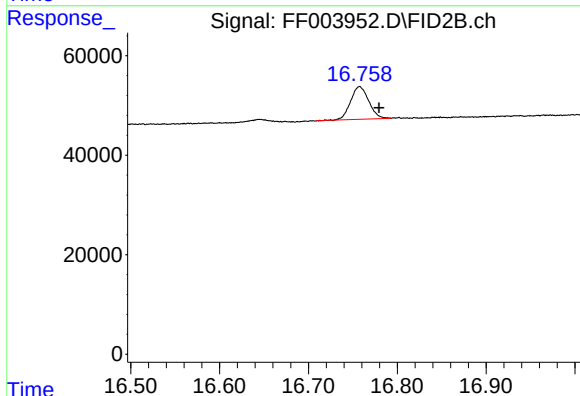


#12 N-OCTACOSANE

R.T.: 16.758 min
Delta R.T.: -0.022 min
Response: 93515
Conc: 0.62 ug/ml

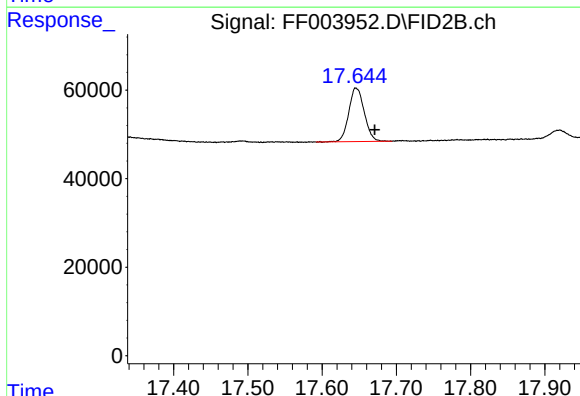


#13 N-TRIACONTANE

R.T.: 17.646 min
Delta R.T.: -0.025 min
Response: 175453
Conc: 1.19 ug/ml

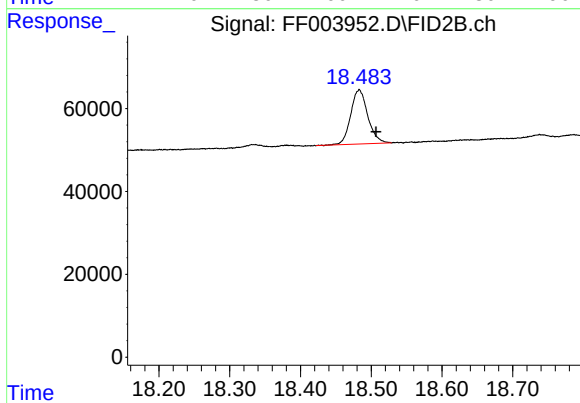

#14 N-DOTRIACONTANE


R.T.: 18.483 min
Delta R.T.: -0.024 min
Response: 218718
Conc: 1.54 ug/ml

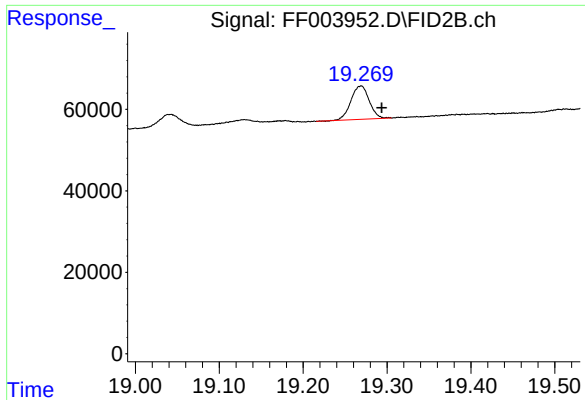

#15 N-TETRATRIACONTANE


R.T.: 19.269 min
Delta R.T.: -0.025 min
Response: 123765
Conc: 0.92 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

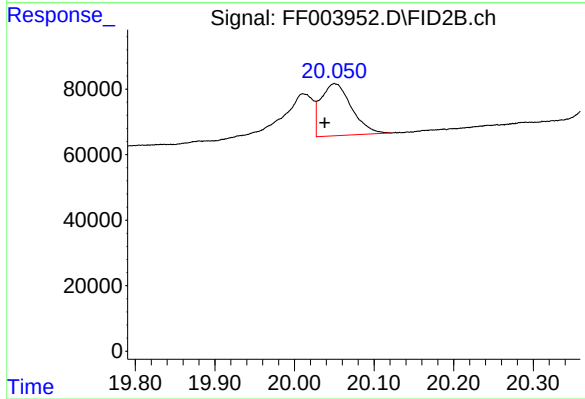

#16 N-HEXATRIACONTANE

R.T.: 20.050 min
Delta R.T.: 0.012 min
Response: 425442
Conc: 3.26 ug/ml

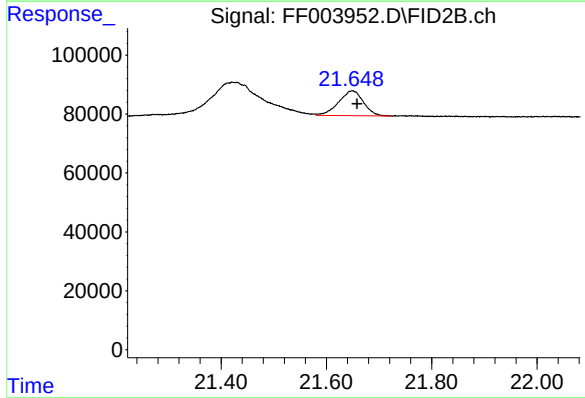

#18 N-TETRACONTANE

R.T.: 21.649 min
Delta R.T.: -0.010 min
Response: 277045
Conc: 2.23 ug/ml