

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
 Data File : FF003954.D
 Signal(s) : FID2B.ch
 Acq On : 22 Mar 2019 12:49
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 I.BLK

Integration File: autoint1.e
 Quant Time: Mar 22 22:58:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.578	2289432	16.444 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.757	87009	0.576 ug/ml
13) N-TRIACONTANE	17.647	168123	1.143 ug/ml
14) N-DOTRIACONTANE	18.482	209149	1.471 ug/ml
15) N-TETRATRIACONTANE	19.268	126998	0.948 ug/ml
16) N-HEXATRIACONTANE	20.056	878841	6.735 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
Data File : FF003954.D
Signal(s) : FID2B.ch
Acq On : 22 Mar 2019 12:49
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 22 22:58:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

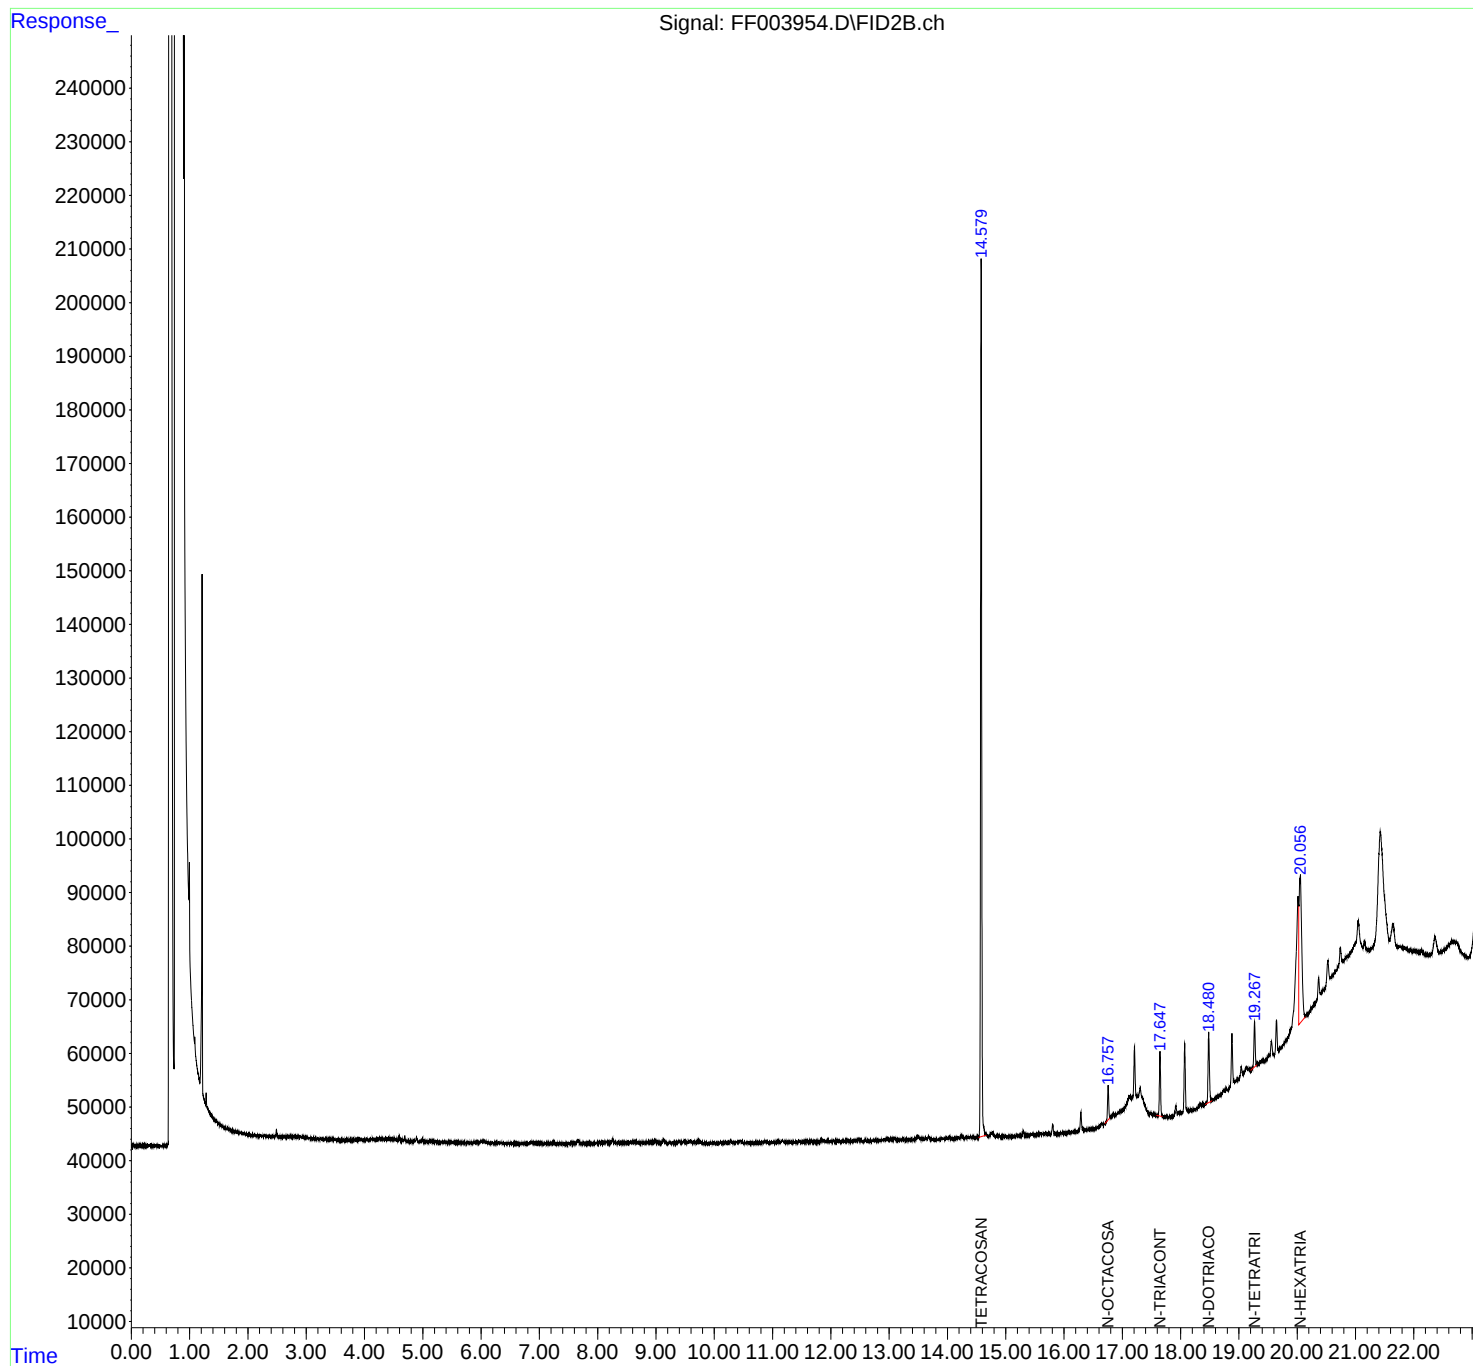


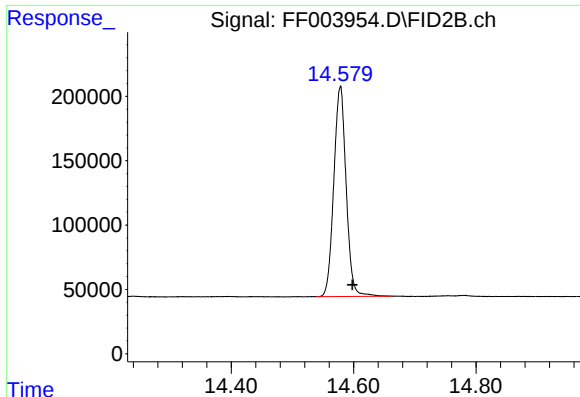

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.578 min
Delta R.T.: -0.020 min
Response: 2289432
Conc: 16.44 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

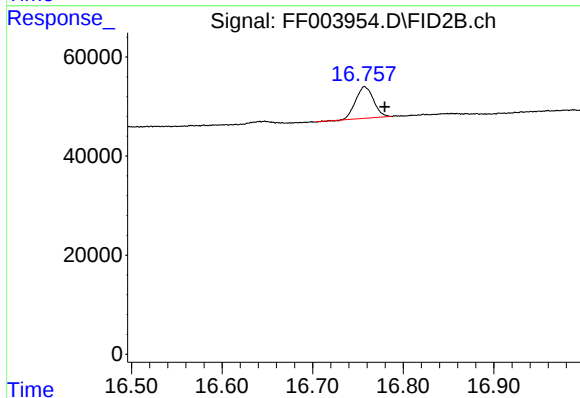


#12 N-OCTACOSANE

R.T.: 16.757 min
Delta R.T.: -0.022 min
Response: 87009
Conc: 0.58 ug/ml

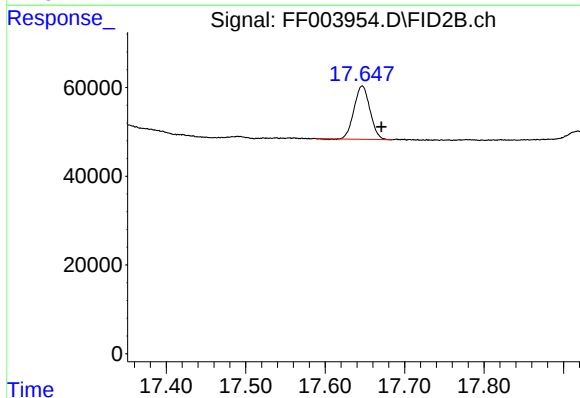


#13 N-TRIACONTANE

R.T.: 17.647 min
Delta R.T.: -0.024 min
Response: 168123
Conc: 1.14 ug/ml

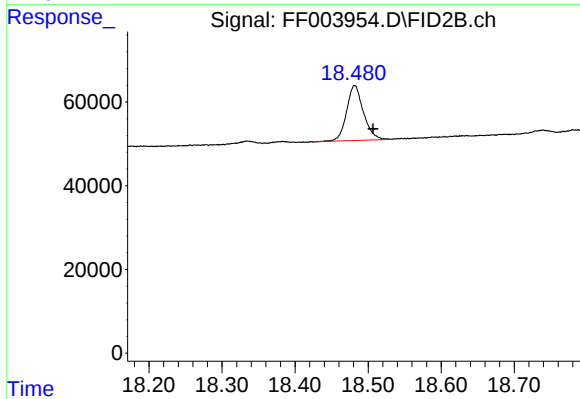

#14 N-DOTRIACONTANE


R.T.: 18.482 min
Delta R.T.: -0.025 min
Response: 209149
Conc: 1.47 ug/ml

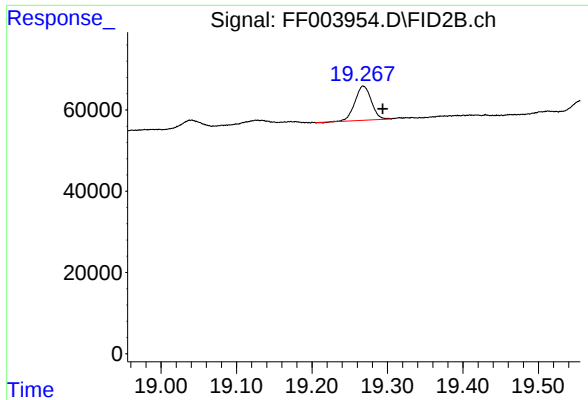

#15 N-TETRATRIACONTANE

R.T.: 19.268 min
Delta R.T.: -0.026 min
Response: 126998
Conc: 0.95 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

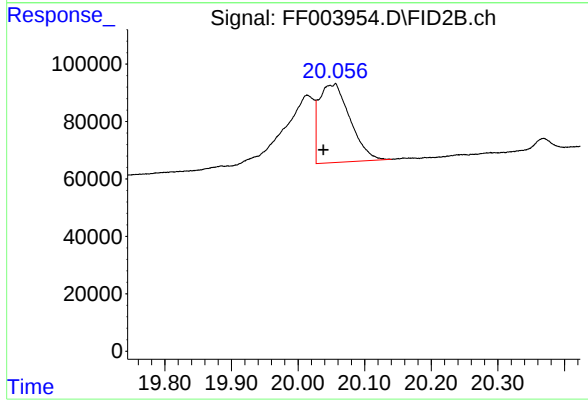

#16 N-HEXATRIACONTANE

R.T.: 20.056 min
Delta R.T.: 0.018 min
Response: 878841
Conc: 6.74 ug/ml