

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
 Data File : FF003956.D
 Signal(s) : FID2B.ch
 Acq On : 22 Mar 2019 13:50
 Operator : AJ\SJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 RT MARKER

Integration File: autoint1.e
 Quant Time: Mar 22 22:59:02 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.329	3251426	20.834 ug/ml
12) N-OCTACOSANE	16.760	3224778	21.340 ug/ml
13) N-TRIACONTANE	17.647	489190	3.326 ug/ml
14) N-DOTRIACONTANE	18.481	611056	4.297 ug/ml
15) N-TETRATRIACONTANE	19.268	369329	2.758 ug/ml
16) N-HEXATRIACONTANE	20.051	489694	3.753 ug/ml
17) N-OCTATRIACONTANE	20.741	144642	1.253 ug/ml
18) N-TETRACONTANE	21.648	628210	5.050 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
Data File : FF003956.D
Signal(s) : FID2B.ch
Acq On : 22 Mar 2019 13:50
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 22 22:59:02 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

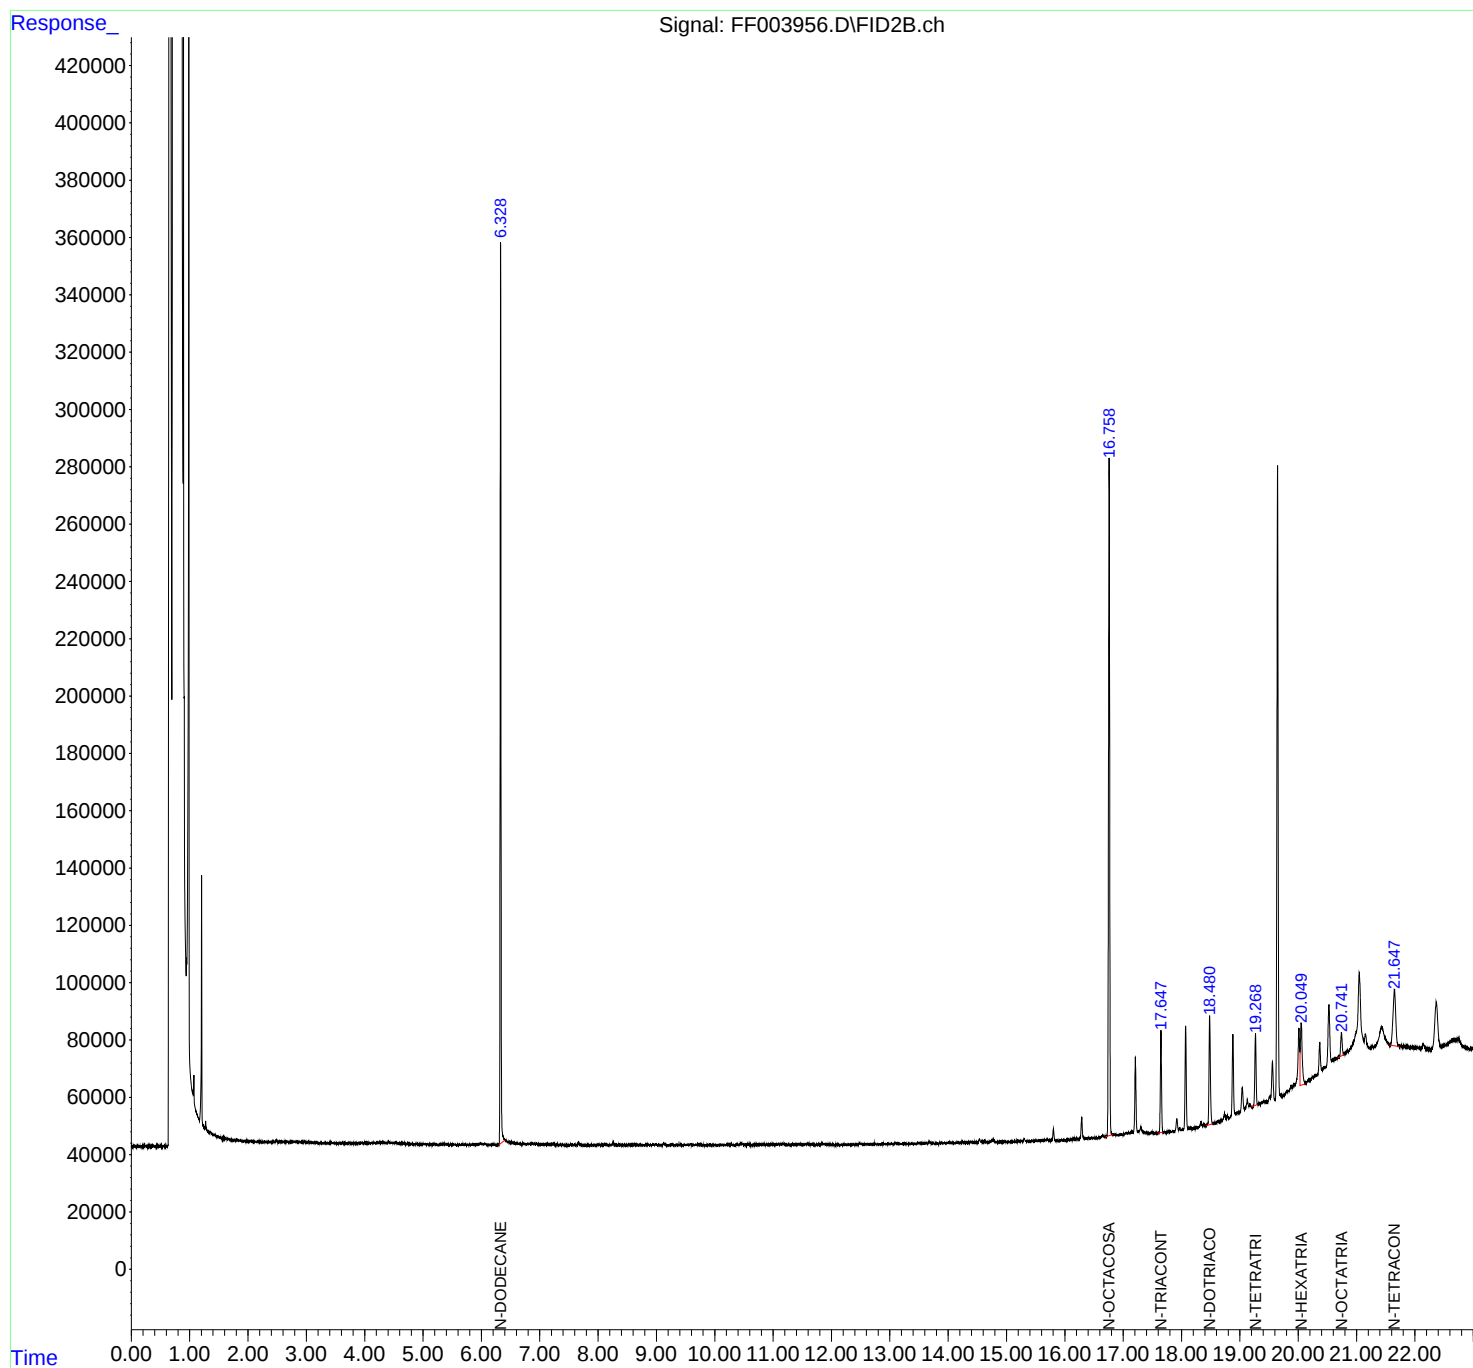


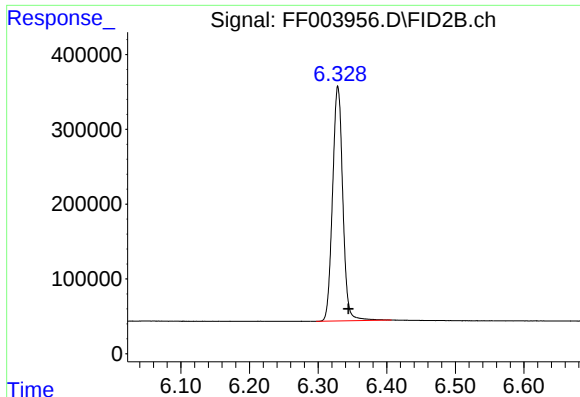

#3 N-DODECANE


R.T.: 6.329 min
Delta R.T.: -0.015 min
Response: 3251426
Conc: 20.83 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

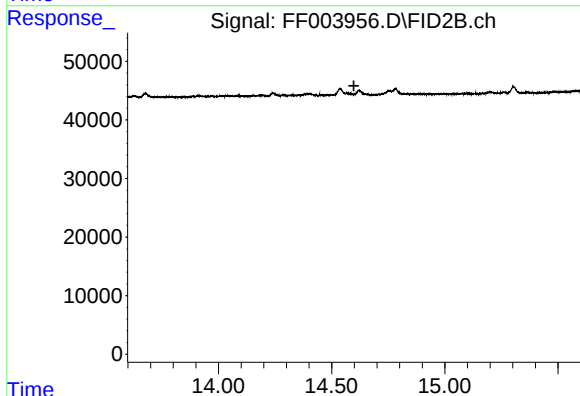


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

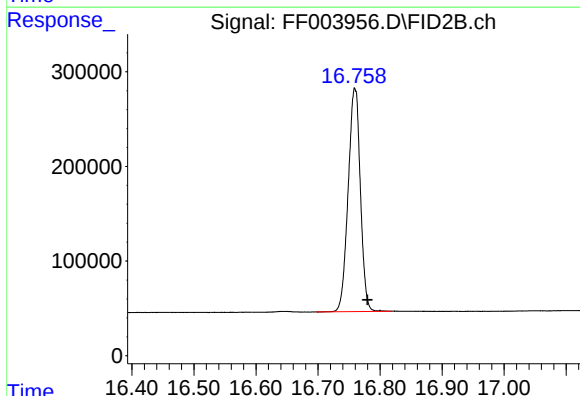


#12 N-OCTACOSANE

R.T.: 16.760 min
Delta R.T.: -0.020 min
Response: 3224778
Conc: 21.34 ug/ml

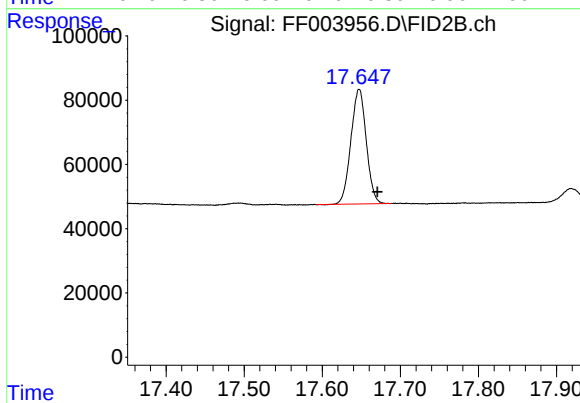

#13 N-TRIACONTANE


R.T.: 17.647 min
Delta R.T.: -0.024 min
Response: 489190
Conc: 3.33 ug/ml

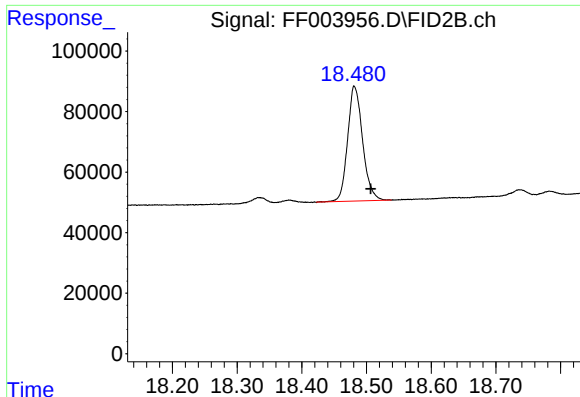

#14 N-DOTRIACONTANE


R.T.: 18.481 min
Delta R.T.: -0.026 min
Response: 611056
Conc: 4.30 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

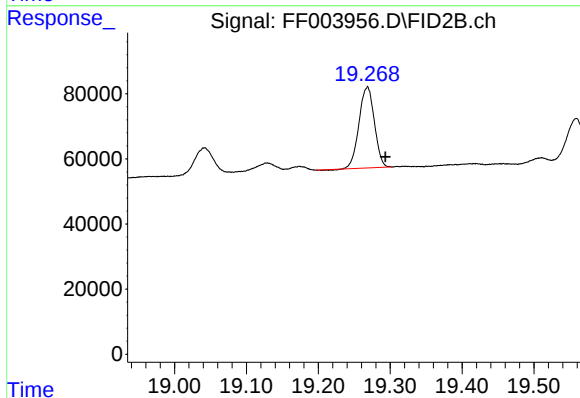


#15 N-TETRATRIACONTANE

R.T.: 19.268 min
Delta R.T.: -0.025 min
Response: 369329
Conc: 2.76 ug/ml

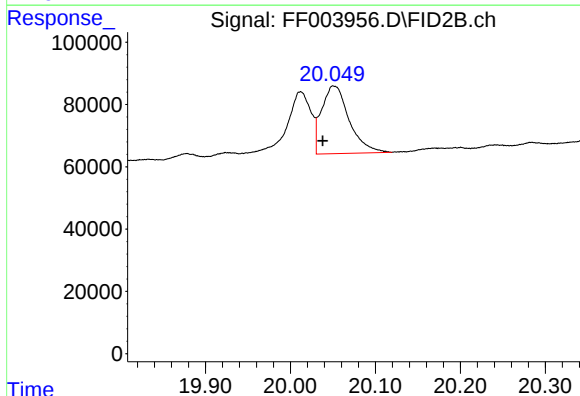


#16 N-HEXATRIACONTANE

R.T.: 20.051 min
Delta R.T.: 0.013 min
Response: 489694
Conc: 3.75 ug/ml

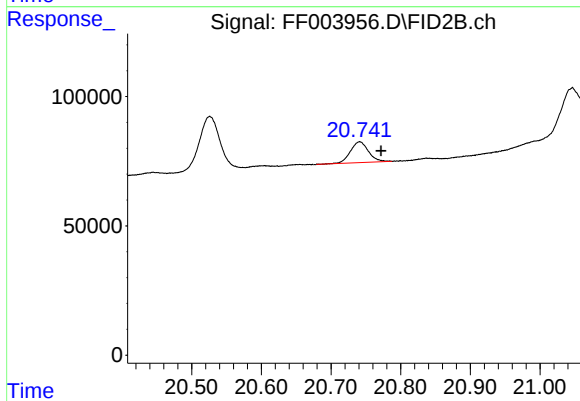

#17 N-OCTATRIACONTANE

R.T.: 20.741 min
Delta R.T.: -0.031 min
Response: 144642
Conc: 1.25 ug/ml

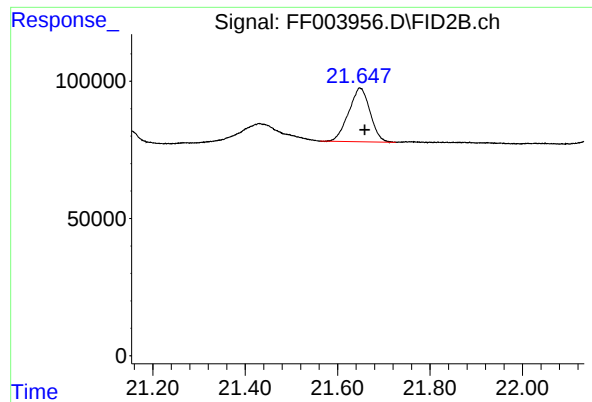

#18 N-TETRACONTANE

R.T.: 21.648 min
Delta R.T.: -0.011 min
Response: 628210
Conc: 5.05 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER