

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
 Data File : FF003959.D
 Signal(s) : FID2B.ch
 Acq On : 22 Mar 2019 15:22
 Operator : AJ\SJ
 Sample : K2050-03
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CS-3

Integration File: autoint1.e
 Quant Time: Mar 22 22:59:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.579	2736698	19.656 ug/ml
Target Compounds			
4) N-TETRADECANE	8.179	502798	3.136 ug/ml
7) N-EICOSANE	12.531	2923885	17.873 ug/ml
8) N-DOCOSANE	13.698	348662	2.160 ug/ml
10) N-TETRACOSANE	14.758	2998154	18.949 ug/ml
11) N-HEXACOSANE	15.783	387711	2.512 ug/ml
12) N-OCTACOSANE	16.767	763890	5.055 ug/ml
13) N-TRIACONTANE	17.669	303846	2.066 ug/ml
14) N-DOTRIACONTANE	18.477	267346	1.880 ug/ml
15) N-TETRATRIACONTANE	19.325	214753	1.604 ug/ml
16) N-HEXATRIACONTANE	20.051	250109	1.917 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
Data File : FF003959.D
Signal(s) : FID2B.ch
Acq On : 22 Mar 2019 15:22
Operator : AJ\SJ
Sample : K2050-03
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CS-3

Integration File: autoint1.e
Quant Time: Mar 22 22:59:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

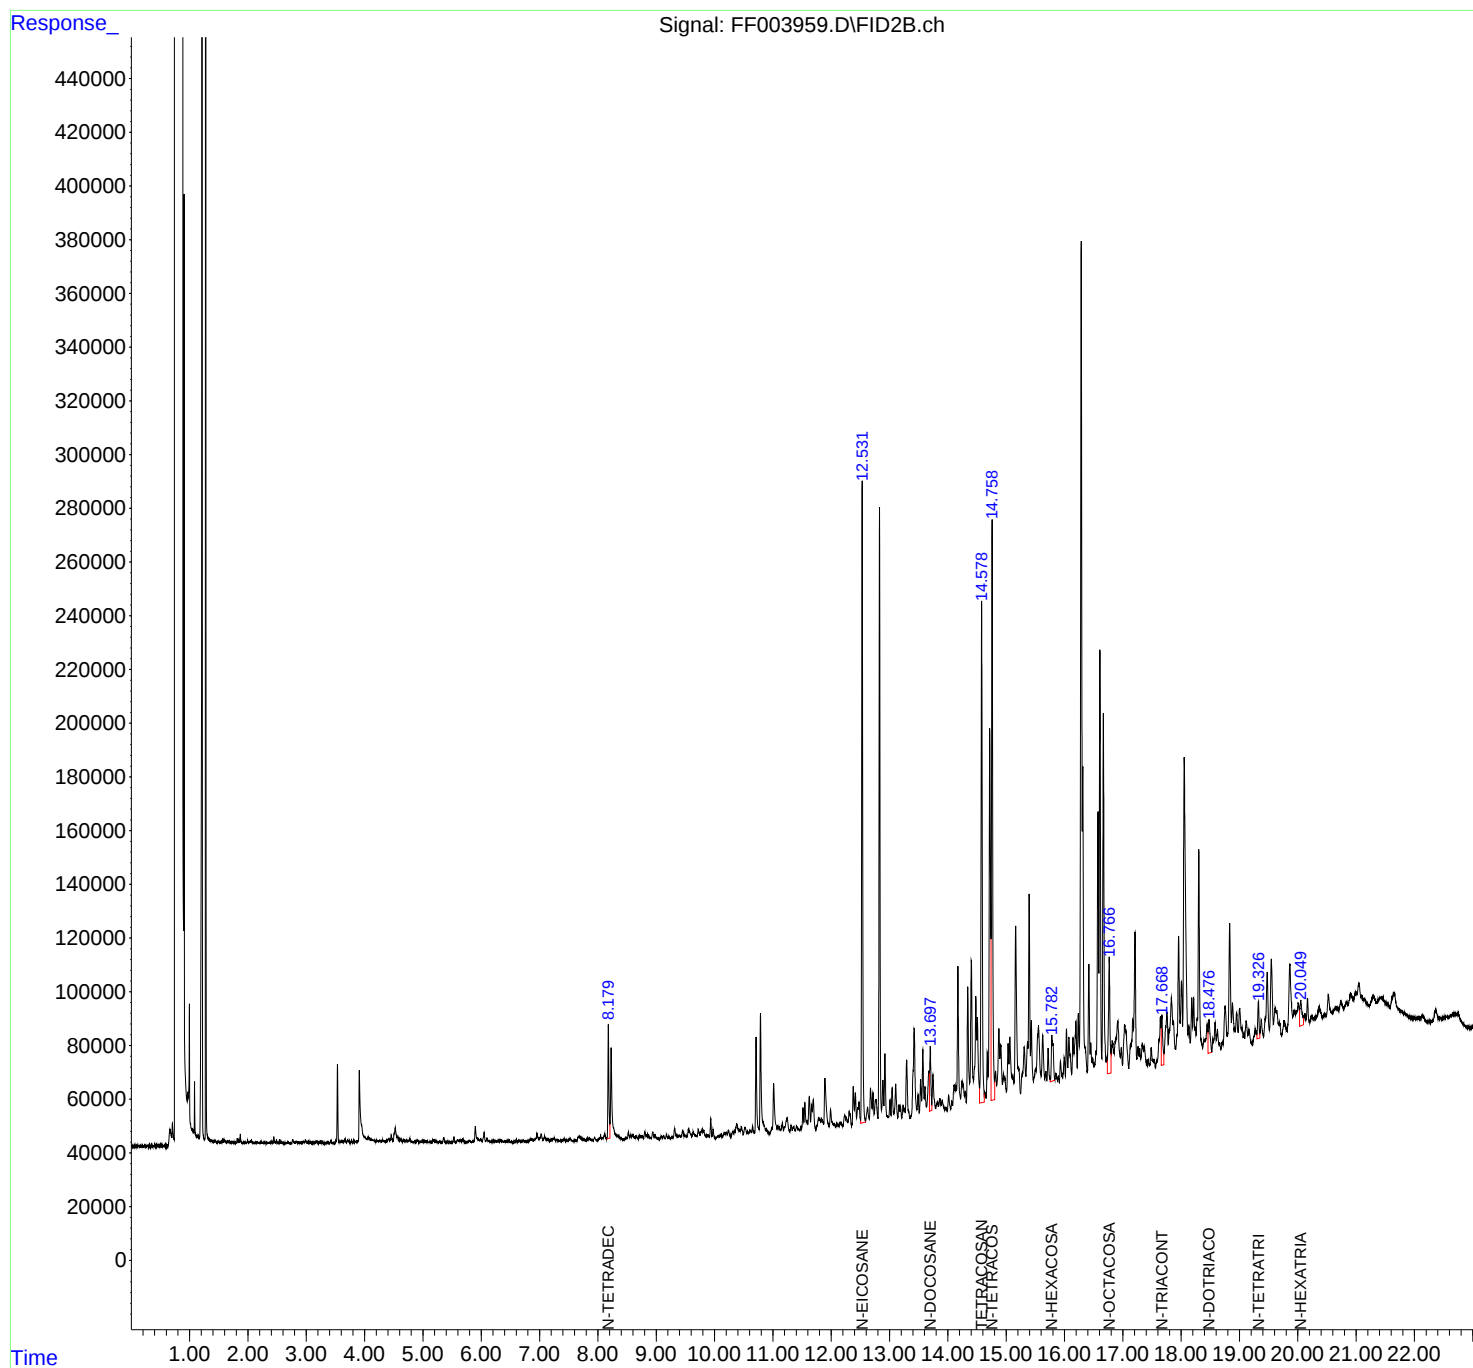


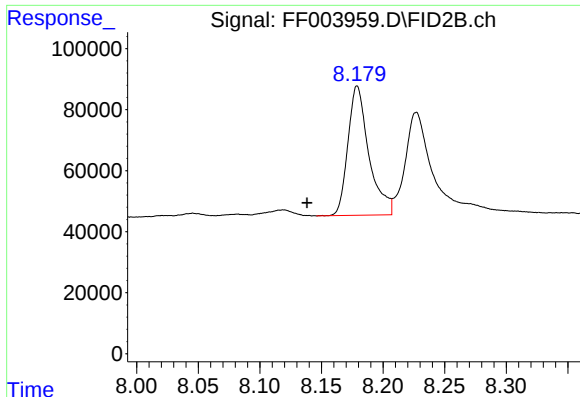

#4 N-TETRADECANE


R.T.: 8.179 min
Delta R.T.: 0.041 min
Response: 502798
Conc: 3.14 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-3

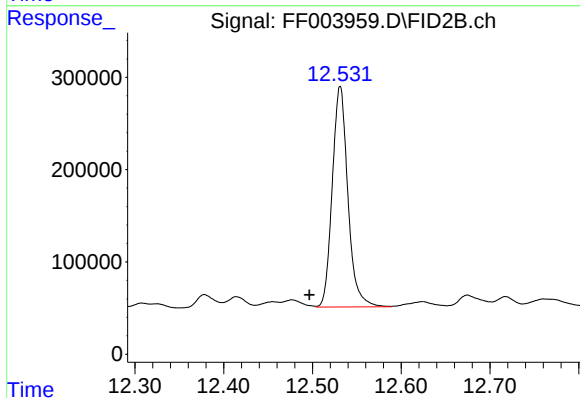


#7 N-EICOSANE

R.T.: 12.531 min
Delta R.T.: 0.035 min
Response: 2923885
Conc: 17.87 ug/ml

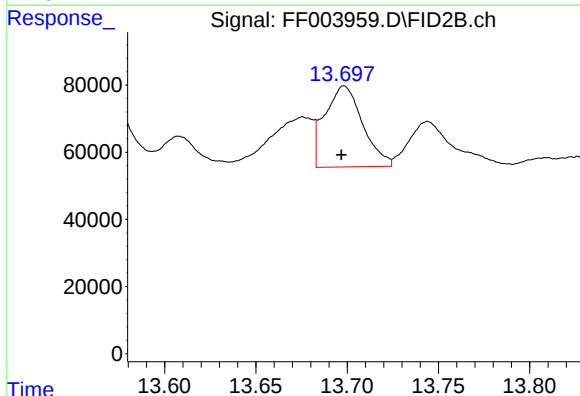


#8 N-DOCOSANE

R.T.: 13.698 min
Delta R.T.: 0.002 min
Response: 348662
Conc: 2.16 ug/ml

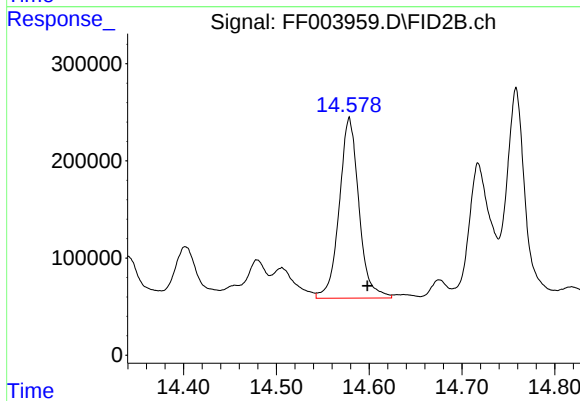

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.579 min
Delta R.T.: -0.020 min
Response: 2736698
Conc: 19.66 ug/ml

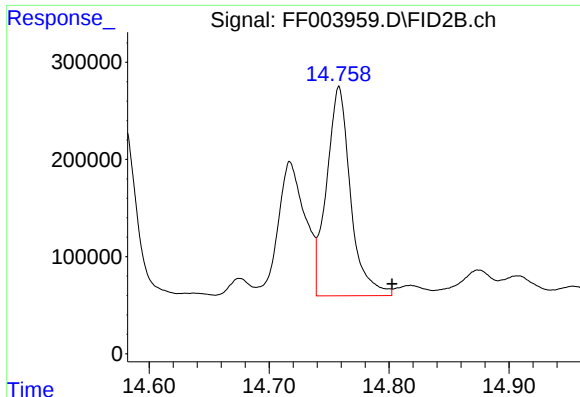

#10 N-TETRACOSANE


R.T.: 14.758 min
Delta R.T.: -0.044 min
Response: 2998154
Conc: 18.95 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-3

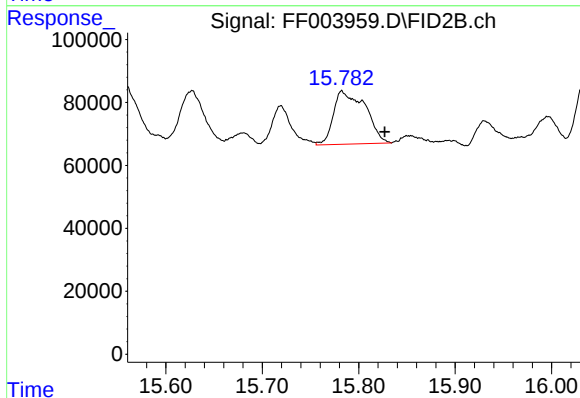


#11 N-HEXACOSANE

R.T.: 15.783 min
Delta R.T.: -0.044 min
Response: 387711
Conc: 2.51 ug/ml

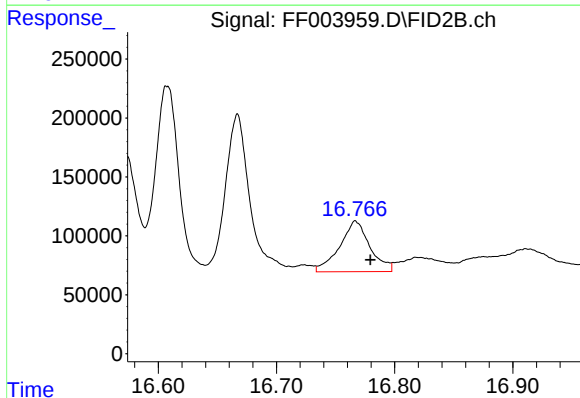


#12 N-OCTACOSANE

R.T.: 16.767 min
Delta R.T.: -0.013 min
Response: 763890
Conc: 5.06 ug/ml

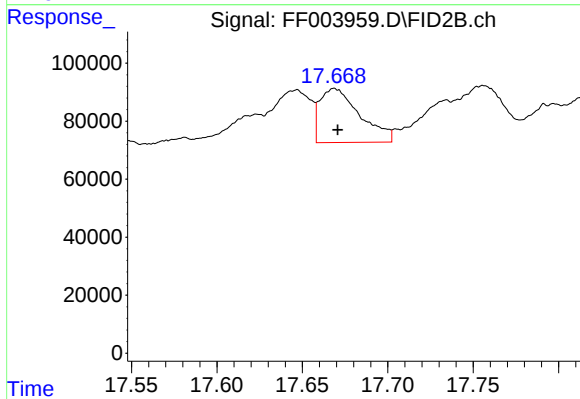

#13 N-TRIACONTANE


R.T.: 17.669 min
Delta R.T.: -0.002 min
Response: 303846
Conc: 2.07 ug/ml

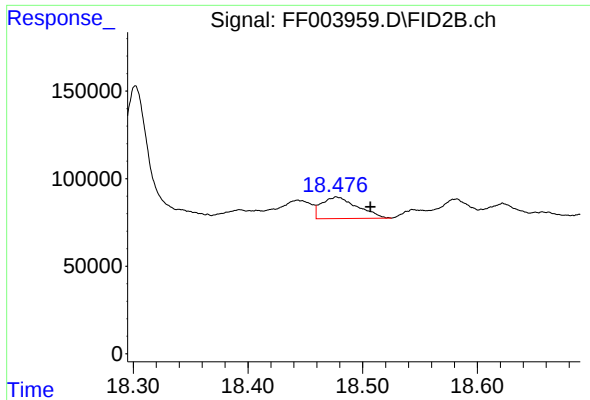

#14 N-DOTRIACONTANE


R.T.: 18.477 min
Delta R.T.: -0.029 min
Response: 267346
Conc: 1.88 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-3

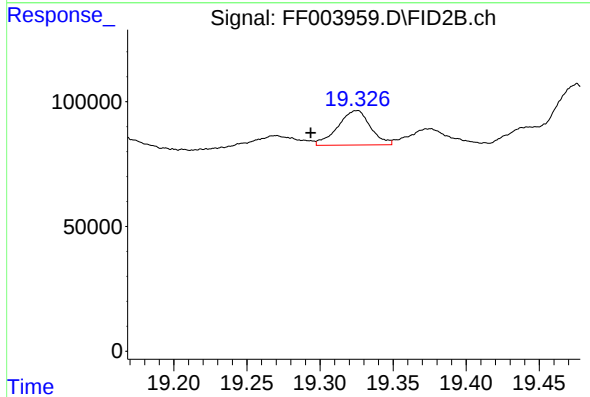

#15 N-TETRATRIACONTANE

R.T.: 19.325 min
Delta R.T.: 0.032 min
Response: 214753
Conc: 1.60 ug/ml

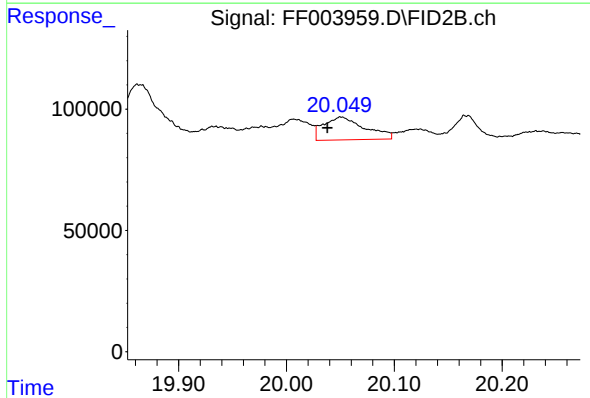

#16 N-HEXATRIACONTANE

R.T.: 20.051 min
Delta R.T.: 0.013 min
Response: 250109
Conc: 1.92 ug/ml