

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
 Data File : FF003961.D
 Signal(s) : FID2B.ch
 Acq On : 22 Mar 2019 16:23
 Operator : AJ\SJ
 Sample : K2050-05
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CS-1

Integration File: autoint1.e
 Quant Time: Mar 22 23:00:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.580	2140451	15.374 ug/ml
Target Compounds			
4) N-TETRADECANE	8.180	344512	2.149 ug/ml
7) N-EICOSANE	12.478	157313	0.962 ug/ml
8) N-DOCOSANE	13.699	709509	4.396 ug/ml
10) N-TETRACOSANE	14.760	3679424	23.255 ug/ml
11) N-HEXACOSANE	15.784	569302	3.689 ug/ml
12) N-OCTACOSANE	16.769	1158391	7.666 ug/ml
13) N-TRIACONTANE	17.671	341256	2.320 ug/ml
14) N-DOTRIACONTANE	18.482	332892	2.341 ug/ml
15) N-TETRATRIACONTANE	19.270	147714	1.103 ug/ml
16) N-HEXATRIACONTANE	20.055	259557	1.989 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
Data File : FF003961.D
Signal(s) : FID2B.ch
Acq On : 22 Mar 2019 16:23
Operator : AJ\SJ
Sample : K2050-05
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CS-1

Integration File: autoint1.e
Quant Time: Mar 22 23:00:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

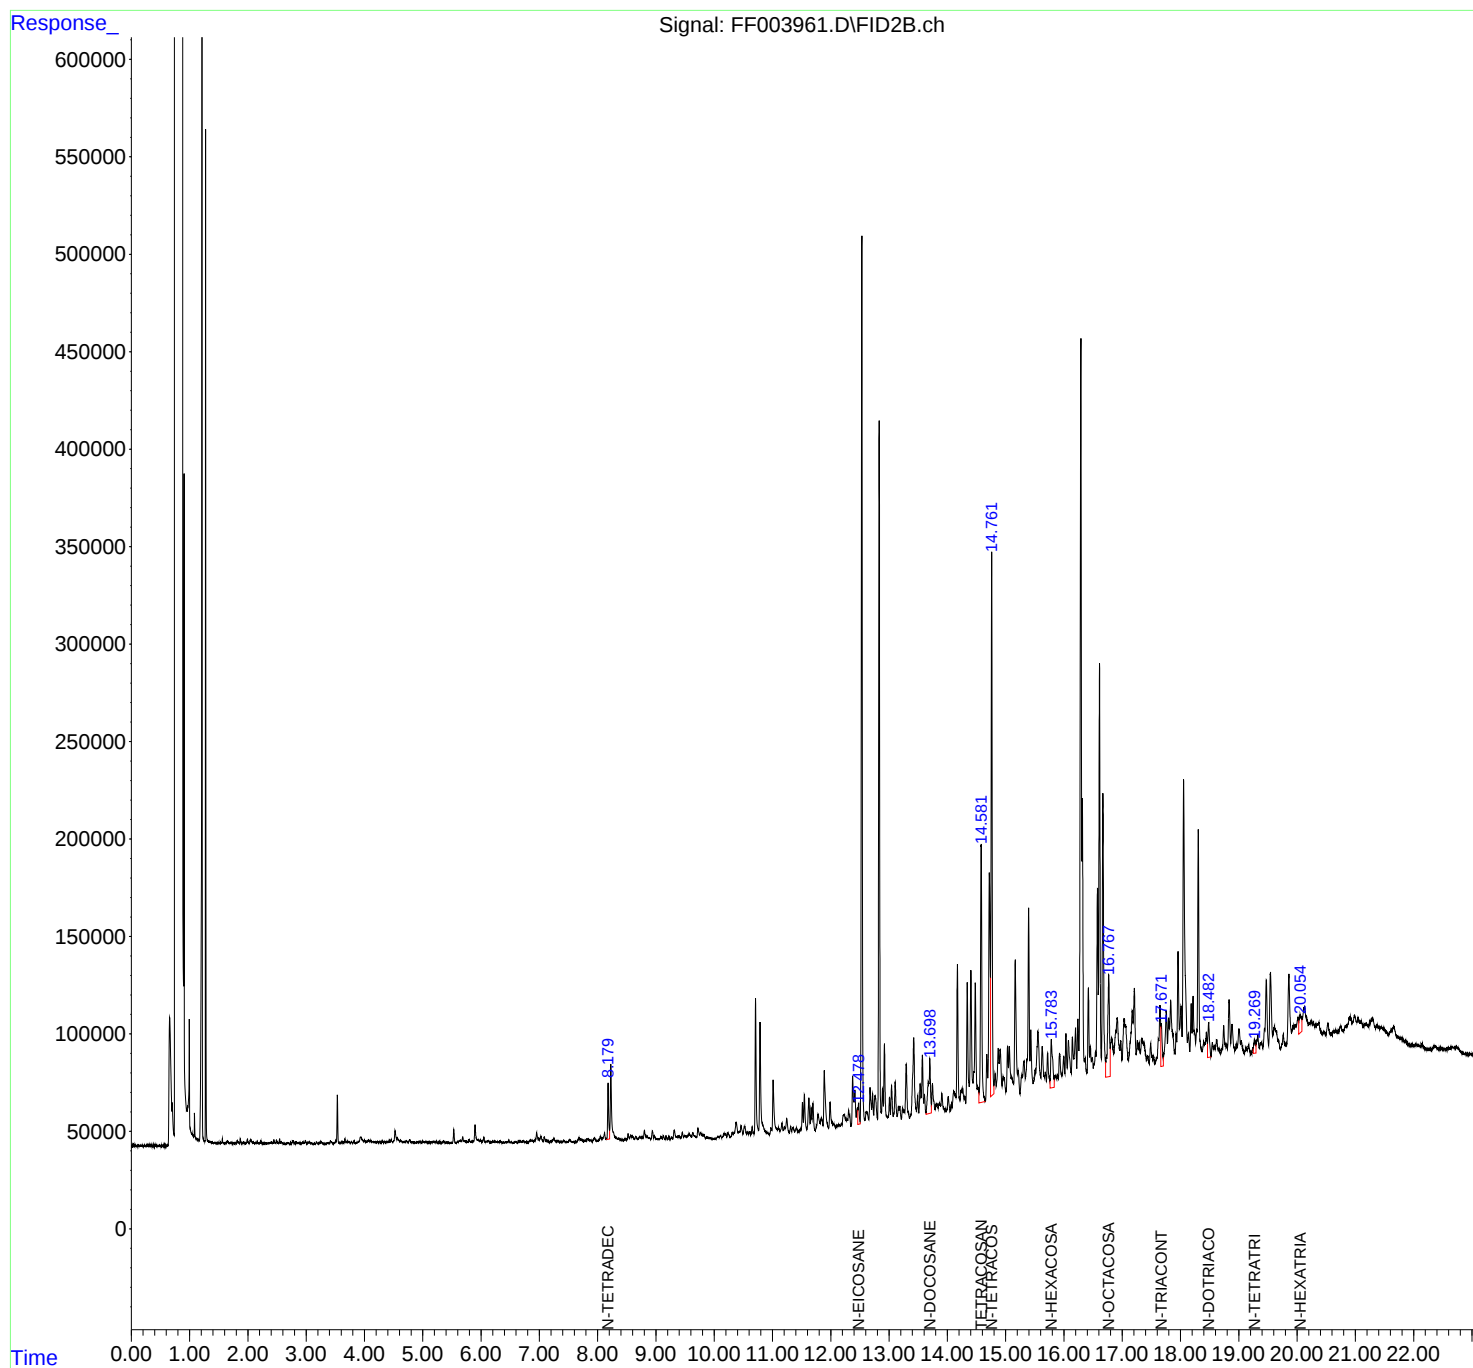


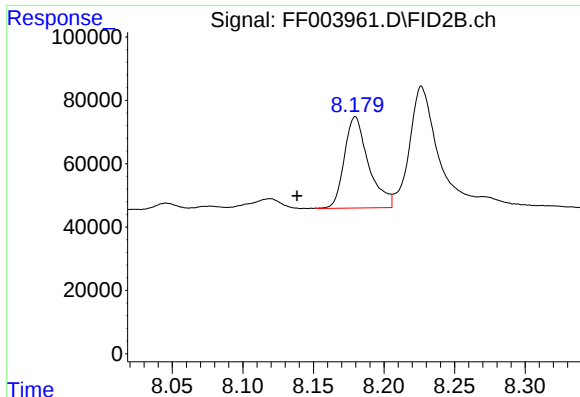

#4 N-TETRADECANE


R.T.: 8.180 min
Delta R.T.: 0.041 min
Response: 344512
Conc: 2.15 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-1

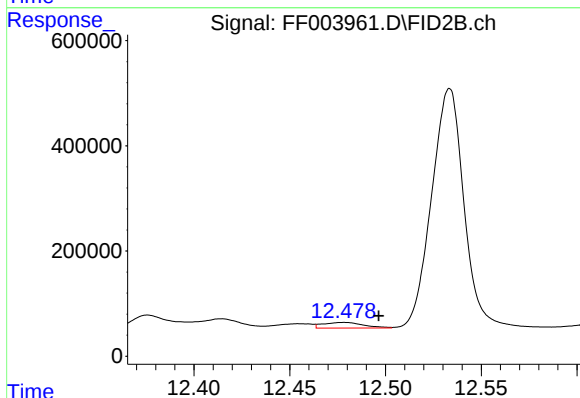


#7 N-EICOSANE

R.T.: 12.478 min
Delta R.T.: -0.018 min
Response: 157313
Conc: 0.96 ug/ml

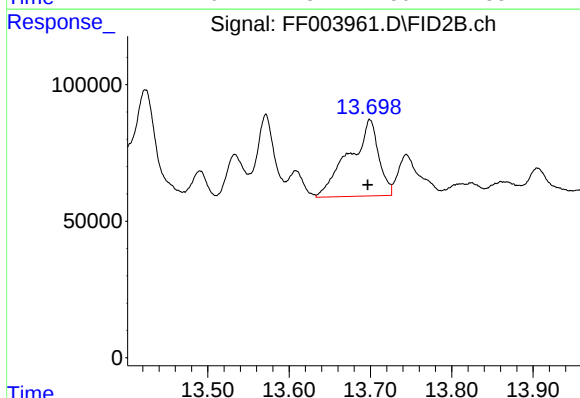


#8 N-DOCOSANE

R.T.: 13.699 min
Delta R.T.: 0.003 min
Response: 709509
Conc: 4.40 ug/ml

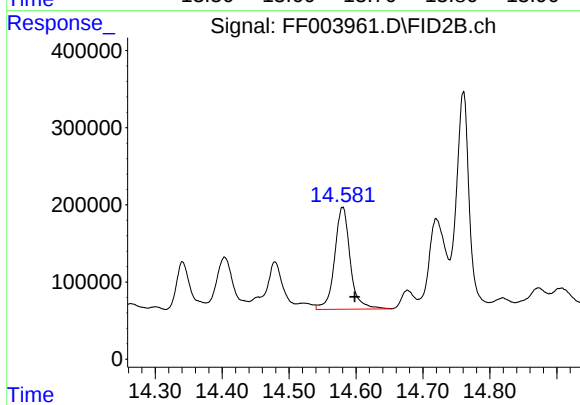

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.580 min
Delta R.T.: -0.018 min
Response: 2140451
Conc: 15.37 ug/ml

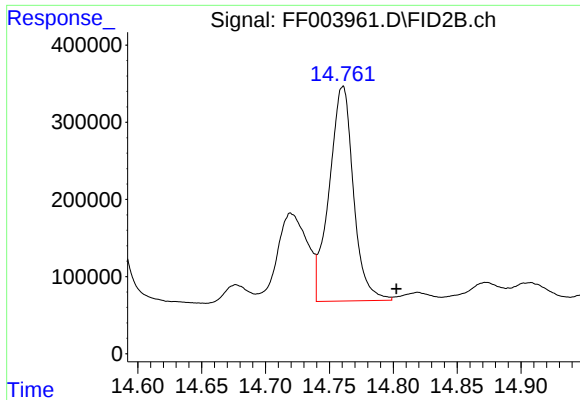

#10 N-TETRACOSANE


R.T.: 14.760 min
Delta R.T.: -0.042 min
Response: 3679424
Conc: 23.26 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-1

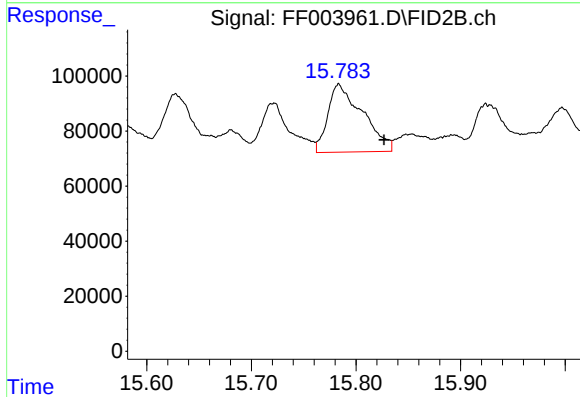


#11 N-HEXACOSANE

R.T.: 15.784 min
Delta R.T.: -0.043 min
Response: 569302
Conc: 3.69 ug/ml

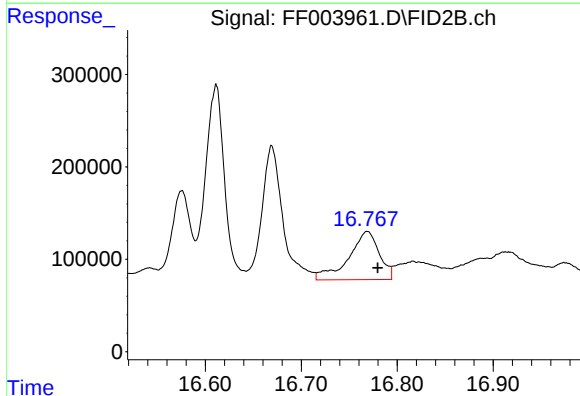


#12 N-OCTACOSANE

R.T.: 16.769 min
Delta R.T.: -0.011 min
Response: 1158391
Conc: 7.67 ug/ml

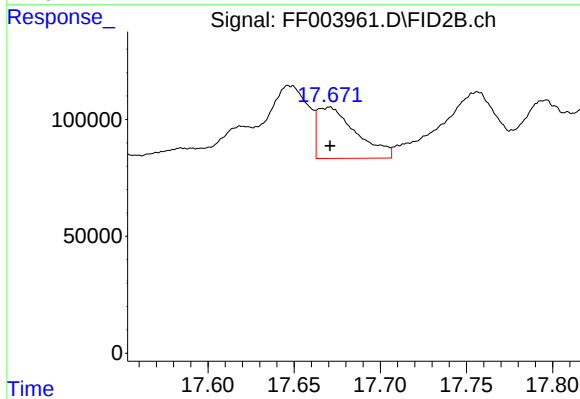

#13 N-TRIACONTANE


R.T.: 17.671 min
Delta R.T.: 0.000 min
Response: 341256
Conc: 2.32 ug/ml

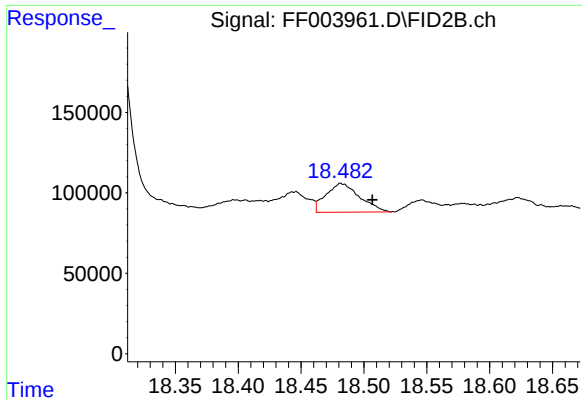

#14 N-DOTRIACONTANE


R.T.: 18.482 min
Delta R.T.: -0.025 min
Response: 332892
Conc: 2.34 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-1

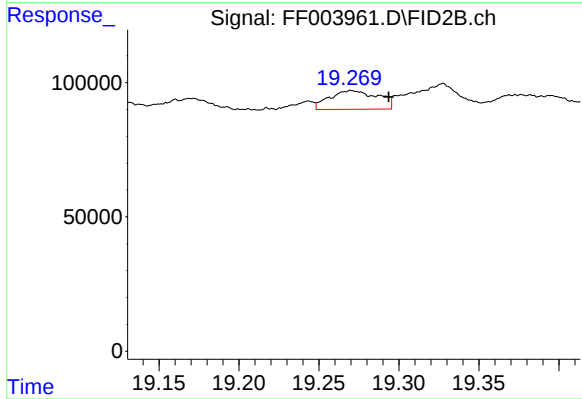

#15 N-TETRATRIACONTANE

R.T.: 19.270 min
Delta R.T.: -0.023 min
Response: 147714
Conc: 1.10 ug/ml

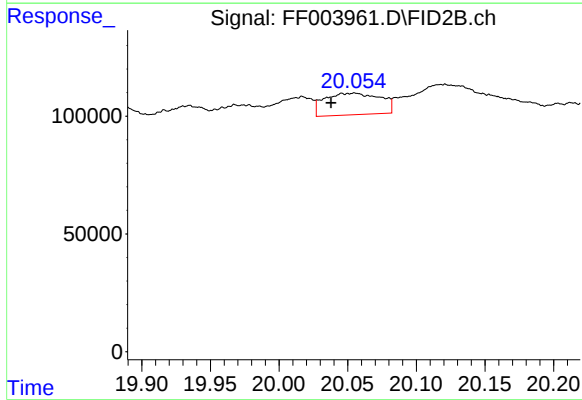

#16 N-HEXATRIACONTANE

R.T.: 20.055 min
Delta R.T.: 0.017 min
Response: 259557
Conc: 1.99 ug/ml