

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
 Data File : FF003962.D
 Signal(s) : FID2B.ch
 Acq On : 22 Mar 2019 16:57
 Operator : AJ\SJ
 Sample : K2050-01 5X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CS-5

Integration File: autoint1.e
 Quant Time: Mar 22 23:00:33 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.580	608852	4.373 ug/ml
Target Compounds			
6) N-OCTADECANE	11.245f	153063	0.929 ug/ml
7) N-EICOSANE	12.536	8258551	50.482 ug/ml
8) N-DOCOSANE	13.700	298483	1.849 ug/ml
10) N-TETRACOSANE	14.759	3790110	23.955 ug/ml
11) N-HEXACOSANE	15.782	356246	2.308 ug/ml
12) N-OCTACOSANE	16.770	322919	2.137 ug/ml
13) N-TRIACONTANE	17.647	163861	1.114 ug/ml
16) N-HEXATRIACONTANE	20.053	329358	2.524 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
Data File : FF003962.D
Signal(s) : FID2B.ch
Acq On : 22 Mar 2019 16:57
Operator : AJ\SJ
Sample : K2050-01 5X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CS-5

Integration File: autoint1.e
Quant Time: Mar 22 23:00:33 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

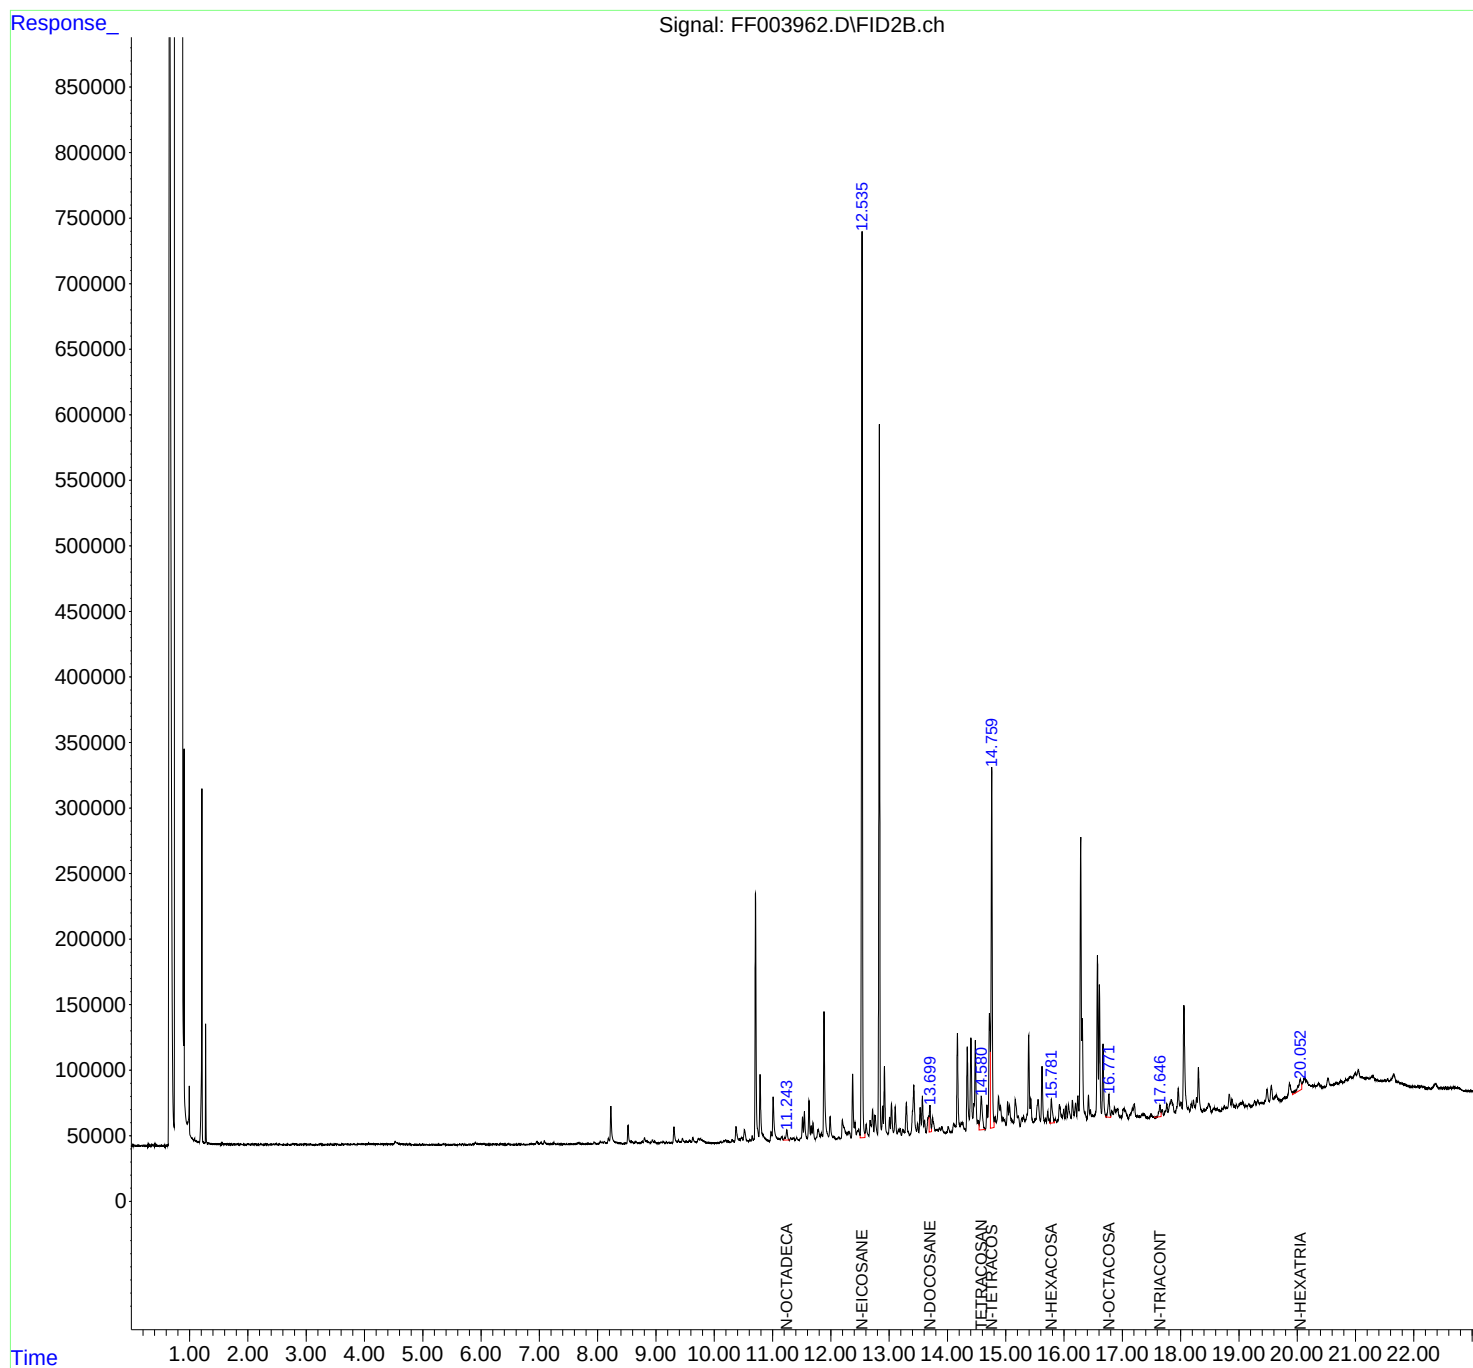


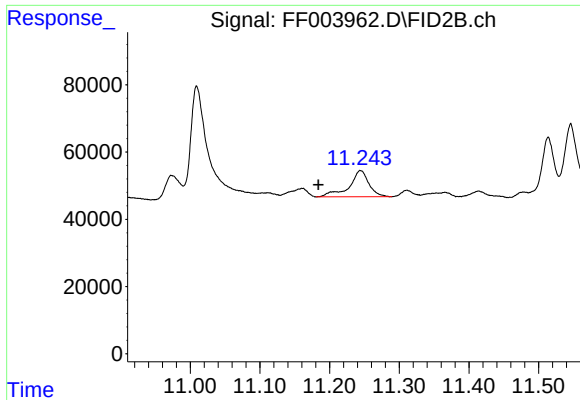

#6 N-OCTADECANE


R.T.: 11.245 min
Delta R.T.: 0.061 min
Response: 153063
Conc: 0.93 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-5

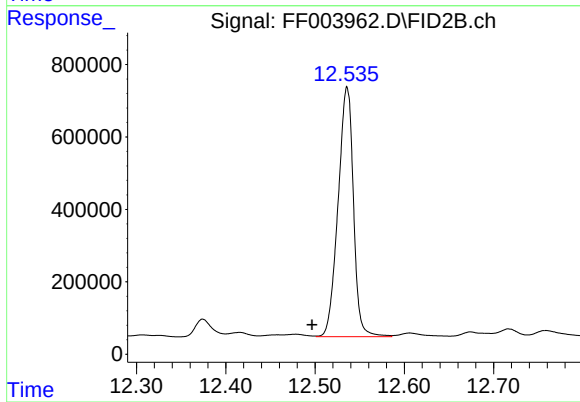


#7 N-EICOSANE

R.T.: 12.536 min
Delta R.T.: 0.039 min
Response: 825851
Conc: 50.48 ug/ml

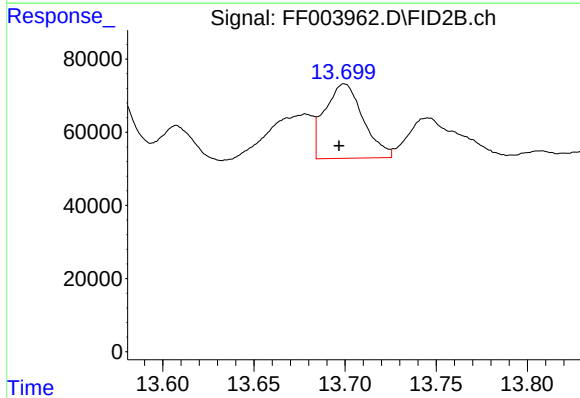


#8 N-DOCOSANE

R.T.: 13.700 min
Delta R.T.: 0.003 min
Response: 298483
Conc: 1.85 ug/ml

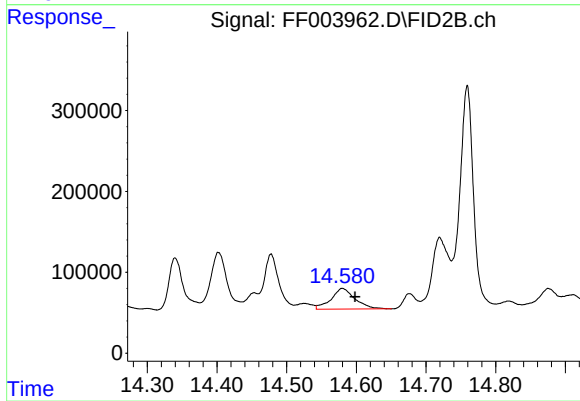

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.580 min
Delta R.T.: -0.018 min
Response: 608852
Conc: 4.37 ug/ml

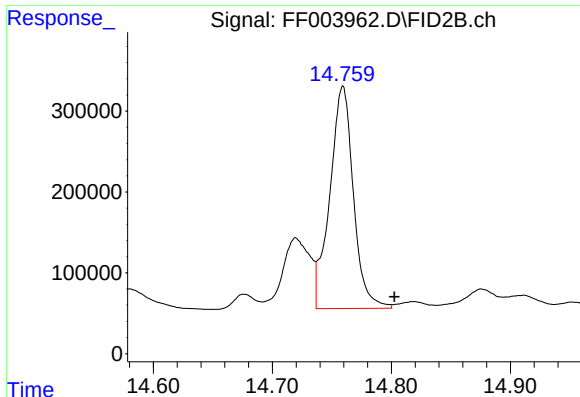

#10 N-TETRACOSANE


R.T.: 14.759 min
Delta R.T.: -0.043 min
Response: 3790110
Conc: 23.95 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-5

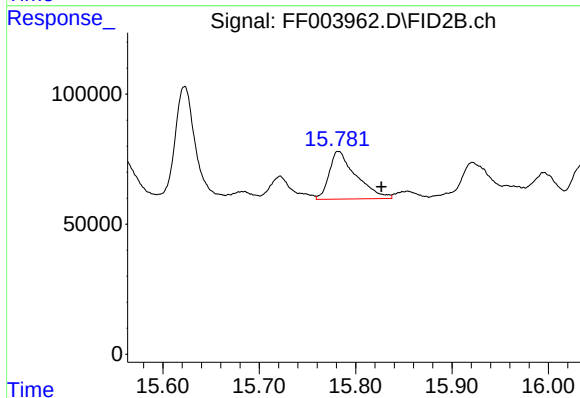


#11 N-HEXACOSANE

R.T.: 15.782 min
Delta R.T.: -0.045 min
Response: 356246
Conc: 2.31 ug/ml

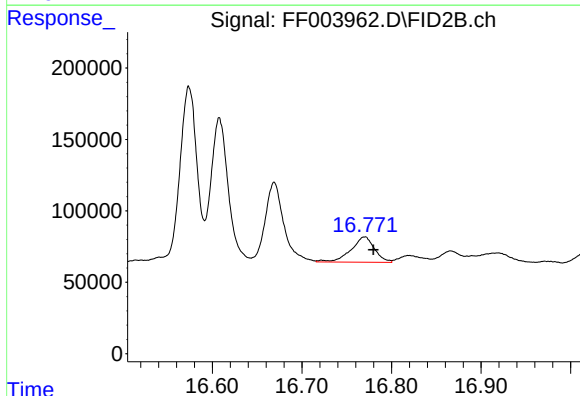


#12 N-OCTACOSANE

R.T.: 16.770 min
Delta R.T.: -0.009 min
Response: 322919
Conc: 2.14 ug/ml

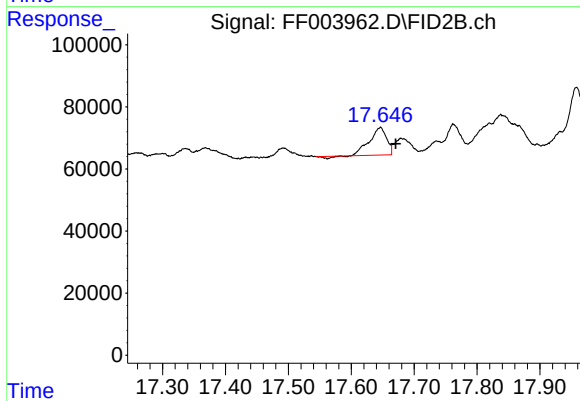

#13 N-TRIACONTANE

R.T.: 17.647 min
Delta R.T.: -0.024 min
Response: 163861
Conc: 1.11 ug/ml

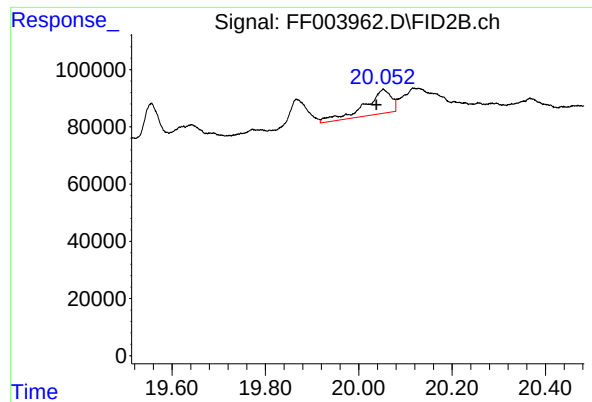

#16 N-HEXATRIACONTANE

R.T.: 20.053 min
Delta R.T.: 0.015 min
Response: 329358
Conc: 2.52 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-5