

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
 Data File : FF003963.D
 Signal(s) : FID2B.ch
 Acq On : 22 Mar 2019 17:27
 Operator : AJ\SJ
 Sample : K2050-04 2X
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 CS-2

Integration File: autoint1.e
 Quant Time: Mar 22 23:00:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.578	1464969	10.522 ug/ml
Target Compounds			
4) N-TETRADECANE	8.181	165885	1.035 ug/ml
7) N-EICOSANE	12.532	3850087	23.535 ug/ml
8) N-DOCOSANE	13.699	522303	3.236 ug/ml
10) N-TETRACOSANE	14.758	2618763	16.551 ug/ml
11) N-HEXACOSANE	15.801	218050	1.413 ug/ml
12) N-OCTACOSANE	16.769	599285	3.966 ug/ml
13) N-TRIACONTANE	17.673	183335	1.246 ug/ml
14) N-DOTRIACONTANE	18.479	296401	2.084 ug/ml
15) N-TETRATRIACONTANE	19.269	115662	0.864 ug/ml
16) N-HEXATRIACONTANE	20.054	250078	1.917 ug/ml
18) N-TETRACONTANE	21.647	253787	2.040 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032219\
Data File : FF003963.D
Signal(s) : FID2B.ch
Acq On : 22 Mar 2019 17:27
Operator : AJ\SJ
Sample : K2050-04 2X
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CS-2

Integration File: autoint1.e
Quant Time: Mar 22 23:00:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

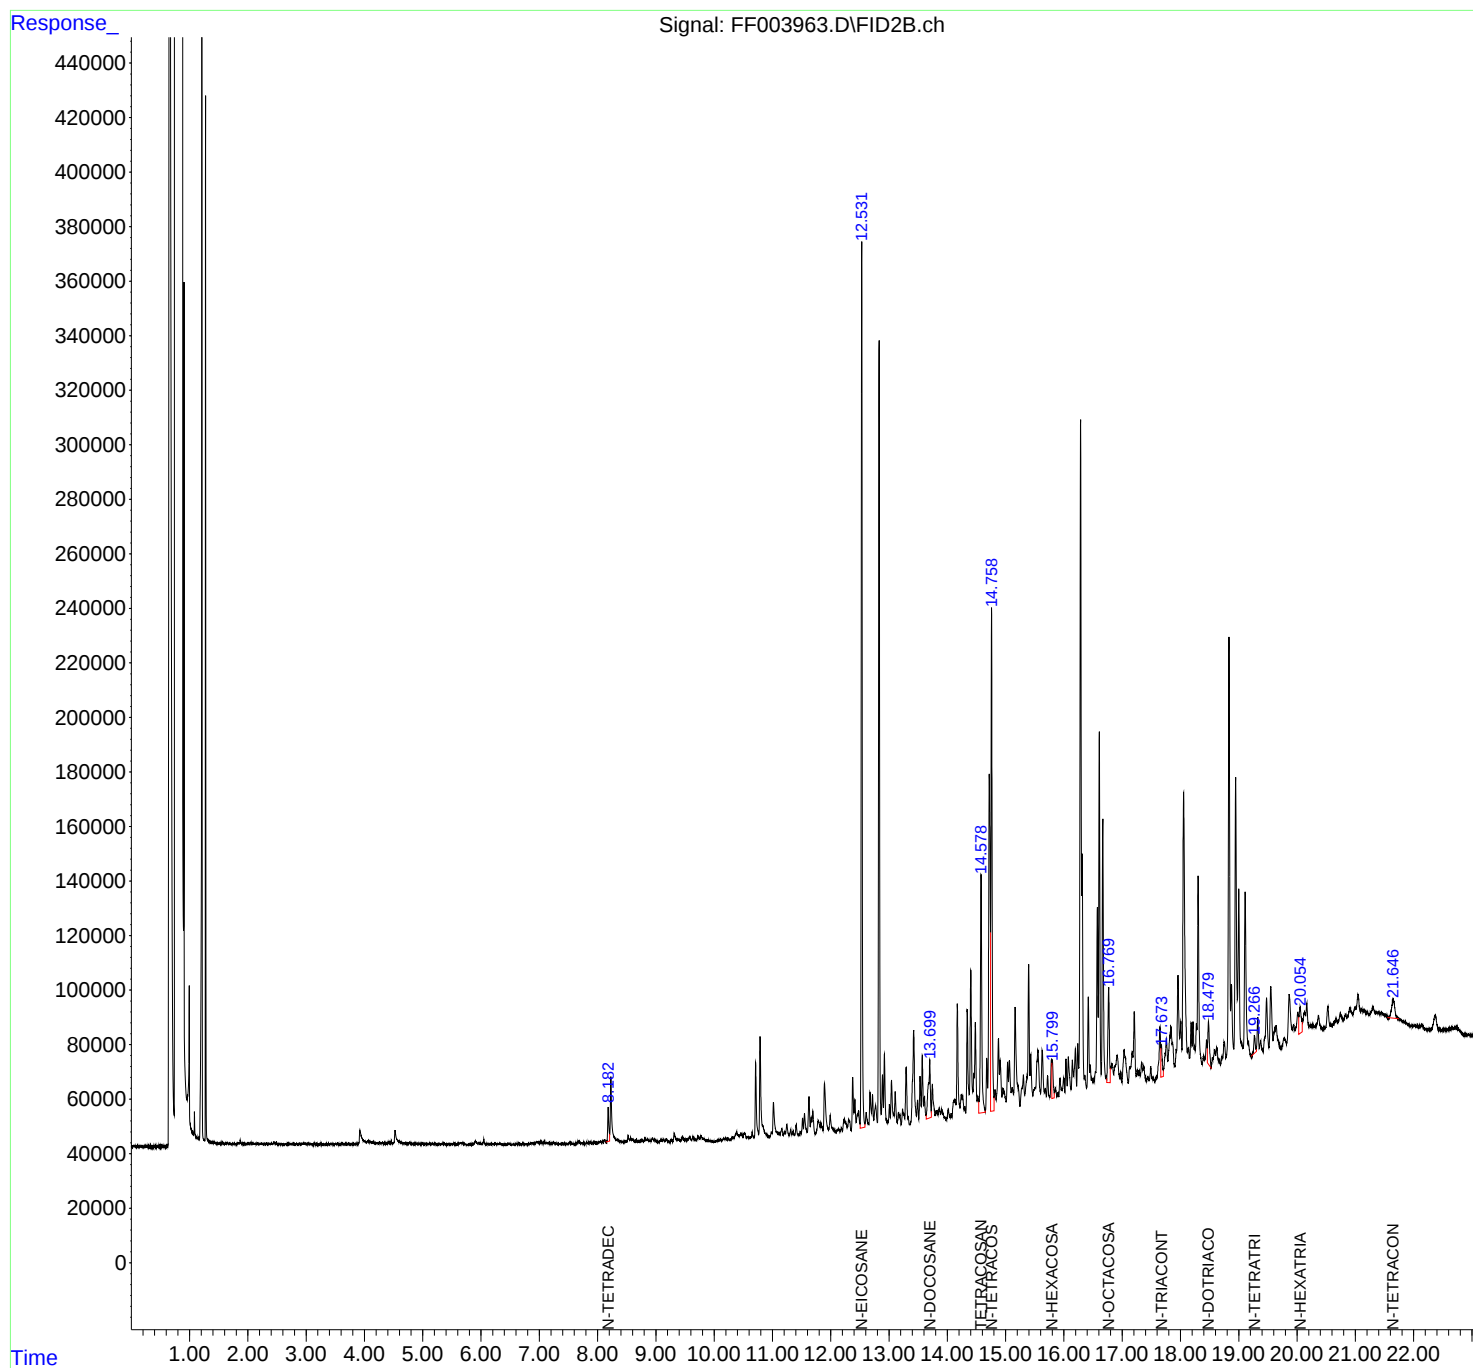


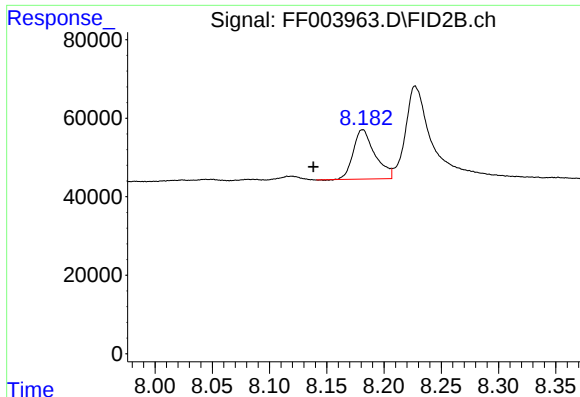

#4 N-TETRADECANE


R.T.: 8.181 min
Delta R.T.: 0.043 min
Response: 165885
Conc: 1.03 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-2

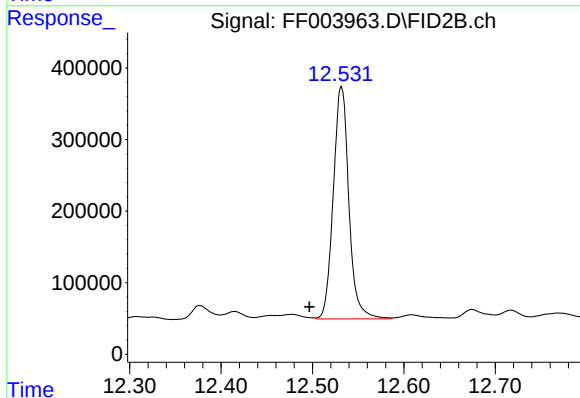


#7 N-EICOSANE

R.T.: 12.532 min
Delta R.T.: 0.035 min
Response: 3850087
Conc: 23.53 ug/ml

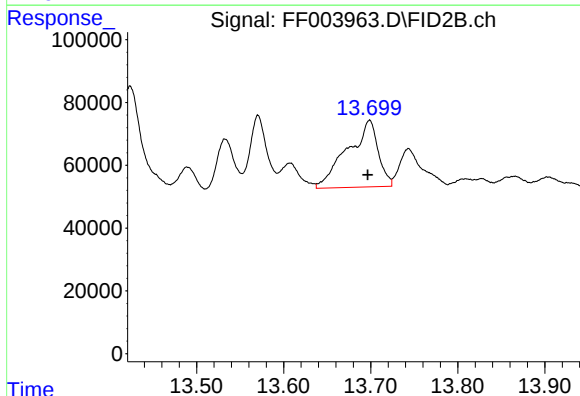


#8 N-DOCOSANE

R.T.: 13.699 min
Delta R.T.: 0.002 min
Response: 522303
Conc: 3.24 ug/ml

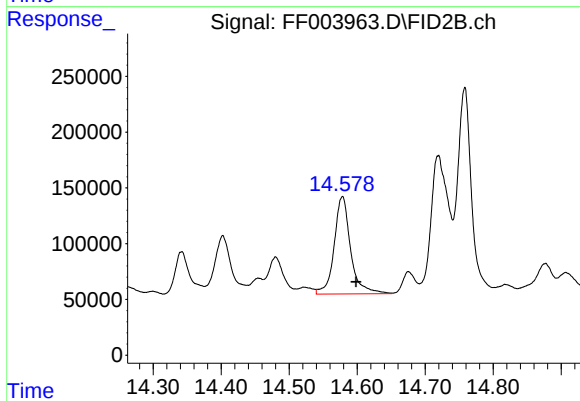

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.578 min
Delta R.T.: -0.020 min
Response: 1464969
Conc: 10.52 ug/ml

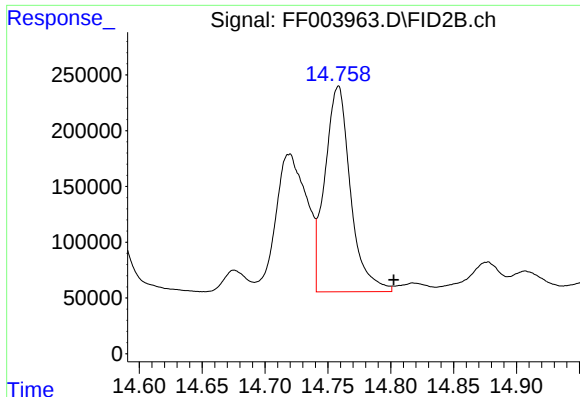

#10 N-TETRACOSANE


R.T.: 14.758 min
Delta R.T.: -0.044 min
Response: 2618763
Conc: 16.55 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-2

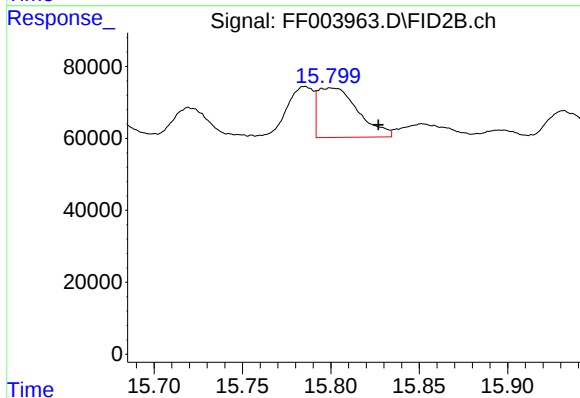


#11 N-HEXACOSANE

R.T.: 15.801 min
Delta R.T.: -0.026 min
Response: 218050
Conc: 1.41 ug/ml

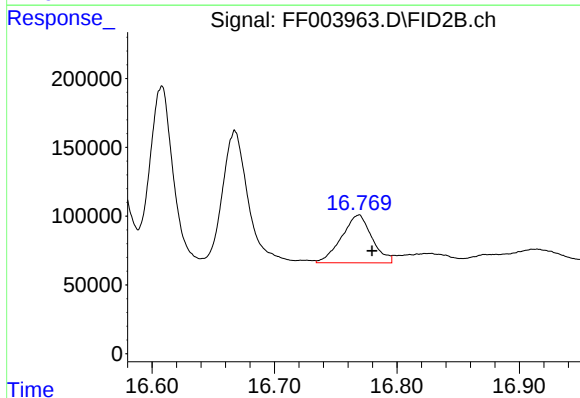


#12 N-OCTACOSANE

R.T.: 16.769 min
Delta R.T.: -0.011 min
Response: 599285
Conc: 3.97 ug/ml

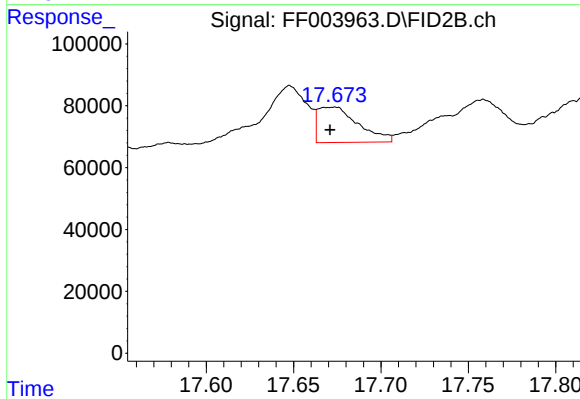

#13 N-TRIACONTANE


R.T.: 17.673 min
Delta R.T.: 0.003 min
Response: 183335
Conc: 1.25 ug/ml

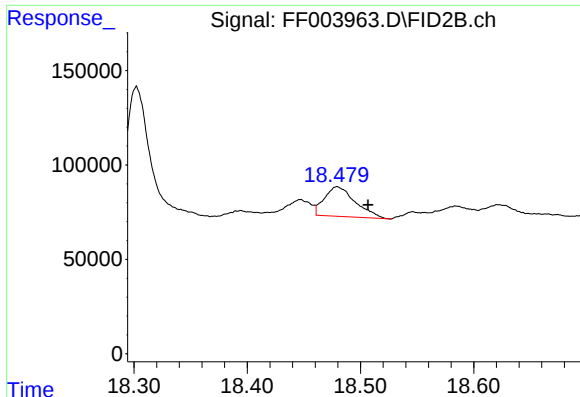

#14 N-DOTRIACONTANE


R.T.: 18.479 min
Delta R.T.: -0.027 min
Response: 296401
Conc: 2.08 ug/ml

Instrument :
FID_F
ClientSampleId :
CS-2

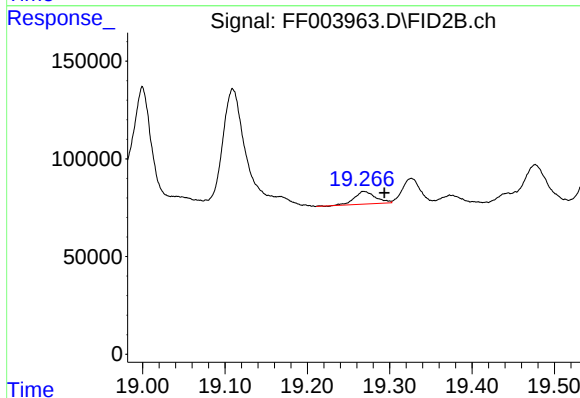


#15 N-TETRATRIACONTANE

R.T.: 19.269 min
Delta R.T.: -0.025 min
Response: 115662
Conc: 0.86 ug/ml

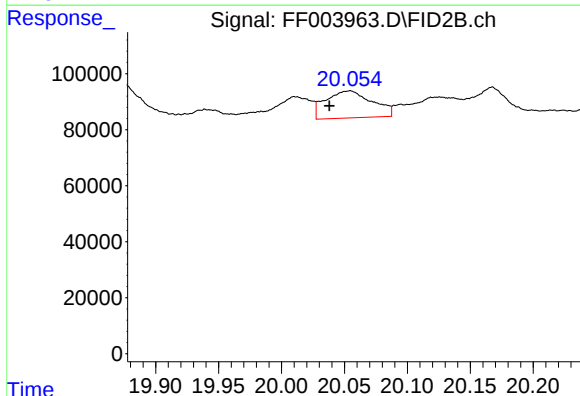

#16 N-HEXATRIACONTANE

R.T.: 20.054 min
Delta R.T.: 0.016 min
Response: 250078
Conc: 1.92 ug/ml

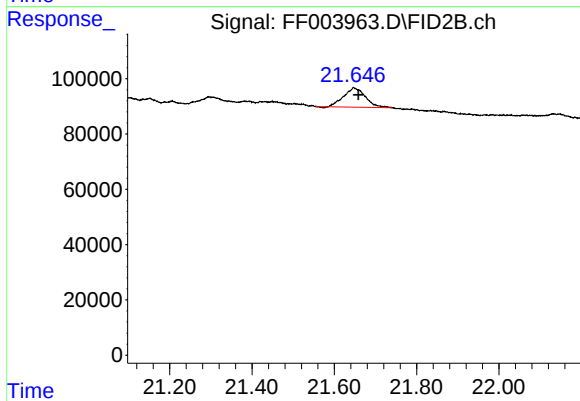

#18 N-TETRACONTANE

R.T.: 21.647 min
Delta R.T.: -0.012 min
Response: 253787
Conc: 2.04 ug/ml