

Data Path : P:\HPCHEM1\FID\_G\Data\FG020718\  
Data File : FG000050.D  
Signal(s) : FID1A.ch  
Acq On : 07 Feb 2018 08:30  
Operator : UA\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Feb 07 12:14:39 2018  
Quant Method : P:\HPCHEM1\FID\_F\Method\FG020118.M  
Quant Title :  
QLast Update : Fri Feb 02 10:17:23 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    |                 | R.T.   | Response | Conc Units  |
|-----------------------------|-----------------|--------|----------|-------------|
| -----                       |                 |        |          |             |
| System Monitoring Compounds |                 |        |          |             |
| Target Compounds            |                 |        |          |             |
| 13)                         | N-TRIACONTANE   | 17.627 | 51215    | 0.389 ug/ml |
| 14)                         | N-DOTRIACONTANE | 18.461 | 64325    | 0.589 ug/ml |
| -----                       |                 |        |          |             |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID\_G\Data\FG020718\  
Data File : FG000050.D  
Signal(s) : FID1A.ch  
Acq On : 07 Feb 2018 08:30  
Operator : UA\AJ  
Sample : MECL2  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Feb 07 12:14:39 2018  
Quant Method : P:\HPCHEM1\FID\_F\Method\FG020118.M  
Quant Title :  
QLast Update : Fri Feb 02 10:17:23 2018  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

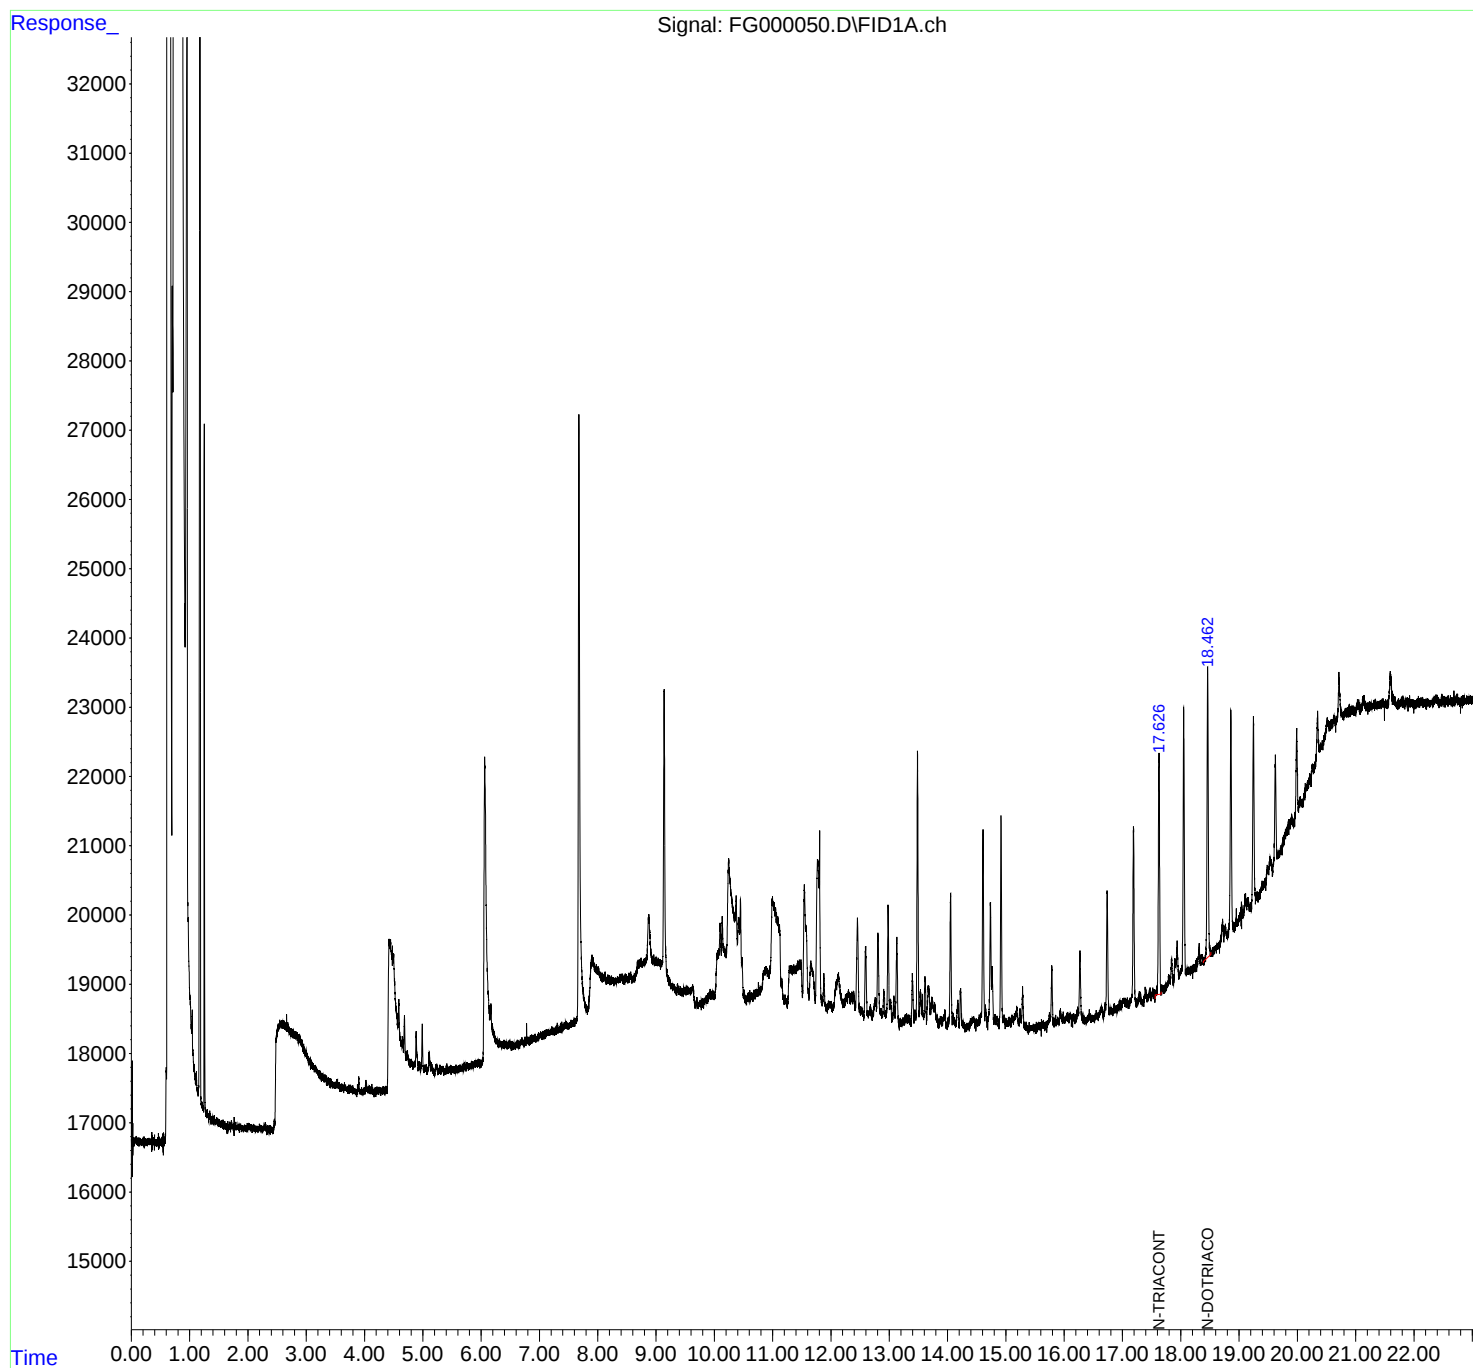

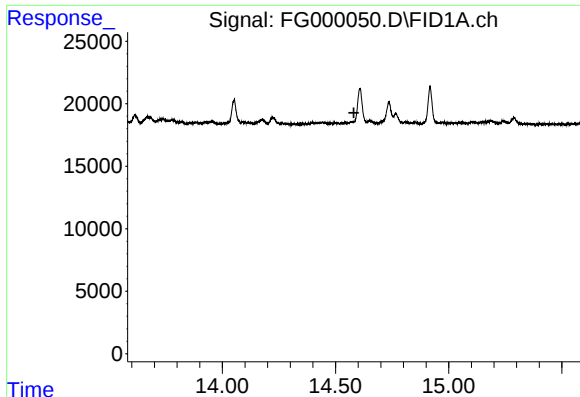


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.581 min  
Response: 0  
Conc: N.D.

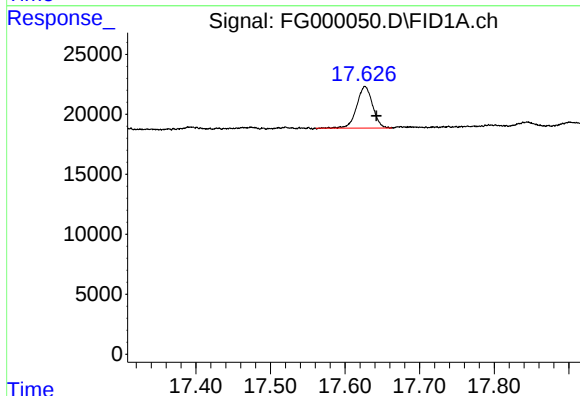

#13 N-TRIACONTANE

R.T.: 17.627 min  
Delta R.T.: -0.015 min  
Response: 51215  
Conc: 0.39 ug/ml

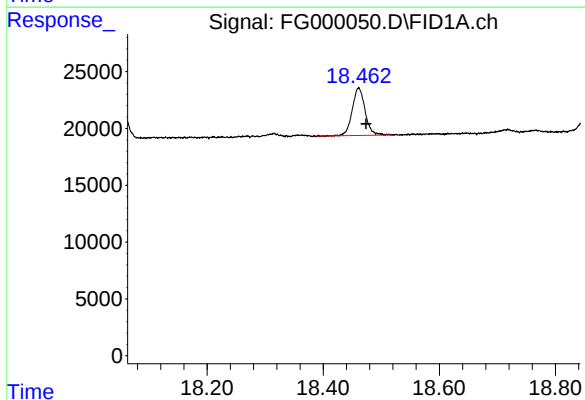

#14 N-DOTRIACONTANE

R.T.: 18.461 min  
Delta R.T.: -0.013 min  
Response: 64325  
Conc: 0.59 ug/ml