

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010919\
 Data File : FF003178.D
 Signal(s) : FID2B.ch
 Acq On : 09 Jan 2019 16:35
 Operator : AJ\SJ
 Sample : K1006-05 2X
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 10 00:23:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.619	866706	6.519 ug/ml
Target Compounds			
4) N-TETRADECANE	8.220	647571	4.248 ug/ml
7) N-EICOSANE	12.569	478115	3.140 ug/ml
10) N-TETRACOSANE	14.792	269227	1.807 ug/ml
11) N-HEXACOSANE	15.846	148720	1.011 ug/ml
12) N-OCTACOSANE	16.799	394810	2.713 ug/ml
13) N-TRIACONTANE	17.692	410854	2.877 ug/ml
14) N-DOTRIACONTANE	18.528	447831	3.361 ug/ml
15) N-TETRATRIACONTANE	19.321	66071	0.533 ug/ml
16) N-HEXATRIACONTANE	20.068	68683	0.609 ug/ml
17) N-OCTATRIACONTANE	20.799	236403	2.359 ug/ml
18) N-TETRACONTANE	21.715	105355	1.045 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010919\
Data File : FF003178.D
Signal(s) : FID2B.ch
Acq On : 09 Jan 2019 16:35
Operator : AJ\SJ
Sample : K1006-05 2X
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 10 00:23:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

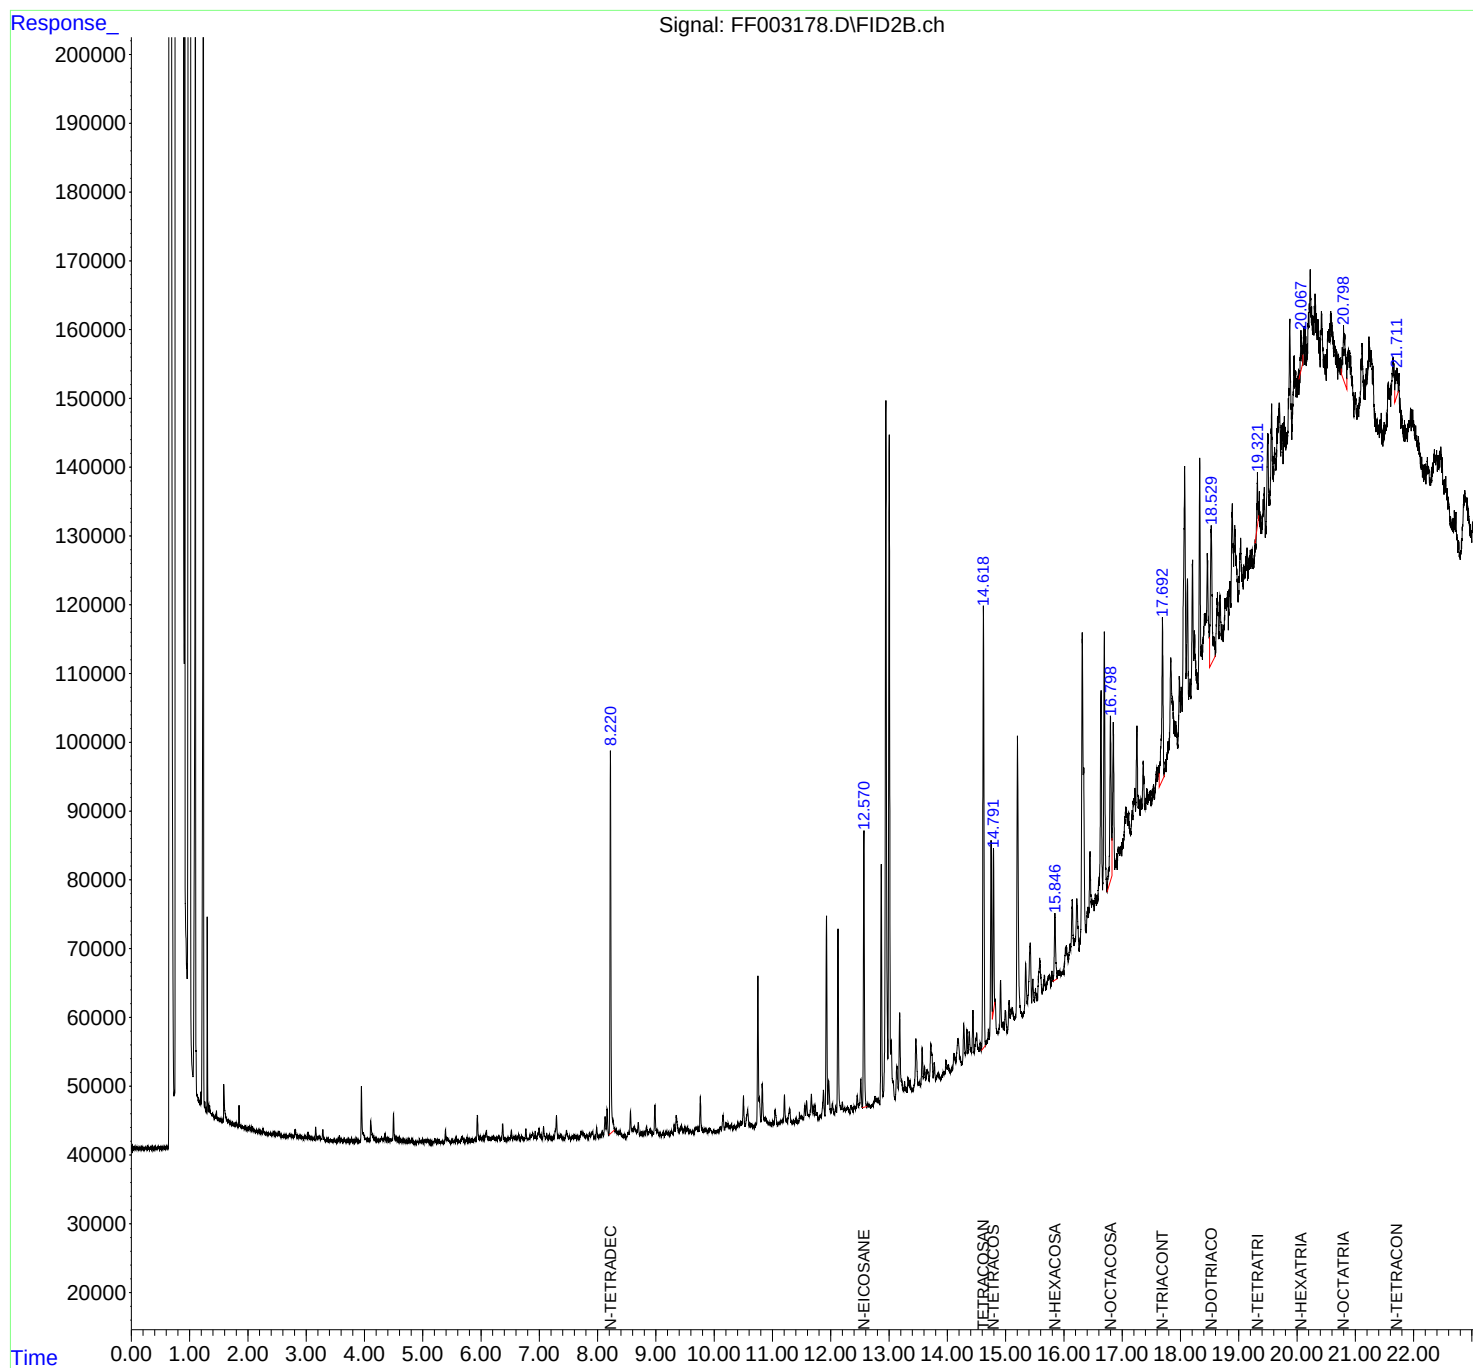

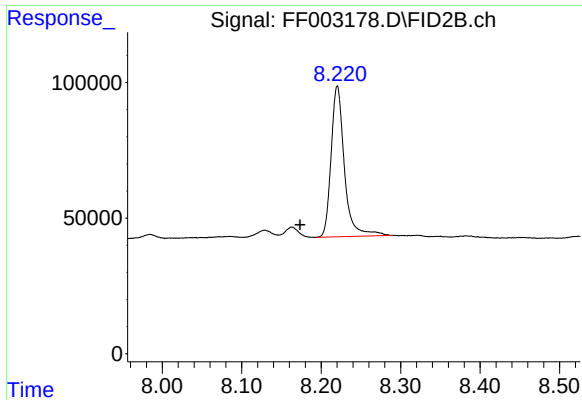


#4 N-TETRADECANE

R.T.: 8.220 min
Delta R.T.: 0.047 min
Response: 647571
Conc: 4.25 ug/ml

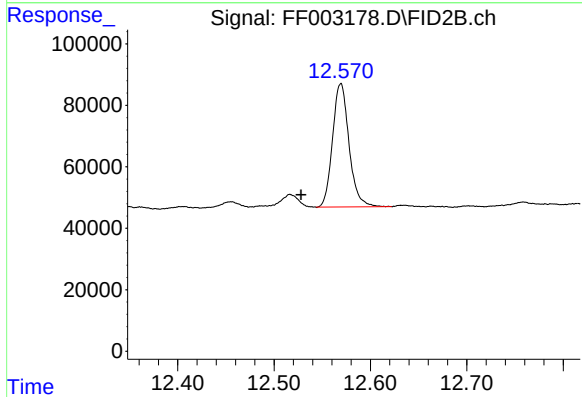


#7 N-EICOSANE

R.T.: 12.569 min
Delta R.T.: 0.041 min
Response: 478115
Conc: 3.14 ug/ml

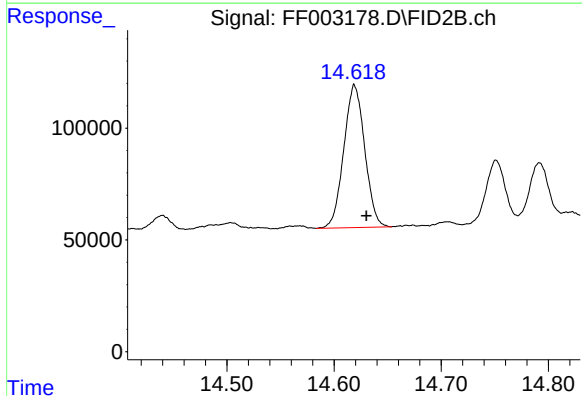


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.619 min
Delta R.T.: -0.011 min
Response: 866706
Conc: 6.52 ug/ml

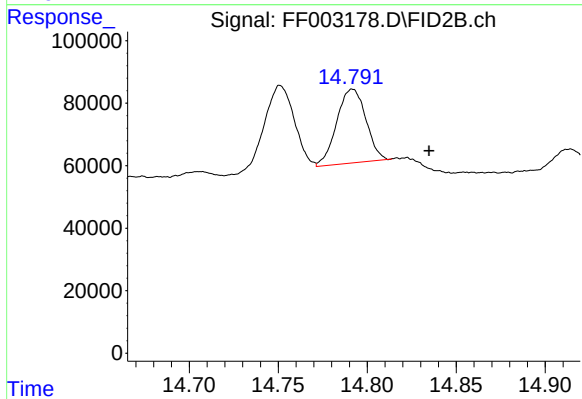


#10 N-TETRACOSANE

R.T.: 14.792 min
Delta R.T.: -0.043 min
Response: 269227
Conc: 1.81 ug/ml

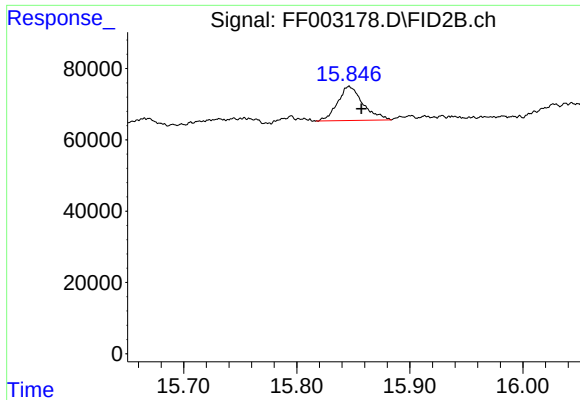


#11 N-HEXACOSANE

R.T.: 15.846 min
Delta R.T.: -0.011 min
Response: 148720
Conc: 1.01 ug/ml

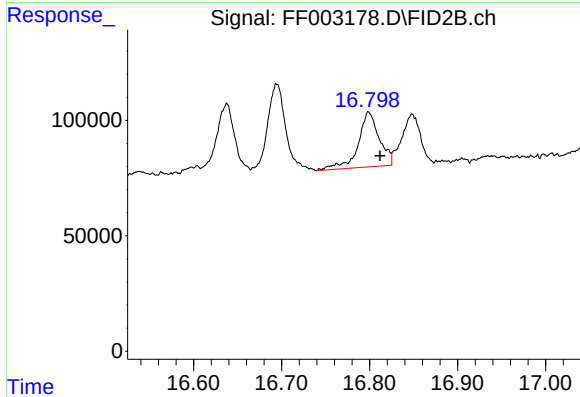


#12 N-OCTACOSANE

R.T.: 16.799 min
Delta R.T.: -0.013 min
Response: 394810
Conc: 2.71 ug/ml

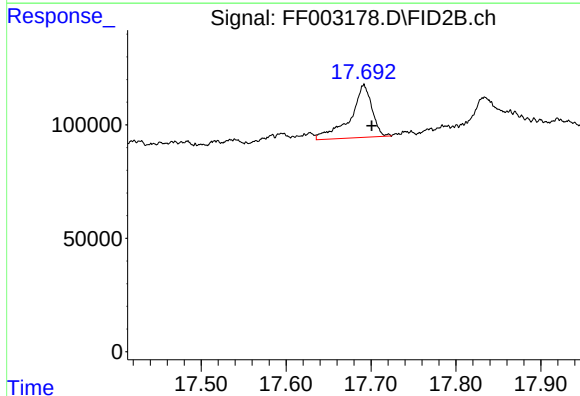


#13 N-TRIACONTANE

R.T.: 17.692 min
Delta R.T.: -0.009 min
Response: 410854
Conc: 2.88 ug/ml

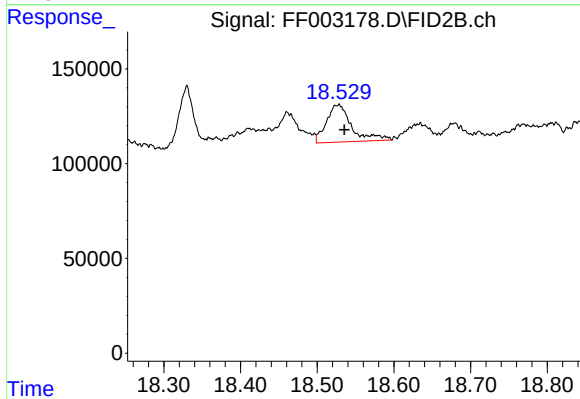


#14 N-DOTRIACONTANE

R.T.: 18.528 min
Delta R.T.: -0.007 min
Response: 447831
Conc: 3.36 ug/ml

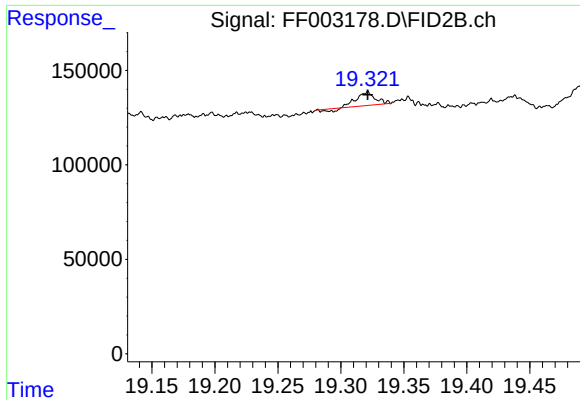


#15 N-TETRATRIACONTANE

R.T.: 19.321 min
Delta R.T.: 0.000 min
Response: 66071
Conc: 0.53 ug/ml

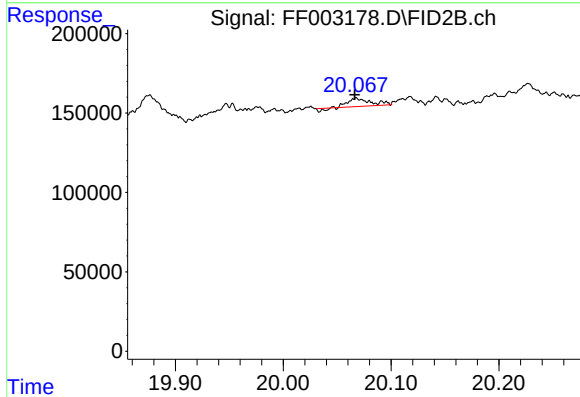


#16 N-HEXATRIACONTANE

R.T.: 20.068 min
Delta R.T.: 0.002 min
Response: 68683
Conc: 0.61 ug/ml

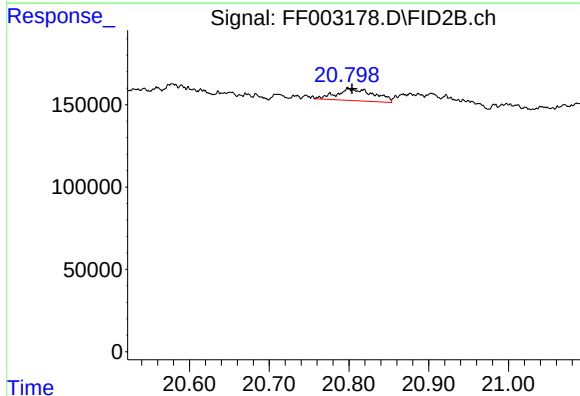

#17 N-OCTATRIACONTANE

R.T.: 20.799 min
Delta R.T.: -0.005 min
Response: 236403
Conc: 2.36 ug/ml

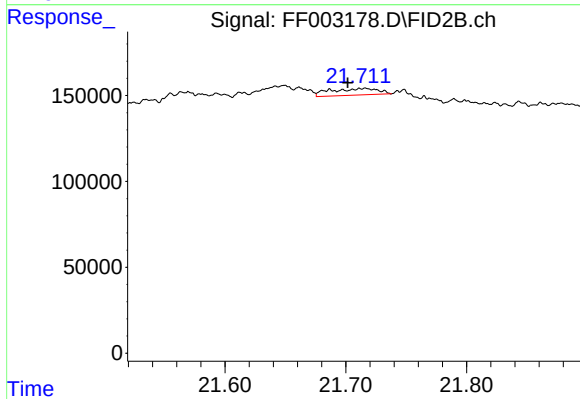

#18 N-TETRACONTANE

R.T.: 21.715 min
Delta R.T.: 0.014 min
Response: 105355
Conc: 1.05 ug/ml