

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010919\
 Data File : FF003180.D
 Signal(s) : FID2B.ch
 Acq On : 09 Jan 2019 17:36
 Operator : AJ\SJ
 Sample : K1087-02
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jan 10 00:24:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
 Quant Title :
 QLast Update : Fri Jan 04 16:10:51 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.619	1411917	10.620 ug/ml
Target Compounds			
4) N-TETRADECANE	8.129	237850	1.560 ug/ml
11) N-HEXACOSANE	15.847	117896	0.801 ug/ml
12) N-OCTACOSANE	16.799	185417	1.274 ug/ml
13) N-TRIACONTANE	17.691	213925	1.498 ug/ml
14) N-DOTRIACONTANE	18.527	495162	3.716 ug/ml
15) N-TETRATRIACONTANE	19.316	75399	0.608 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF010919\
Data File : FF003180.D
Signal(s) : FID2B.ch
Acq On : 09 Jan 2019 17:36
Operator : AJ\SJ
Sample : K1087-02
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jan 10 00:24:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF010419.M
Quant Title :
QLast Update : Fri Jan 04 16:10:51 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

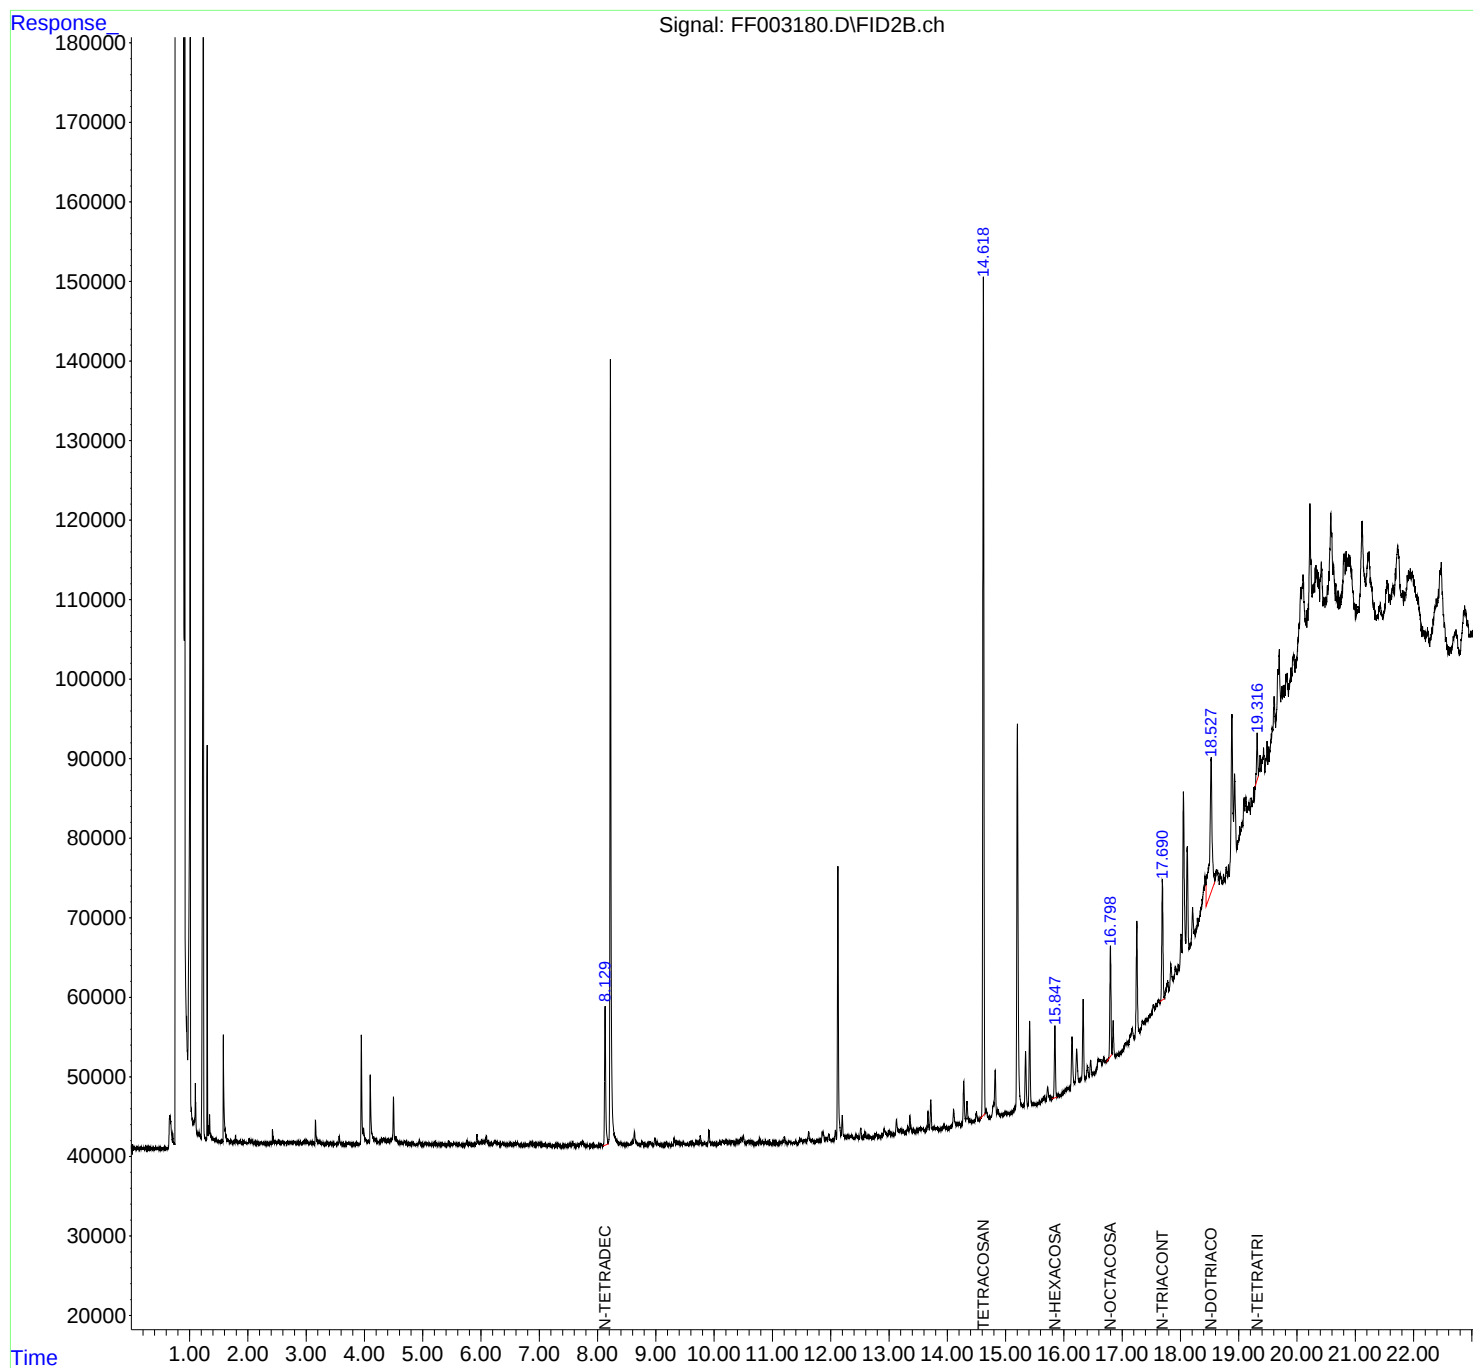

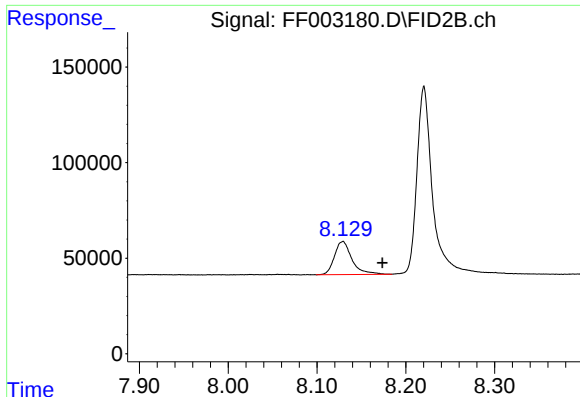


#4 N-TETRADECANE

R.T.: 8.129 min
Delta R.T.: -0.045 min
Response: 237850
Conc: 1.56 ug/ml

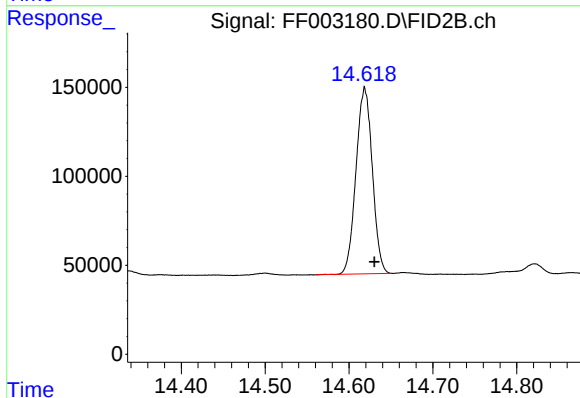


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.619 min
Delta R.T.: -0.012 min
Response: 1411917
Conc: 10.62 ug/ml

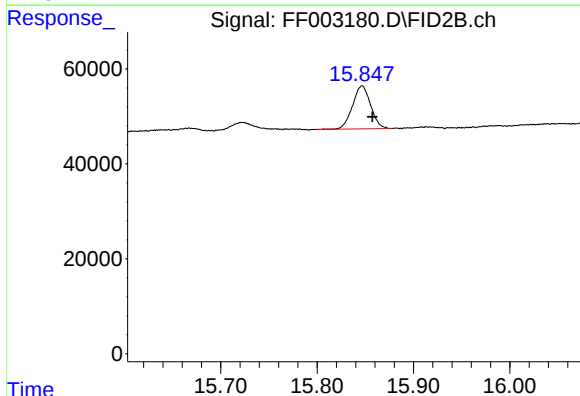


#11 N-HEXACOSANE

R.T.: 15.847 min
Delta R.T.: -0.011 min
Response: 117896
Conc: 0.80 ug/ml

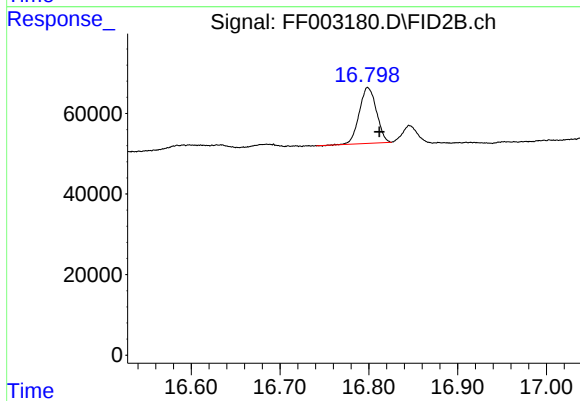


#12 N-OCTACOSANE

R.T.: 16.799 min
Delta R.T.: -0.013 min
Response: 185417
Conc: 1.27 ug/ml

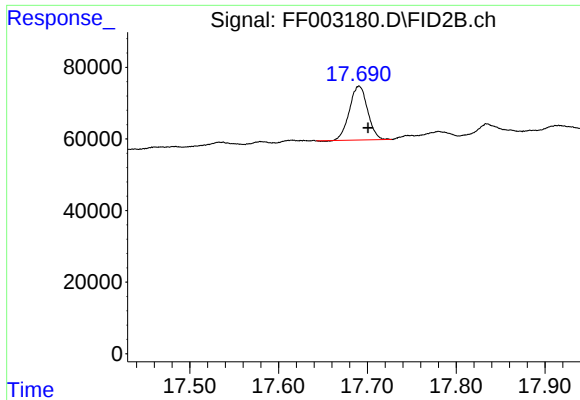


#13 N-TRIACONTANE

R.T.: 17.691 min
Delta R.T.: -0.010 min
Response: 213925
Conc: 1.50 ug/ml

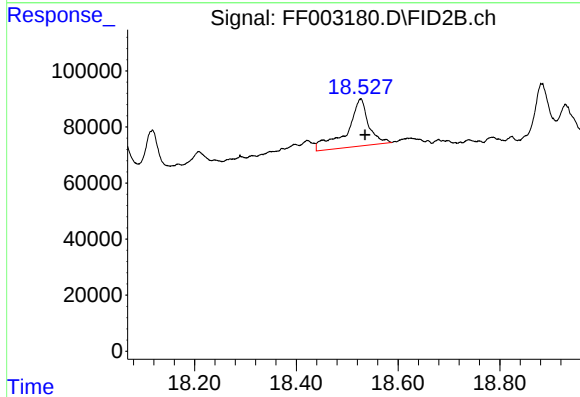

#14 N-DOTRIACONTANE

R.T.: 18.527 min
Delta R.T.: -0.008 min
Response: 495162
Conc: 3.72 ug/ml

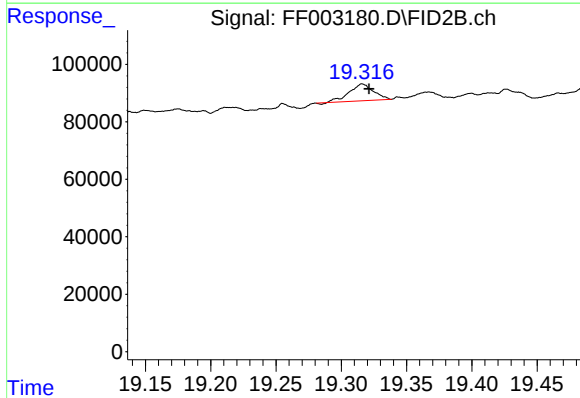

#15 N-TETRATRIACONTANE

R.T.: 19.316 min
Delta R.T.: -0.005 min
Response: 75399
Conc: 0.61 ug/ml