

Data Path : P:\HPCHEM1\FID_F\Data\FF021418\
 Data File : FF000108.D
 Signal(s) : FID2B.ch
 Acq On : 14 Feb 2018 09:46
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 15 08:55:30 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF020118.M
 Quant Title :
 QLast Update : Fri Feb 02 10:05:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.632	6266111	55.016 ug/ml
Target Compounds			
2) N-DECANE	4.384	8879379	57.337 ug/ml
3) N-DODECANE	6.400	8700385	56.333 ug/ml
4) N-TETRADECANE	8.191	8476541	55.512 ug/ml
5) N-HEXADECANE	9.789	8135757	55.317 ug/ml
6) N-OCTADECANE	11.228	7880039	54.164 ug/ml
7) N-EICOSANE	12.537	7491972	54.857 ug/ml
8) N-DOCOSANE	13.734	7178578	55.080 ug/ml
10) N-TETRACOSANE	14.835	6890491	54.375 ug/ml
11) N-HEXACOSANE	15.856	6540817	53.939 ug/ml
12) N-OCTACOSANE	16.804	6236503	53.690 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_F\Data\FF021418\
Data File : FF000108.D
Signal(s) : FID2B.ch
Acq On : 14 Feb 2018 09:46
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 15 08:55:30 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF020118.M
Quant Title :
QLast Update : Fri Feb 02 10:05:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

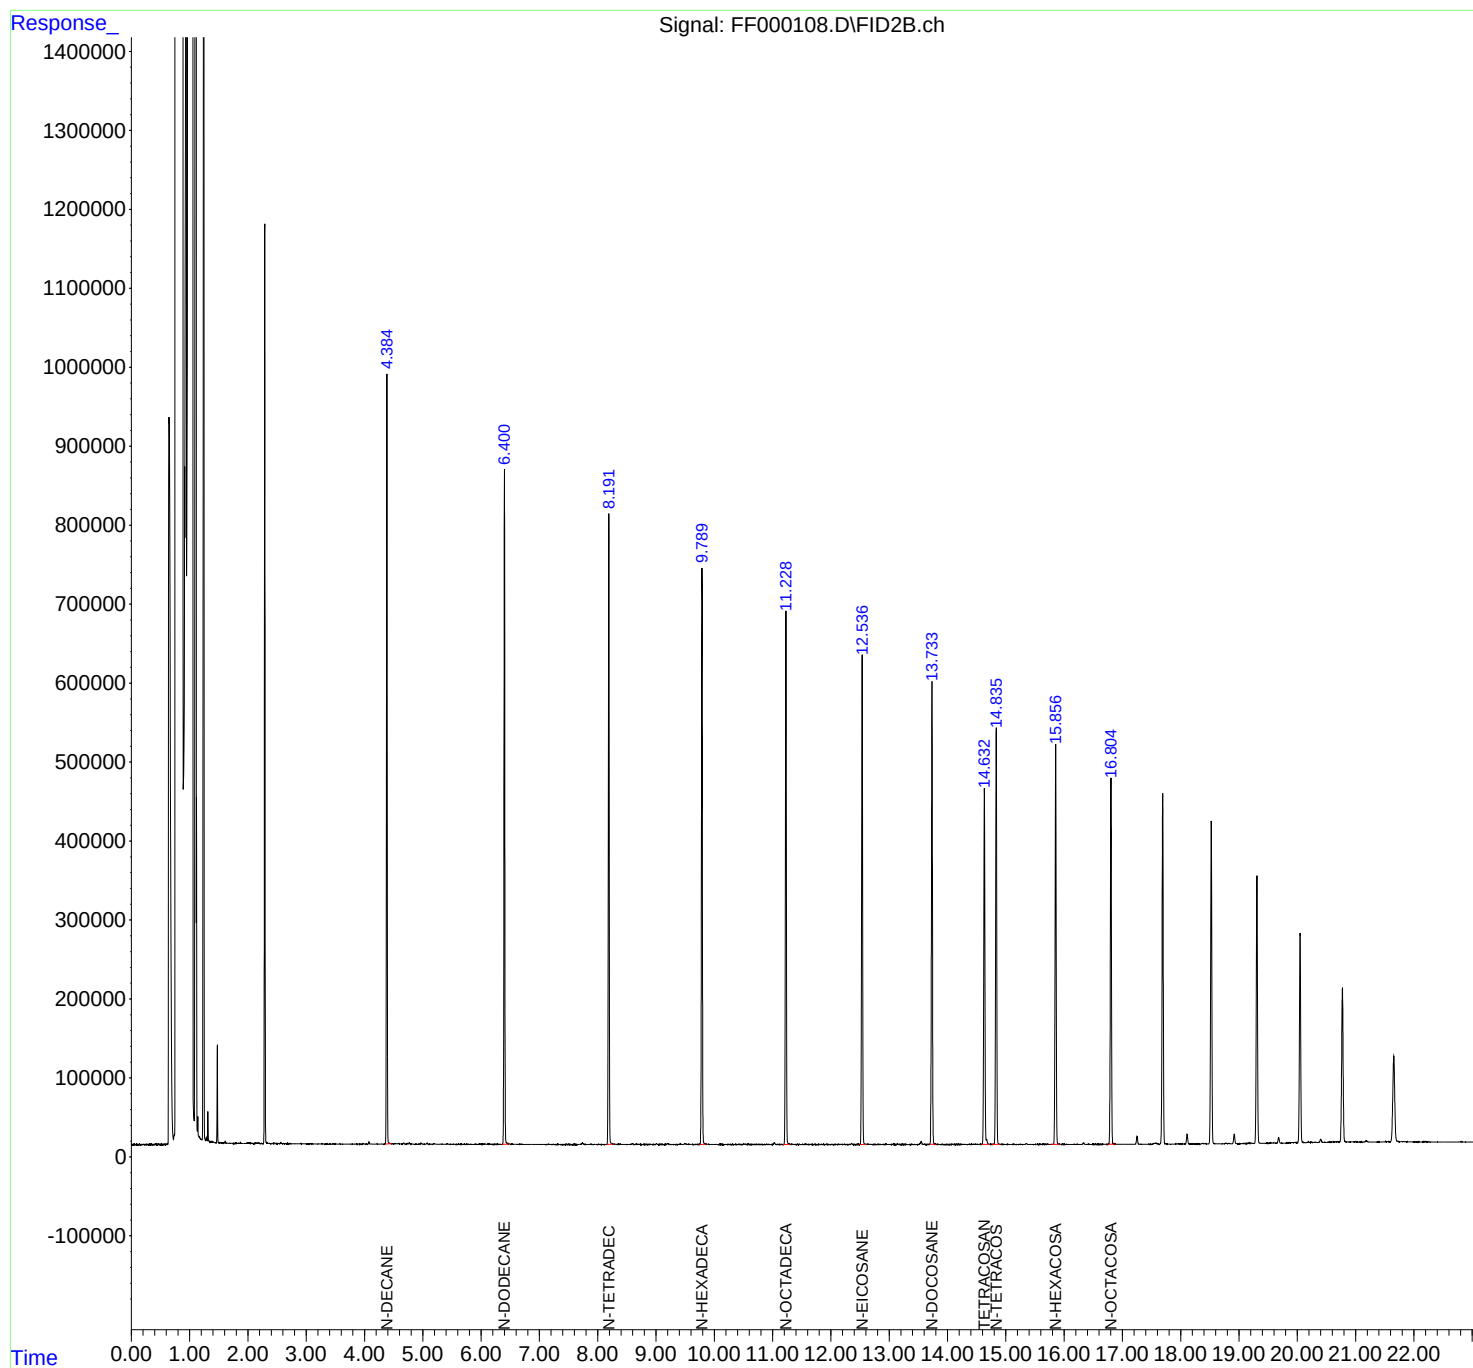

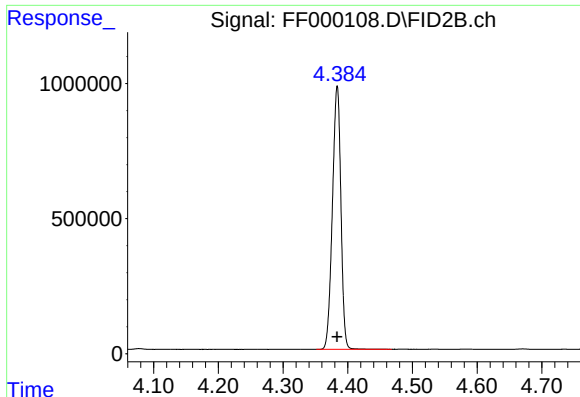


#2 N-DECANE

R.T.: 4.384 min
Delta R.T.: 0.000 min
Response: 8879379
Conc: 57.34 ug/ml

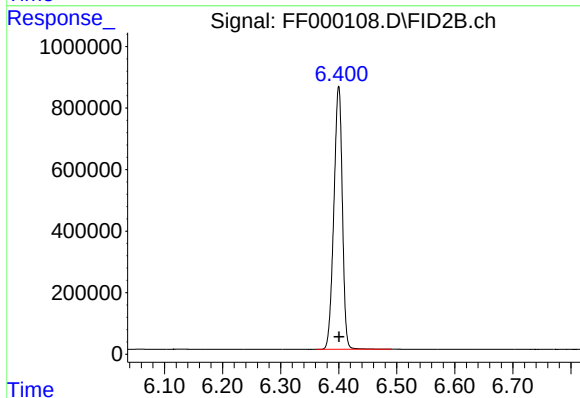


#3 N-DODECANE

R.T.: 6.400 min
Delta R.T.: 0.000 min
Response: 8700385
Conc: 56.33 ug/ml

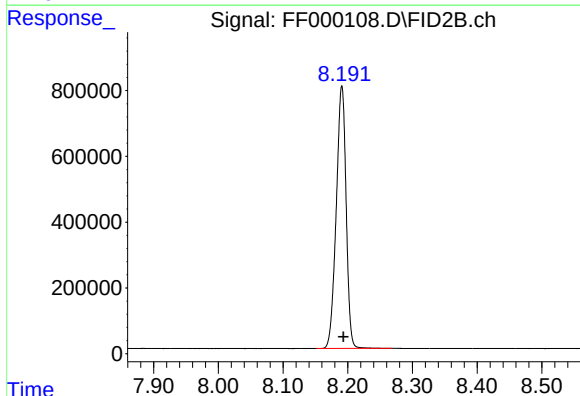


#4 N-TETRADECANE

R.T.: 8.191 min
Delta R.T.: -0.003 min
Response: 8476541
Conc: 55.51 ug/ml

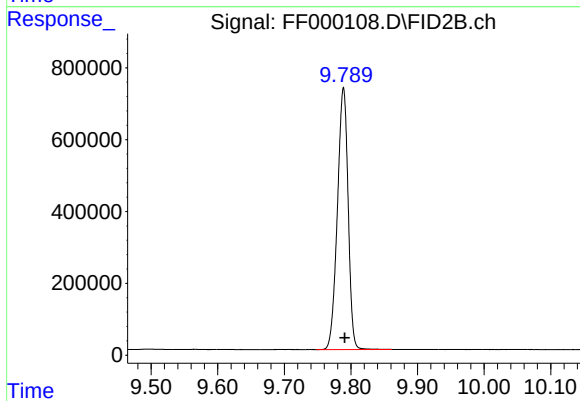


#5 N-HEXADECANE

R.T.: 9.789 min
Delta R.T.: -0.002 min
Response: 8135757
Conc: 55.32 ug/ml

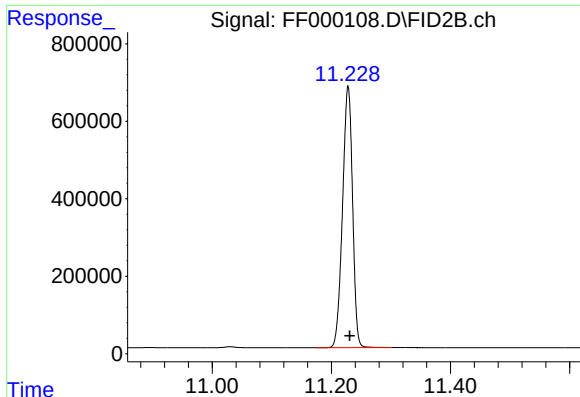


#6 N-OCTADECANE

R.T.: 11.228 min
Delta R.T.: -0.003 min
Response: 7880039
Conc: 54.16 ug/ml

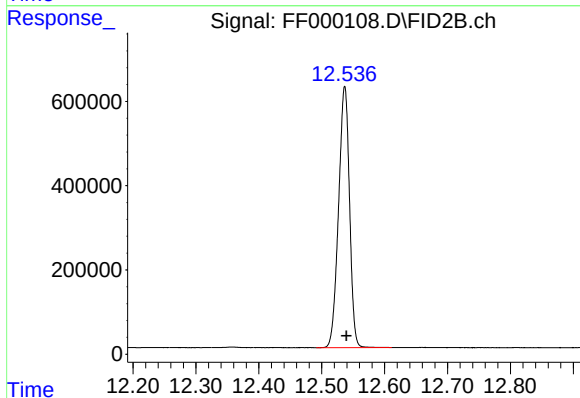


#7 N-EICOSANE

R.T.: 12.537 min
Delta R.T.: -0.003 min
Response: 7491972
Conc: 54.86 ug/ml

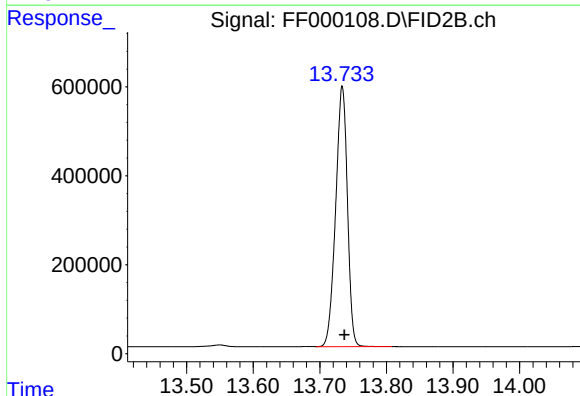


#8 N-DOCOSANE

R.T.: 13.734 min
Delta R.T.: -0.003 min
Response: 7178578
Conc: 55.08 ug/ml

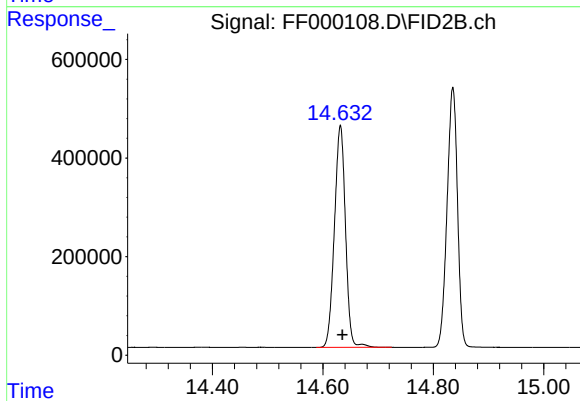


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.632 min
Delta R.T.: -0.004 min
Response: 6266111
Conc: 55.02 ug/ml

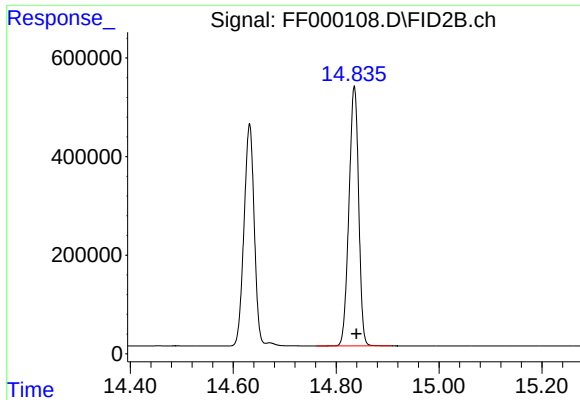


#10 N-TETRACOSANE

R.T.: 14.835 min
Delta R.T.: -0.004 min
Response: 6890491
Conc: 54.38 ug/ml

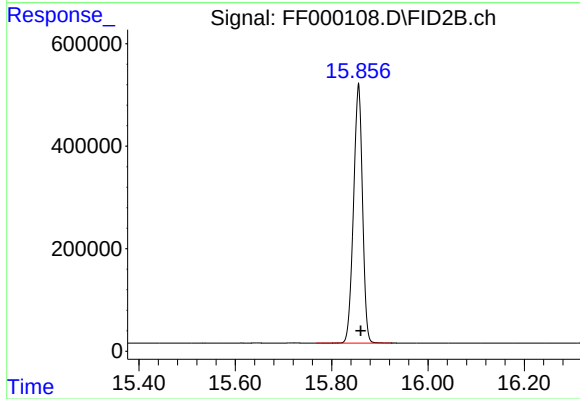

#11 N-HEXACOSANE

R.T.: 15.856 min
Delta R.T.: -0.005 min
Response: 6540817
Conc: 53.94 ug/ml

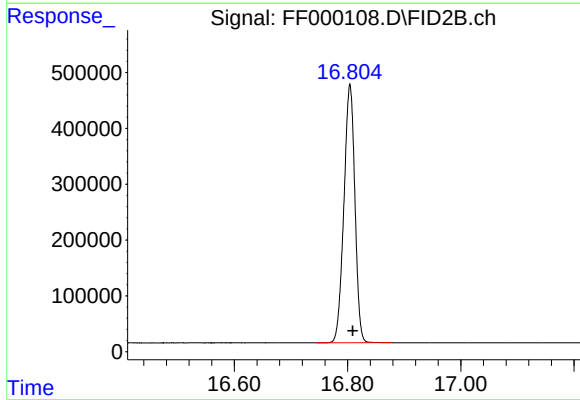

#12 N-OCTACOSANE

R.T.: 16.804 min
Delta R.T.: -0.005 min
Response: 6236503
Conc: 53.69 ug/ml