

Data Path : P:\HPCHEM1\FID_F\Data\FF021518\
 Data File : FF000140.D
 Signal(s) : FID2B.ch
 Acq On : 16 Feb 2018 00:11
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 16 07:50:48 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF020118.M
 Quant Title :
 QLast Update : Fri Feb 02 10:05:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.633	4920106	43.198 ug/mlm
Target Compounds			
2) N-DECANE	4.385	7226392	46.664 ug/ml
3) N-DODECANE	6.401	6931808	44.882 ug/ml
4) N-TETRADECANE	8.192	6626944	43.399 ug/ml
5) N-HEXADECANE	9.789	6257061	42.543 ug/ml
6) N-OCTADECANE	11.228	5991882	41.186 ug/ml
7) N-EICOSANE	12.537	5697088	41.714 ug/ml
8) N-DOCOSANE	13.734	5558784	42.652 ug/ml
10) N-TETRACOSANE	14.837	5506299	43.452 ug/ml
11) N-HEXACOSANE	15.857	5545189	45.729 ug/ml
12) N-OCTACOSANE	16.807	5637876	48.537 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_F\Data\FF021518\
Data File : FF000140.D
Signal(s) : FID2B.ch
Acq On : 16 Feb 2018 00:11
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 16 07:50:48 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF020118.M
Quant Title :
QLast Update : Fri Feb 02 10:05:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

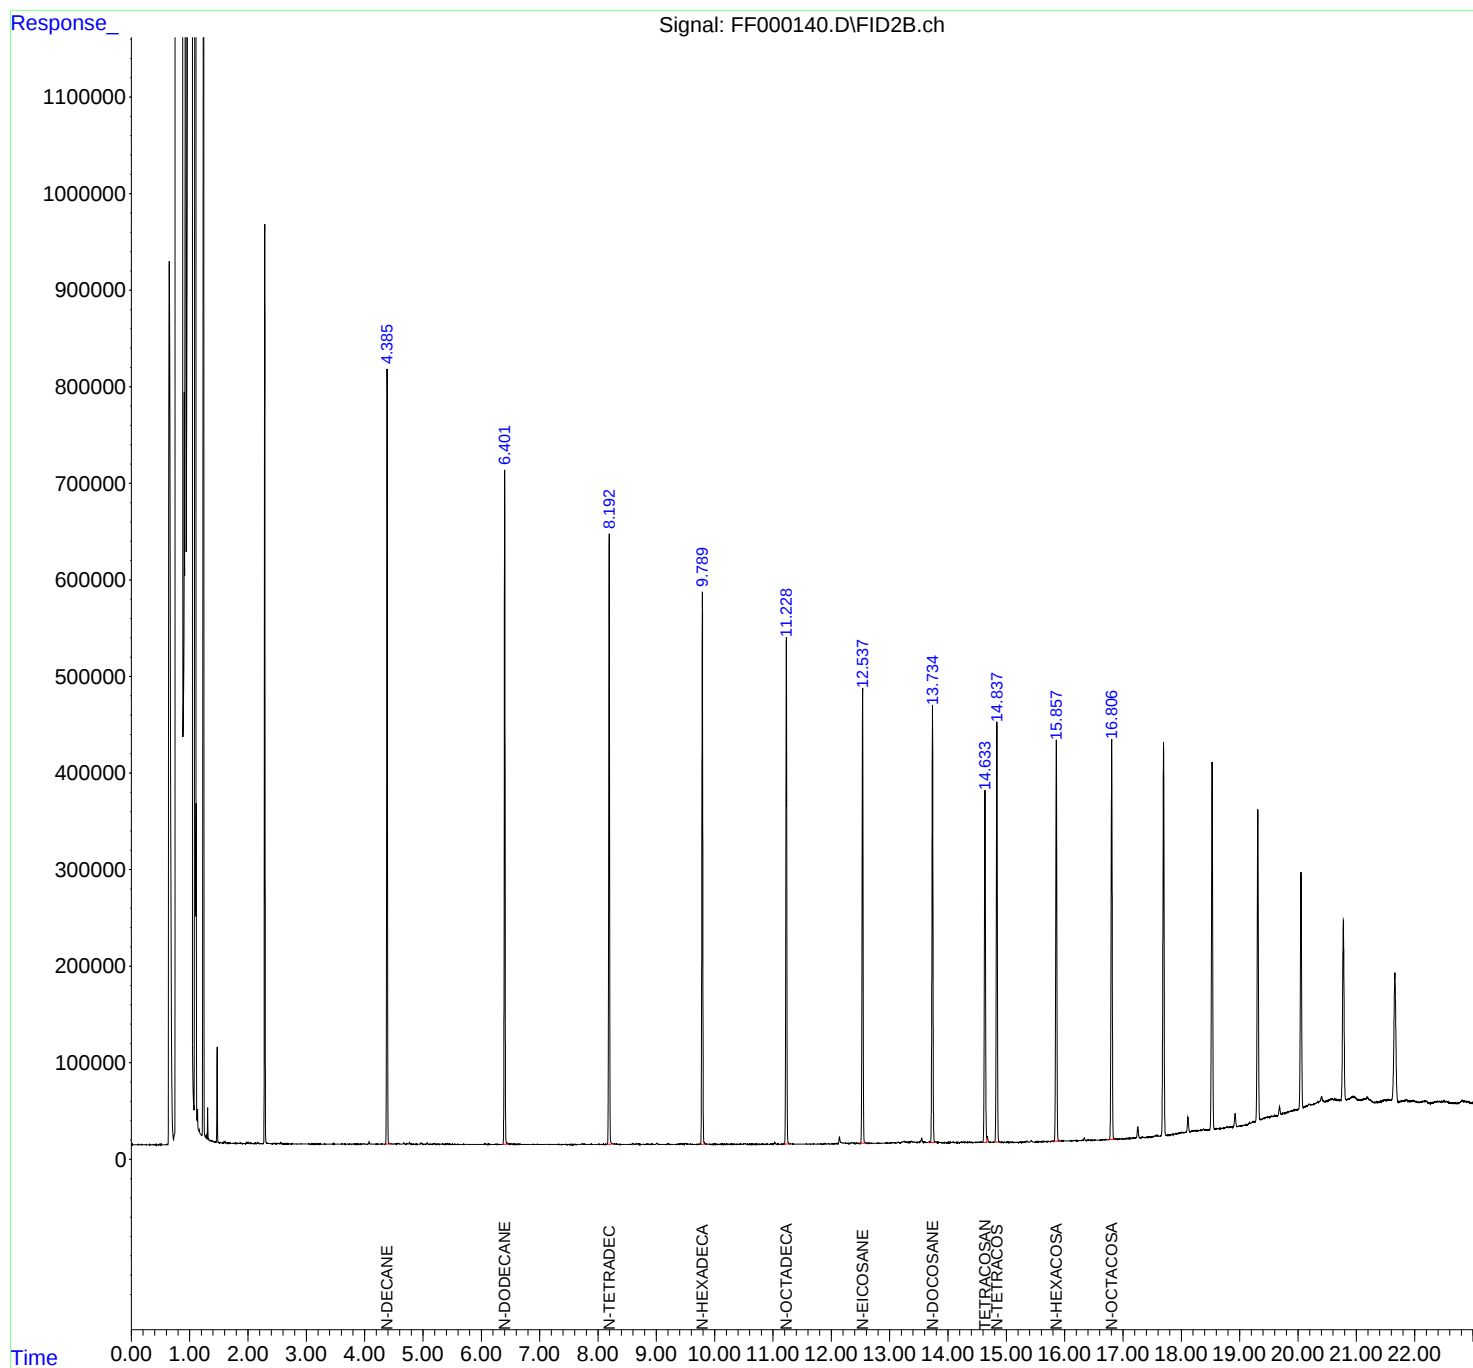

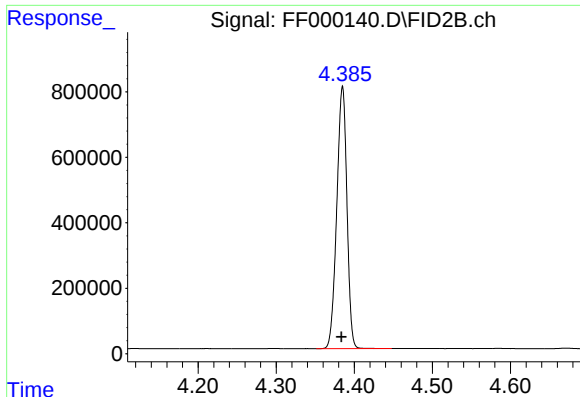


#2 N-DECANE

R.T.: 4.385 min
Delta R.T.: 0.001 min
Response: 7226392
Conc: 46.66 ug/ml

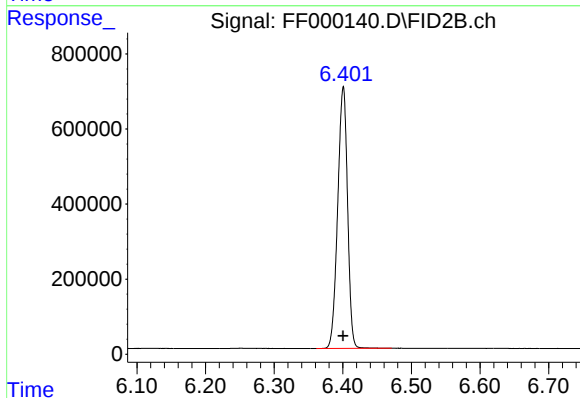


#3 N-DODECANE

R.T.: 6.401 min
Delta R.T.: 0.000 min
Response: 6931808
Conc: 44.88 ug/ml

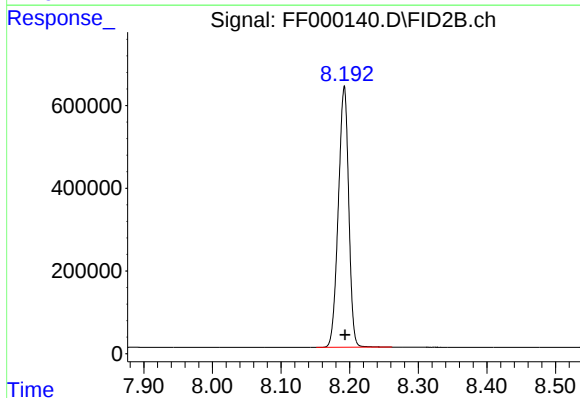


#4 N-TETRADECANE

R.T.: 8.192 min
Delta R.T.: -0.002 min
Response: 6626944
Conc: 43.40 ug/ml

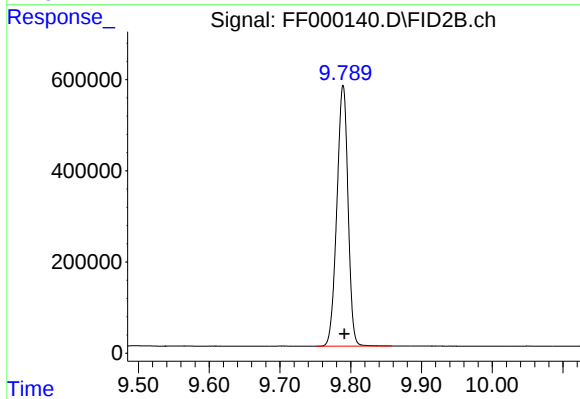


#5 N-HEXADECANE

R.T.: 9.789 min
Delta R.T.: -0.002 min
Response: 6257061
Conc: 42.54 ug/ml

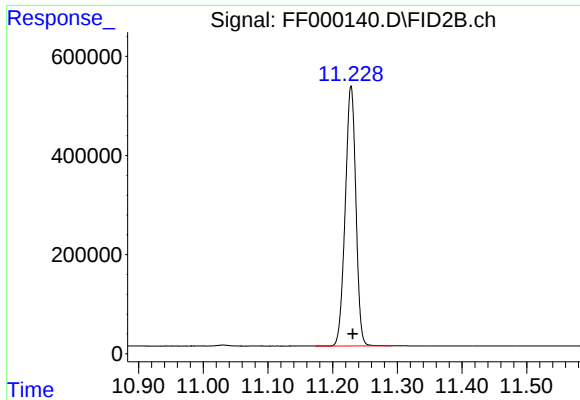


#6 N-OCTADECANE

R.T.: 11.228 min
Delta R.T.: -0.003 min
Response: 5991882
Conc: 41.19 ug/ml

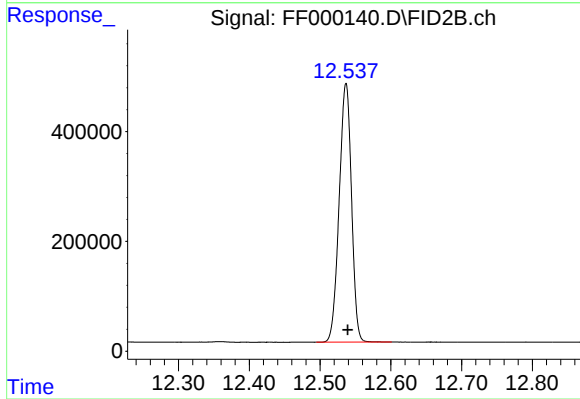


#7 N-EICOSANE

R.T.: 12.537 min
Delta R.T.: -0.003 min
Response: 5697088
Conc: 41.71 ug/ml

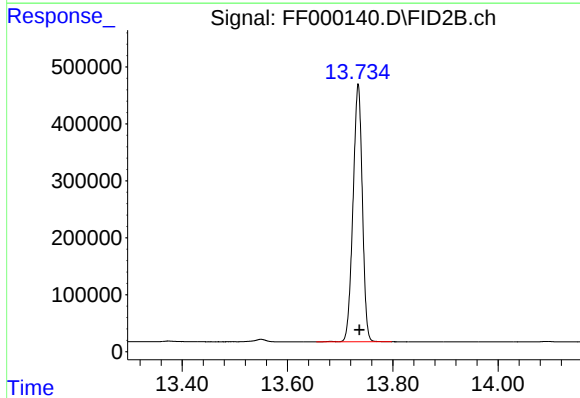


#8 N-DOCOSANE

R.T.: 13.734 min
Delta R.T.: -0.003 min
Response: 5558784
Conc: 42.65 ug/ml

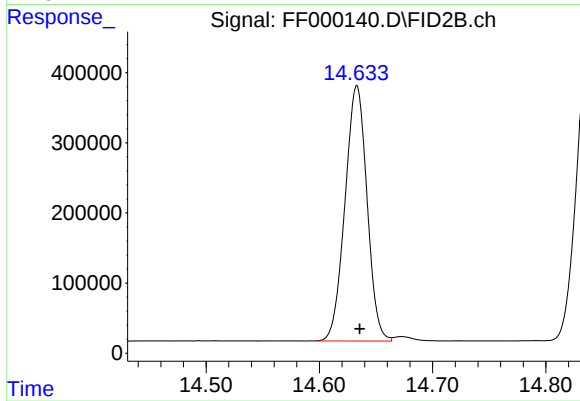


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.633 min
Delta R.T.: -0.003 min
Response: 4920106
Conc: 43.20 ug/ml m

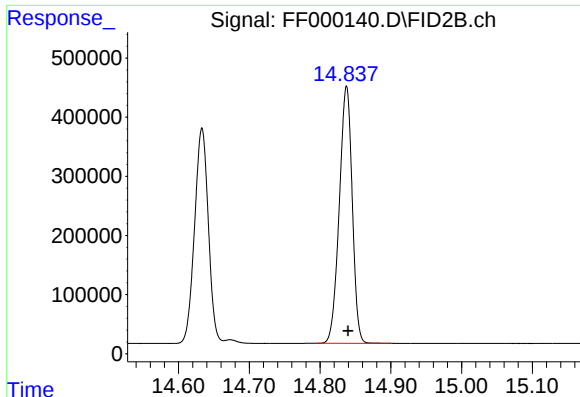


#10 N-TETRACOSANE

R.T.: 14.837 min
Delta R.T.: -0.002 min
Response: 5506299
Conc: 43.45 ug/ml

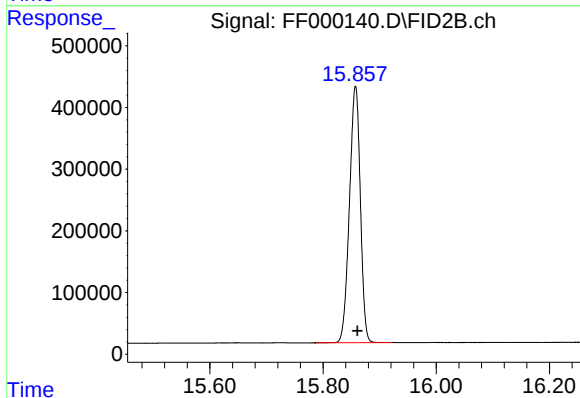

#11 N-HEXACOSANE

R.T.: 15.857 min
Delta R.T.: -0.003 min
Response: 5545189
Conc: 45.73 ug/ml

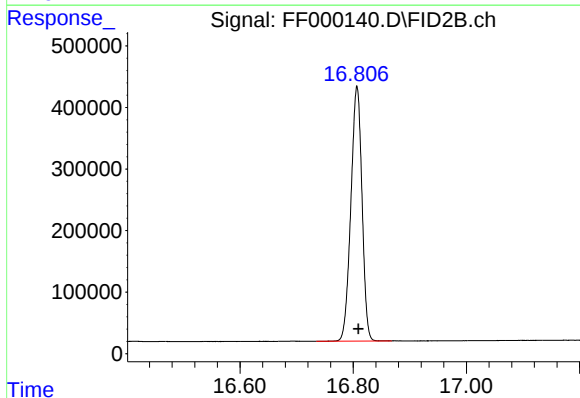

#12 N-OCTACOSANE

R.T.: 16.807 min
Delta R.T.: -0.002 min
Response: 5637876
Conc: 48.54 ug/ml