

Data Path : P:\HPCHEM1\FID_F\Data\FF022018\
 Data File : FF000179.D
 Signal(s) : FID2B.ch
 Acq On : 20 Feb 2018 17:02
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 21 04:21:15 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF020118.M
 Quant Title :
 QLast Update : Fri Feb 02 10:05:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.636	6389543	56.100 ug/ml
Target Compounds			
2) N-DECANE	4.384	8016049	51.763 ug/ml
3) N-DODECANE	6.401	7739667	50.113 ug/ml
4) N-TETRADECANE	8.193	7425968	48.632 ug/ml
5) N-HEXADECANE	9.791	7055037	47.969 ug/ml
6) N-OCTADECANE	11.231	6797561	46.723 ug/ml
7) N-EICOSANE	12.539	6478919	47.439 ug/ml
8) N-DOCOSANE	13.736	6306155	48.386 ug/ml
10) N-TETRACOSANE	14.839	6232472	49.183 ug/ml
11) N-HEXACOSANE	15.859	6204522	51.166 ug/ml
12) N-OCTACOSANE	16.808	6200570	53.381 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_F\Data\FF022018\
Data File : FF000179.D
Signal(s) : FID2B.ch
Acq On : 20 Feb 2018 17:02
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 21 04:21:15 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF020118.M
Quant Title :
QLast Update : Fri Feb 02 10:05:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

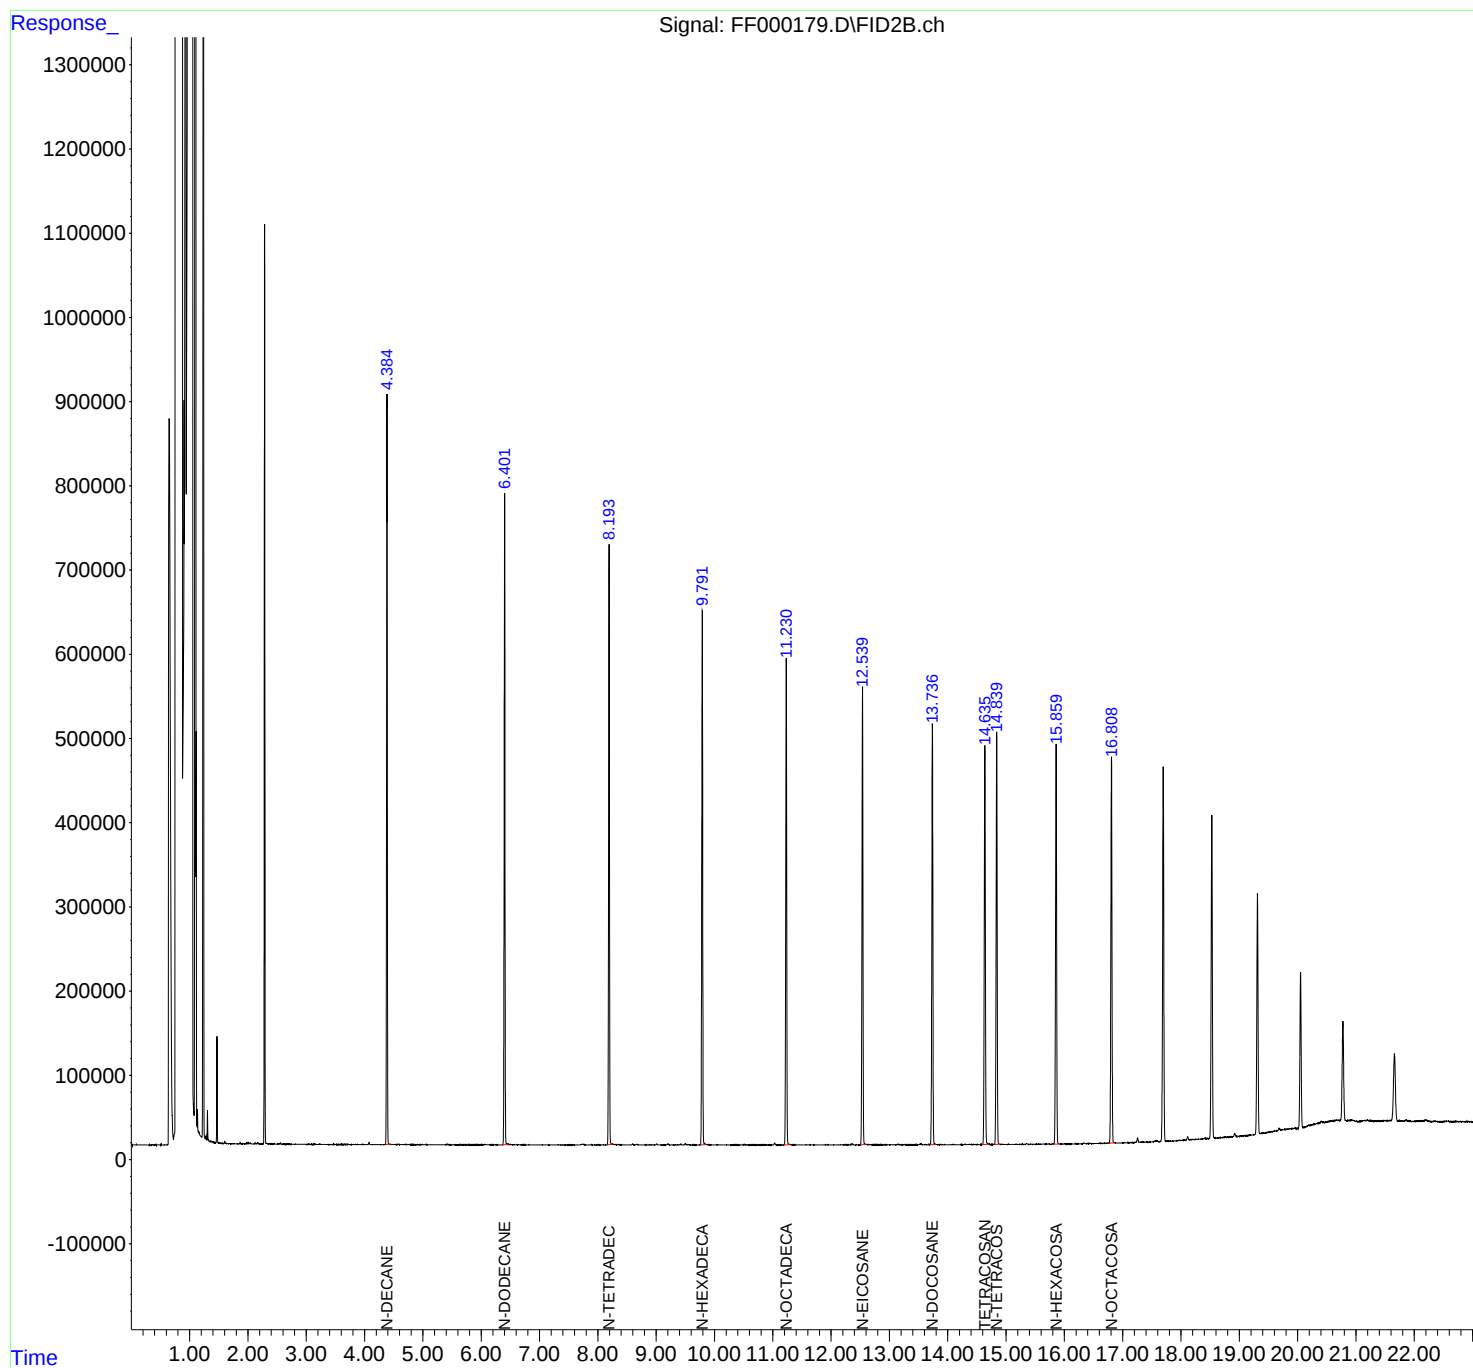

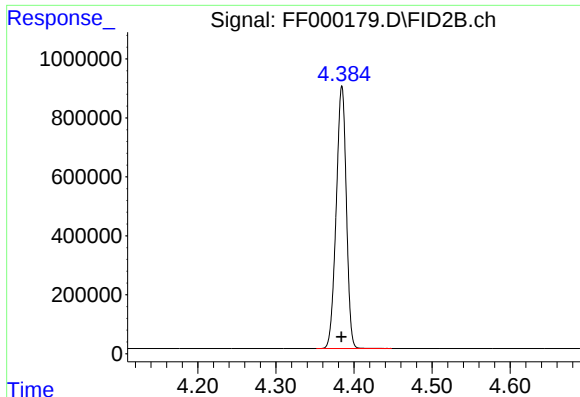


#2 N-DECANE

R.T.: 4.384 min
Delta R.T.: 0.000 min
Response: 8016049
Conc: 51.76 ug/ml

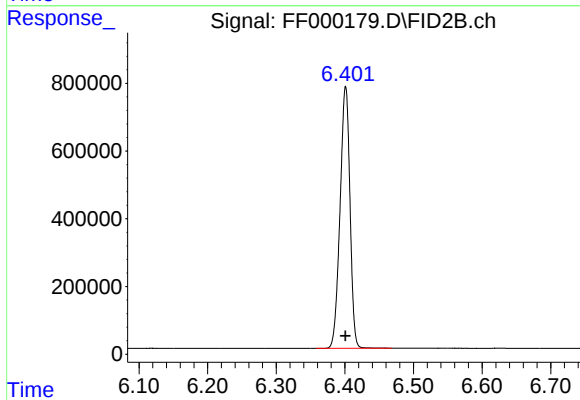


#3 N-DODECANE

R.T.: 6.401 min
Delta R.T.: 0.000 min
Response: 7739667
Conc: 50.11 ug/ml

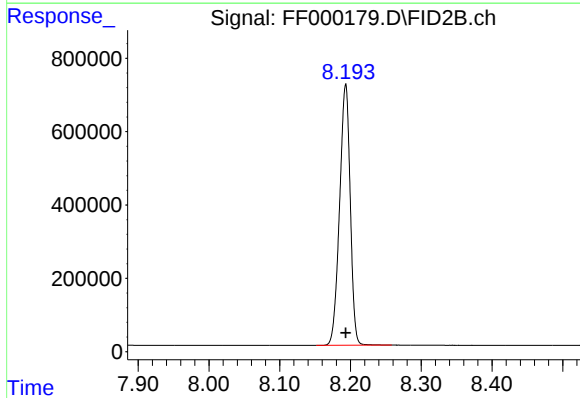


#4 N-TETRADECANE

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 7425968
Conc: 48.63 ug/ml

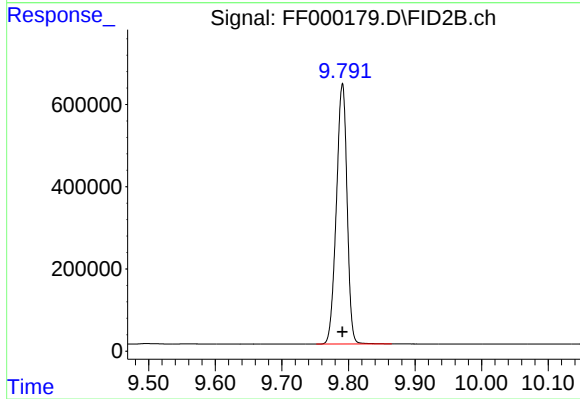


#5 N-HEXADECANE

R.T.: 9.791 min
Delta R.T.: 0.000 min
Response: 7055037
Conc: 47.97 ug/ml

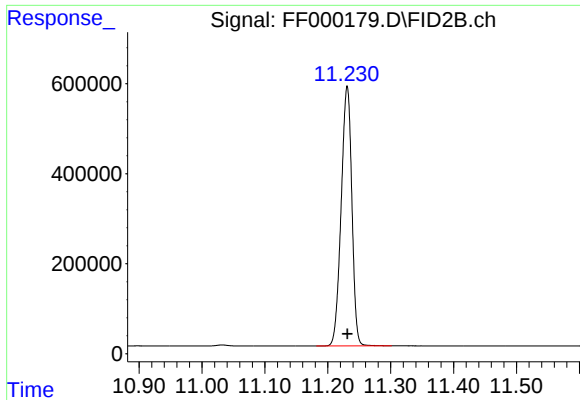


#6 N-OCTADECANE

R.T.: 11.231 min
Delta R.T.: 0.000 min
Response: 6797561
Conc: 46.72 ug/ml

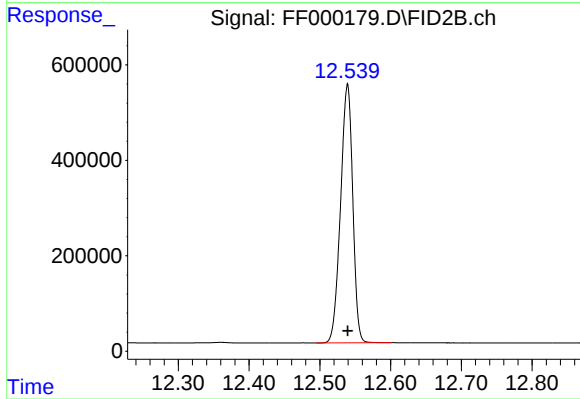


#7 N-EICOSANE

R.T.: 12.539 min
Delta R.T.: 0.000 min
Response: 6478919
Conc: 47.44 ug/ml

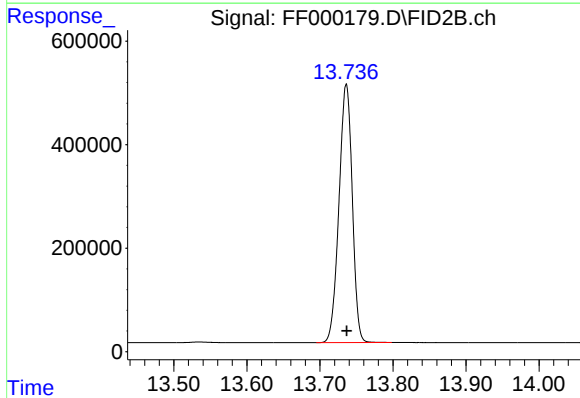


#8 N-DOCOSANE

R.T.: 13.736 min
Delta R.T.: 0.000 min
Response: 6306155
Conc: 48.39 ug/ml

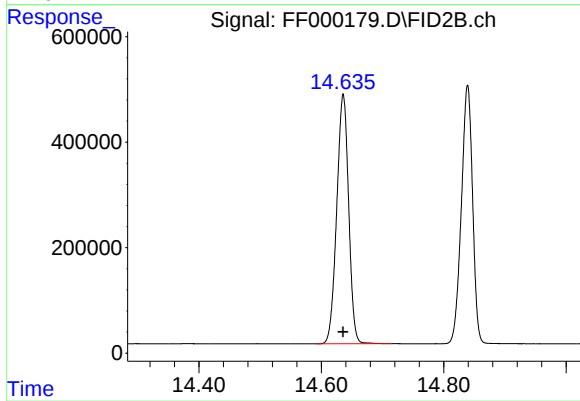


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.636 min
Delta R.T.: 0.000 min
Response: 6389543
Conc: 56.10 ug/ml

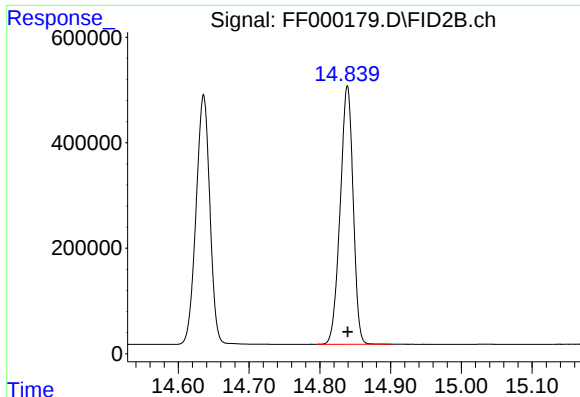


#10 N-TETRACOSANE

R.T.: 14.839 min
Delta R.T.: 0.000 min
Response: 6232472
Conc: 49.18 ug/ml

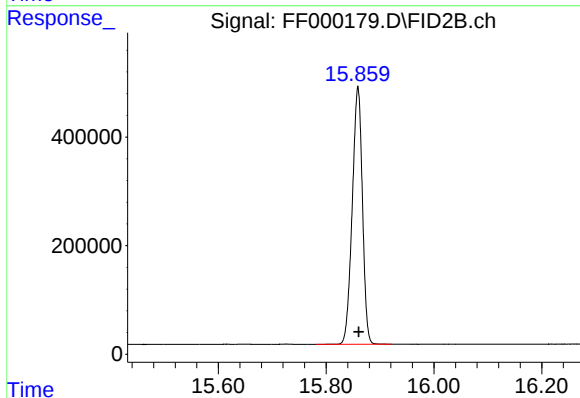

#11 N-HEXACOSANE

R.T.: 15.859 min
Delta R.T.: -0.002 min
Response: 6204522
Conc: 51.17 ug/ml

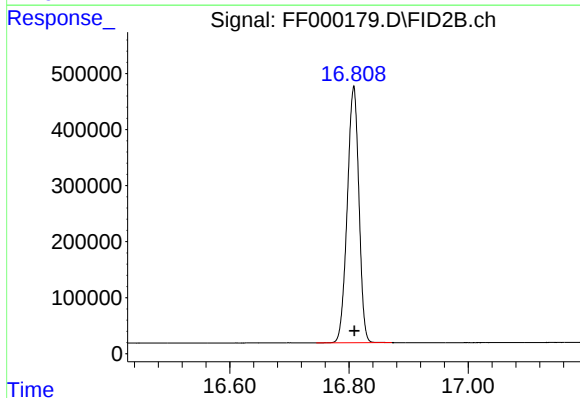

#12 N-OCTACOSANE

R.T.: 16.808 min
Delta R.T.: -0.001 min
Response: 6200570
Conc: 53.38 ug/ml