

Data Path : P:\HPCHEM1\FID_F\Data\FF022318\
 Data File : FF000225.D
 Signal(s) : FID2B.ch
 Acq On : 23 Feb 2018 18:18
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Feb 24 04:34:08 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF020118.M
 Quant Title :
 QLast Update : Fri Feb 02 10:05:00 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.637	5902207	51.821 ug/ml
Target Compounds			
2) N-DECANE	4.385	7560476	48.821 ug/ml
3) N-DODECANE	6.401	7125571	46.137 ug/ml
4) N-TETRADECANE	8.193	6722102	44.022 ug/ml
5) N-HEXADECANE	9.791	6315555	42.941 ug/ml
6) N-OCTADECANE	11.231	6071635	41.734 ug/ml
7) N-EICOSANE	12.539	5819922	42.614 ug/ml
8) N-DOCOSANE	13.738	5730369	43.968 ug/ml
10) N-TETRACOSANE	14.840	5776056	45.581 ug/ml
11) N-HEXACOSANE	15.861	5853139	48.268 ug/ml
12) N-OCTACOSANE	16.810	5943611	51.169 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_F\Data\FF022318\
Data File : FF000225.D
Signal(s) : FID2B.ch
Acq On : 23 Feb 2018 18:18
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Feb 24 04:34:08 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF020118.M
Quant Title :
QLast Update : Fri Feb 02 10:05:00 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

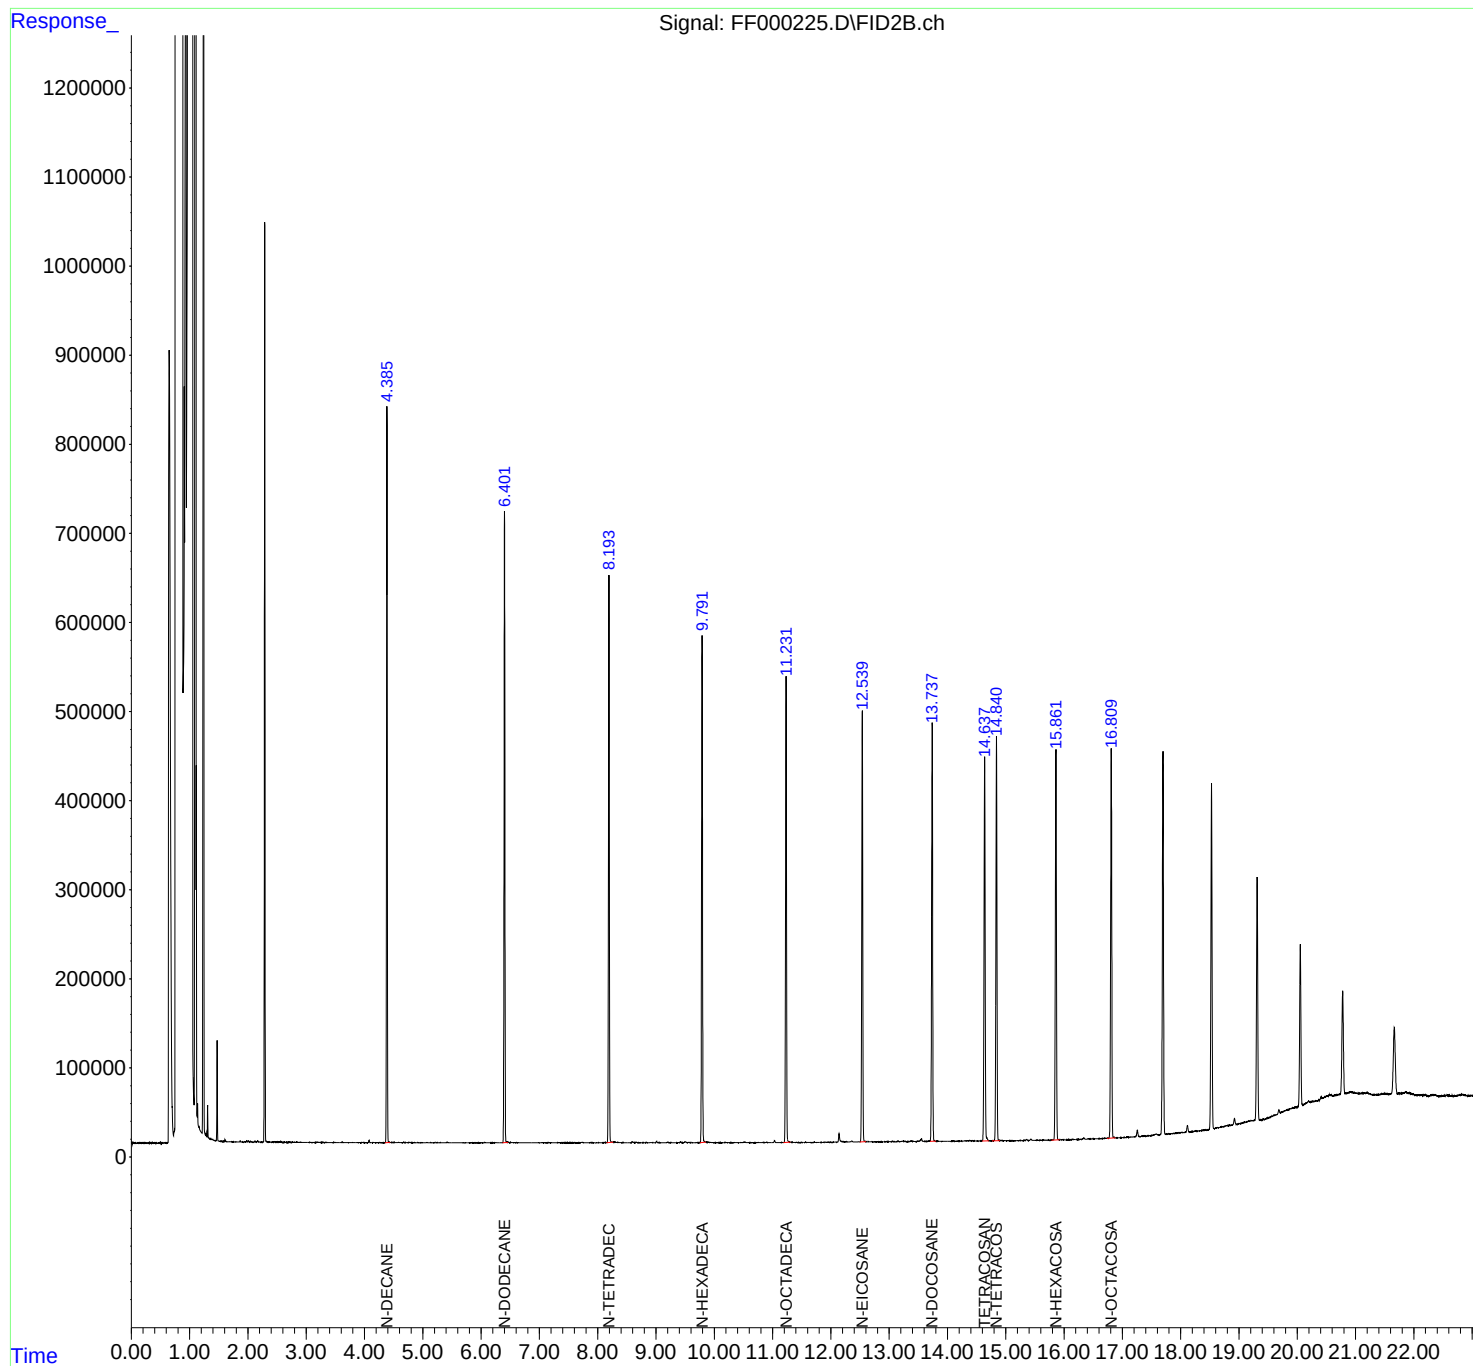

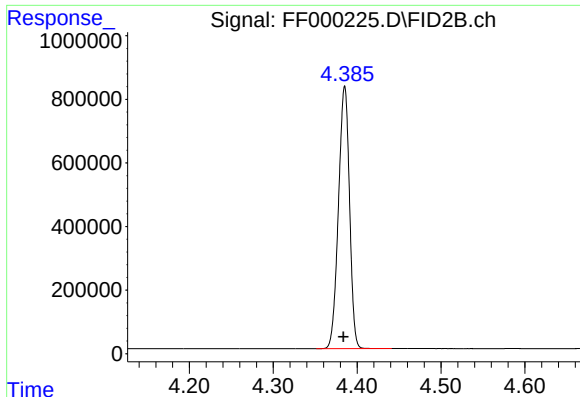


#2 N-DECANE

R.T.: 4.385 min
Delta R.T.: 0.001 min
Response: 7560476
Conc: 48.82 ug/ml

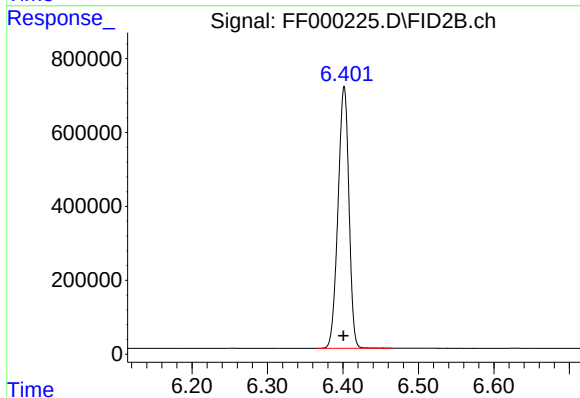


#3 N-DODECANE

R.T.: 6.401 min
Delta R.T.: 0.000 min
Response: 7125571
Conc: 46.14 ug/ml

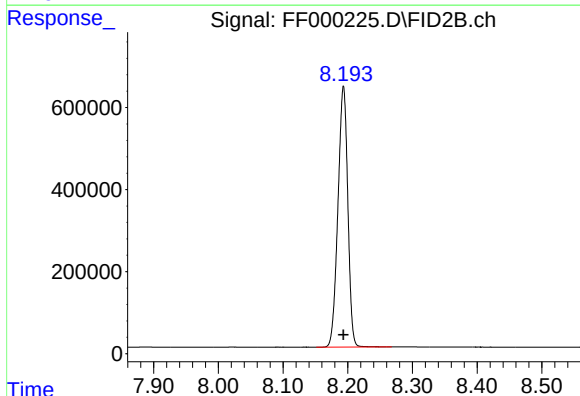


#4 N-TETRADECANE

R.T.: 8.193 min
Delta R.T.: 0.000 min
Response: 6722102
Conc: 44.02 ug/ml

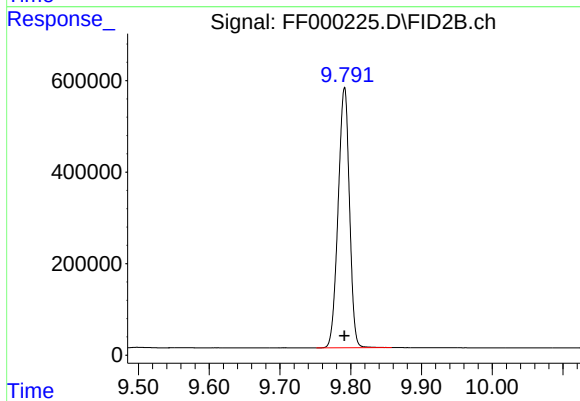


#5 N-HEXADECANE

R.T.: 9.791 min
Delta R.T.: 0.000 min
Response: 6315555
Conc: 42.94 ug/ml

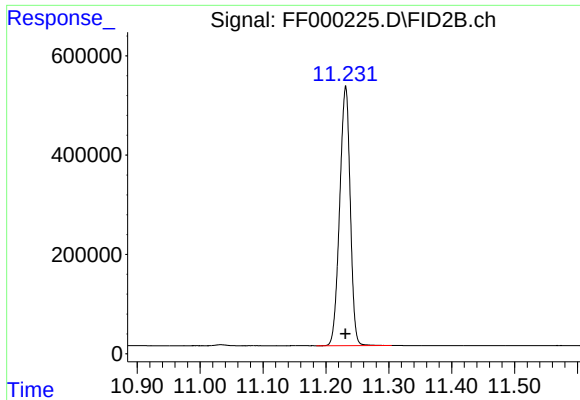


#6 N-OCTADECANE

R.T.: 11.231 min
Delta R.T.: 0.000 min
Response: 6071635
Conc: 41.73 ug/ml

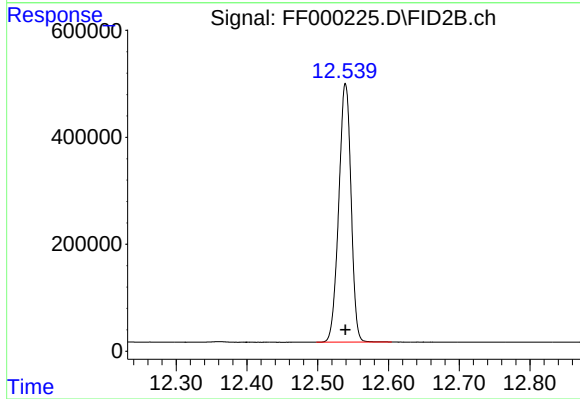


#7 N-EICOSANE

R.T.: 12.539 min
Delta R.T.: 0.000 min
Response: 5819922
Conc: 42.61 ug/ml

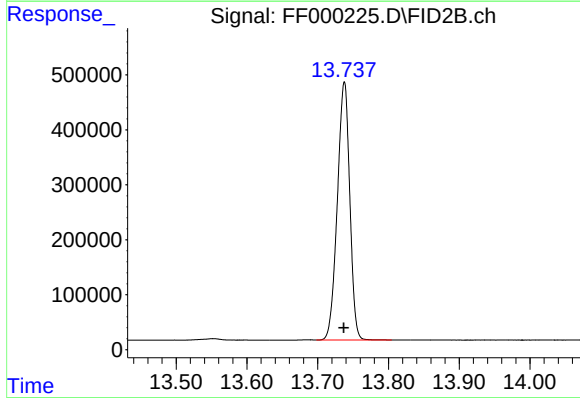


#8 N-DOCOSANE

R.T.: 13.738 min
Delta R.T.: 0.000 min
Response: 5730369
Conc: 43.97 ug/ml

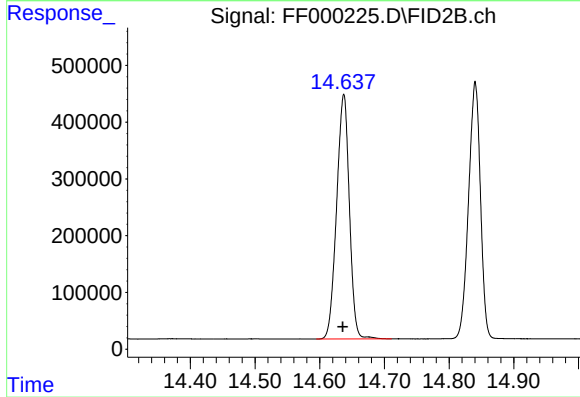


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.637 min
Delta R.T.: 0.001 min
Response: 5902207
Conc: 51.82 ug/ml

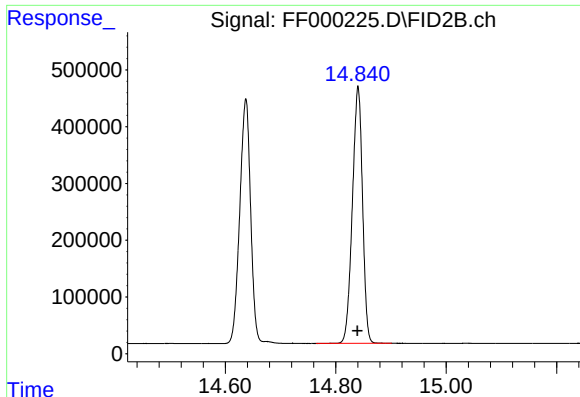


#10 N-TETRACOSANE

R.T.: 14.840 min
Delta R.T.: 0.000 min
Response: 5776056
Conc: 45.58 ug/ml

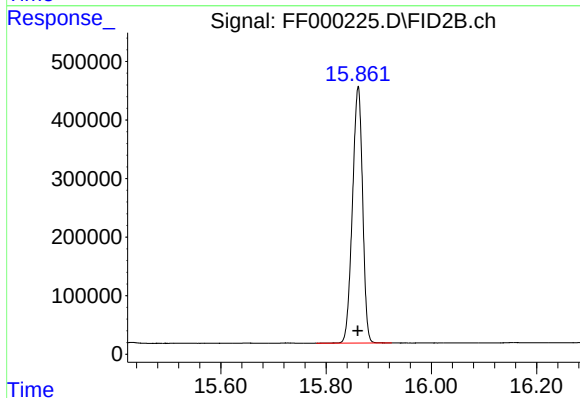

#11 N-HEXACOSANE

R.T.: 15.861 min
Delta R.T.: 0.000 min
Response: 5853139
Conc: 48.27 ug/ml

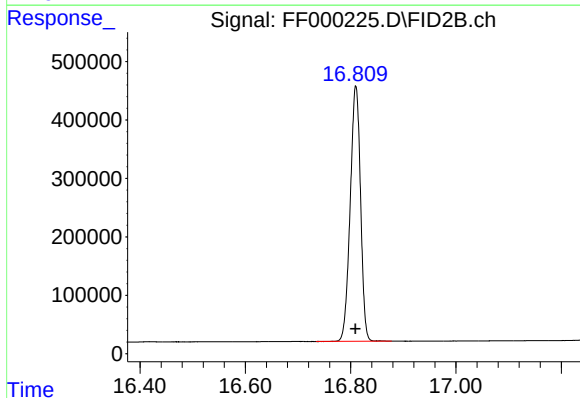

#12 N-OCTACOSANE

R.T.: 16.810 min
Delta R.T.: 0.000 min
Response: 5943611
Conc: 51.17 ug/ml