

Data Path : P:\HPCHEM1\FID_F\Data\FF031518\
 Data File : FF000278.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2018 08:12
 Operator : UA\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 15 11:56:41 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF031518.M
 Quant Title :
 QLast Update : Thu Mar 15 11:28:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.603	46019	0.402 ug/ml
Target Compounds			
6) N-OCTADECANE	11.161f	1061291	8.369 ug/ml
7) N-EICOSANE	12.513	219124	1.706 ug/ml
8) N-DOCOSANE	13.740	64690	0.502 ug/ml
13) N-TRIACONTANE	17.679	82732	0.939 ug/ml
15) N-TETRATRIACONTANE	19.308	151813	2.738 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_F\Data\FF031518\
Data File : FF000278.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2018 08:12
Operator : UA\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 15 11:56:41 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF031518.M
Quant Title :
QLast Update : Thu Mar 15 11:28:02 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

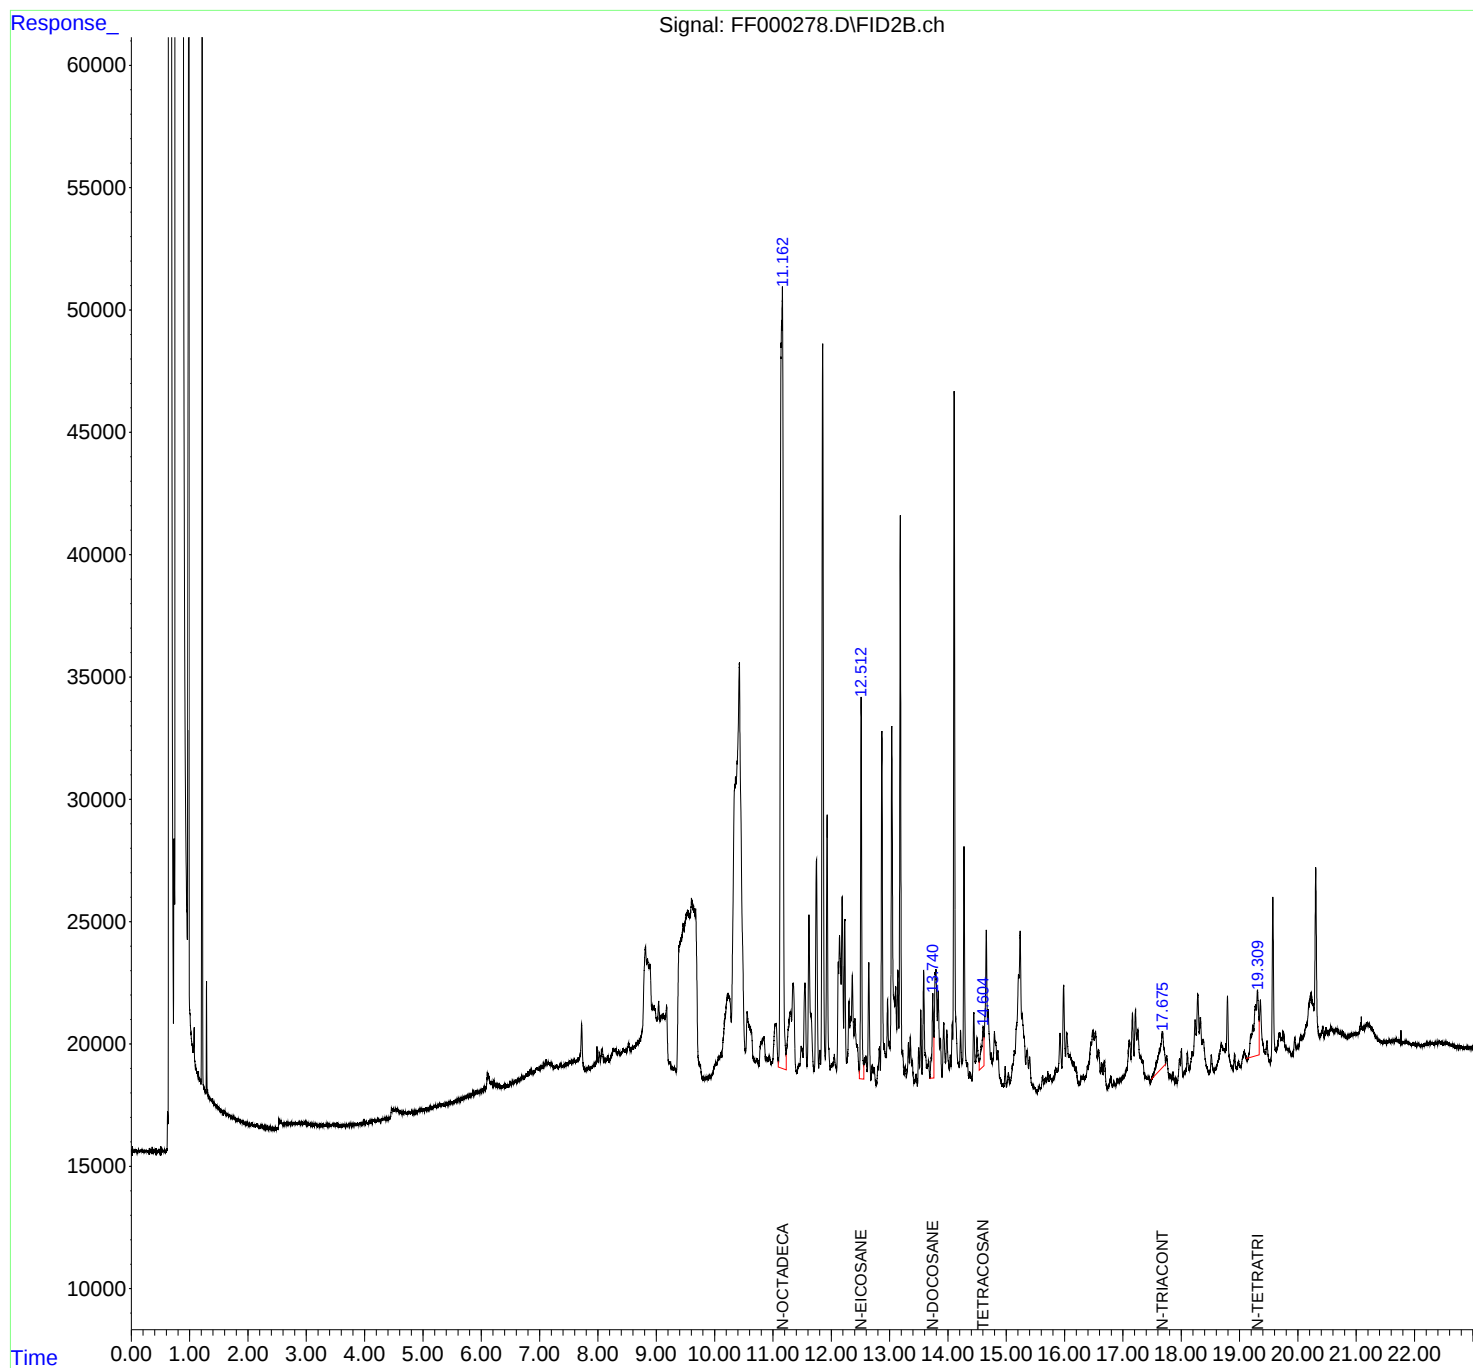


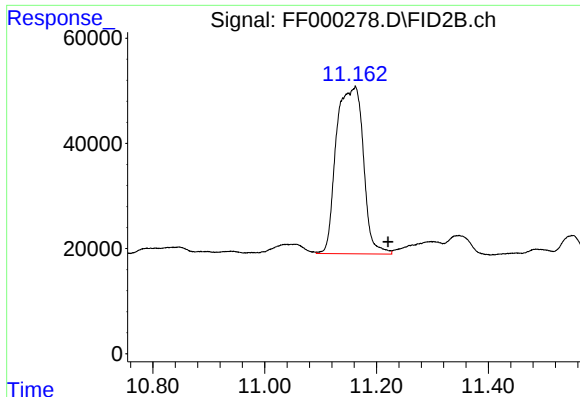

#6 N-OCTADECANE


R.T.: 11.161 min
Delta R.T.: -0.060 min
Response: 1061291
Conc: 8.37 ug/ml

Instrument :
FID_F
ClientSampleId :

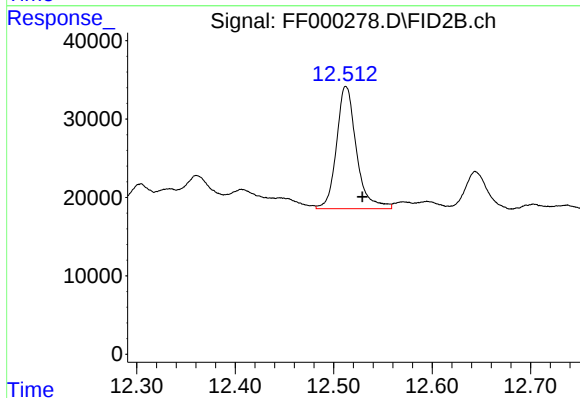


#7 N-EICOSANE

R.T.: 12.513 min
Delta R.T.: -0.017 min
Response: 219124
Conc: 1.71 ug/ml

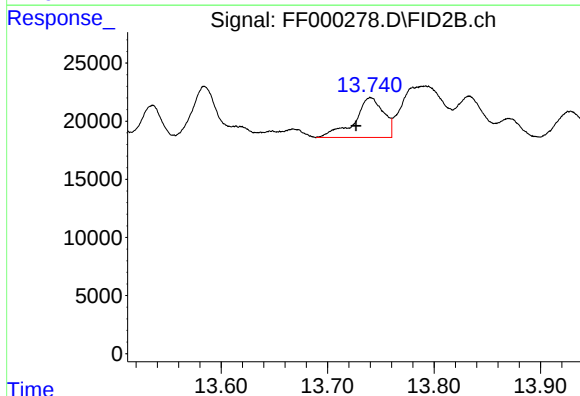


#8 N-DOCOSANE

R.T.: 13.740 min
Delta R.T.: 0.013 min
Response: 64690
Conc: 0.50 ug/ml

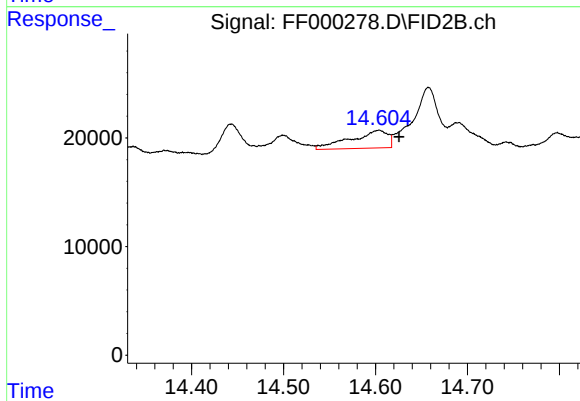

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.603 min
Delta R.T.: -0.022 min
Response: 46019
Conc: 0.40 ug/ml

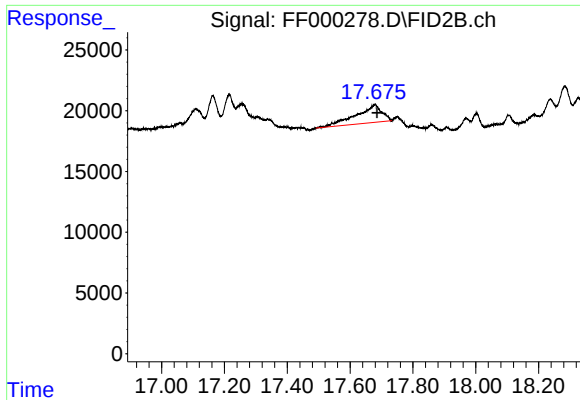

#13 N-TRIACONTANE

R.T.: 17.679 min
Delta R.T.: -0.006 min
Response: 82732
Conc: 0.94 ug/ml

Instrument :
FID_F
ClientSampleId :

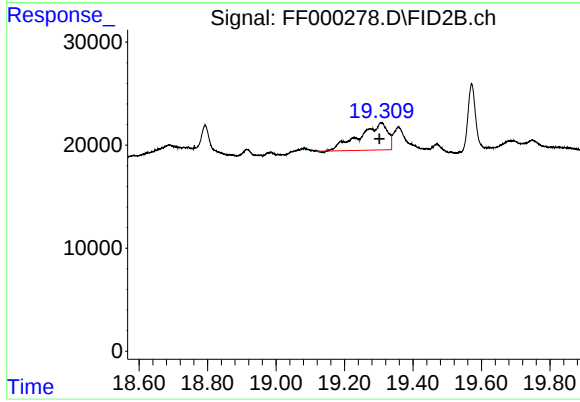

#15 N-TETRATRIACONTANE

R.T.: 19.308 min
Delta R.T.: 0.006 min
Response: 151813
Conc: 2.74 ug/ml