

Data Path : P:\HPCHEM1\FID_F\Data\FF031518\
 Data File : FF000291.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2018 14:28
 Operator : UA\AJ
 Sample : J1888-19
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 15 15:08:43 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF031518.M
 Quant Title :
 QLast Update : Thu Mar 15 11:28:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.624	3049081	26.623 ug/ml
Target Compounds			
1) N-OCTANE	2.271	240113	2.688 ug/ml
2) N-DECANE	4.373	4160660	43.062 ug/ml
3) N-DODECANE	6.392	7237764	69.823 ug/ml
4) N-TETRADECANE	8.185	9837331	86.075 ug/ml
5) N-HEXADECANE	9.784	12772698	105.612 ug/ml
6) N-OCTADECANE	11.223	11473639	90.479 ug/ml
7) N-EICOSANE	12.530	7312711	56.933 ug/ml
8) N-DOCOSANE	13.724	3061875	23.738 ug/ml
10) N-TETRACOSANE	14.826	339872	2.580 ug/ml
11) N-HEXACOSANE	15.847	24523	0.202 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_F\Data\FF031518\
Data File : FF000291.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2018 14:28
Operator : UA\AJ
Sample : J1888-19
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 15 15:08:43 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF031518.M
Quant Title :
QLast Update : Thu Mar 15 11:28:02 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

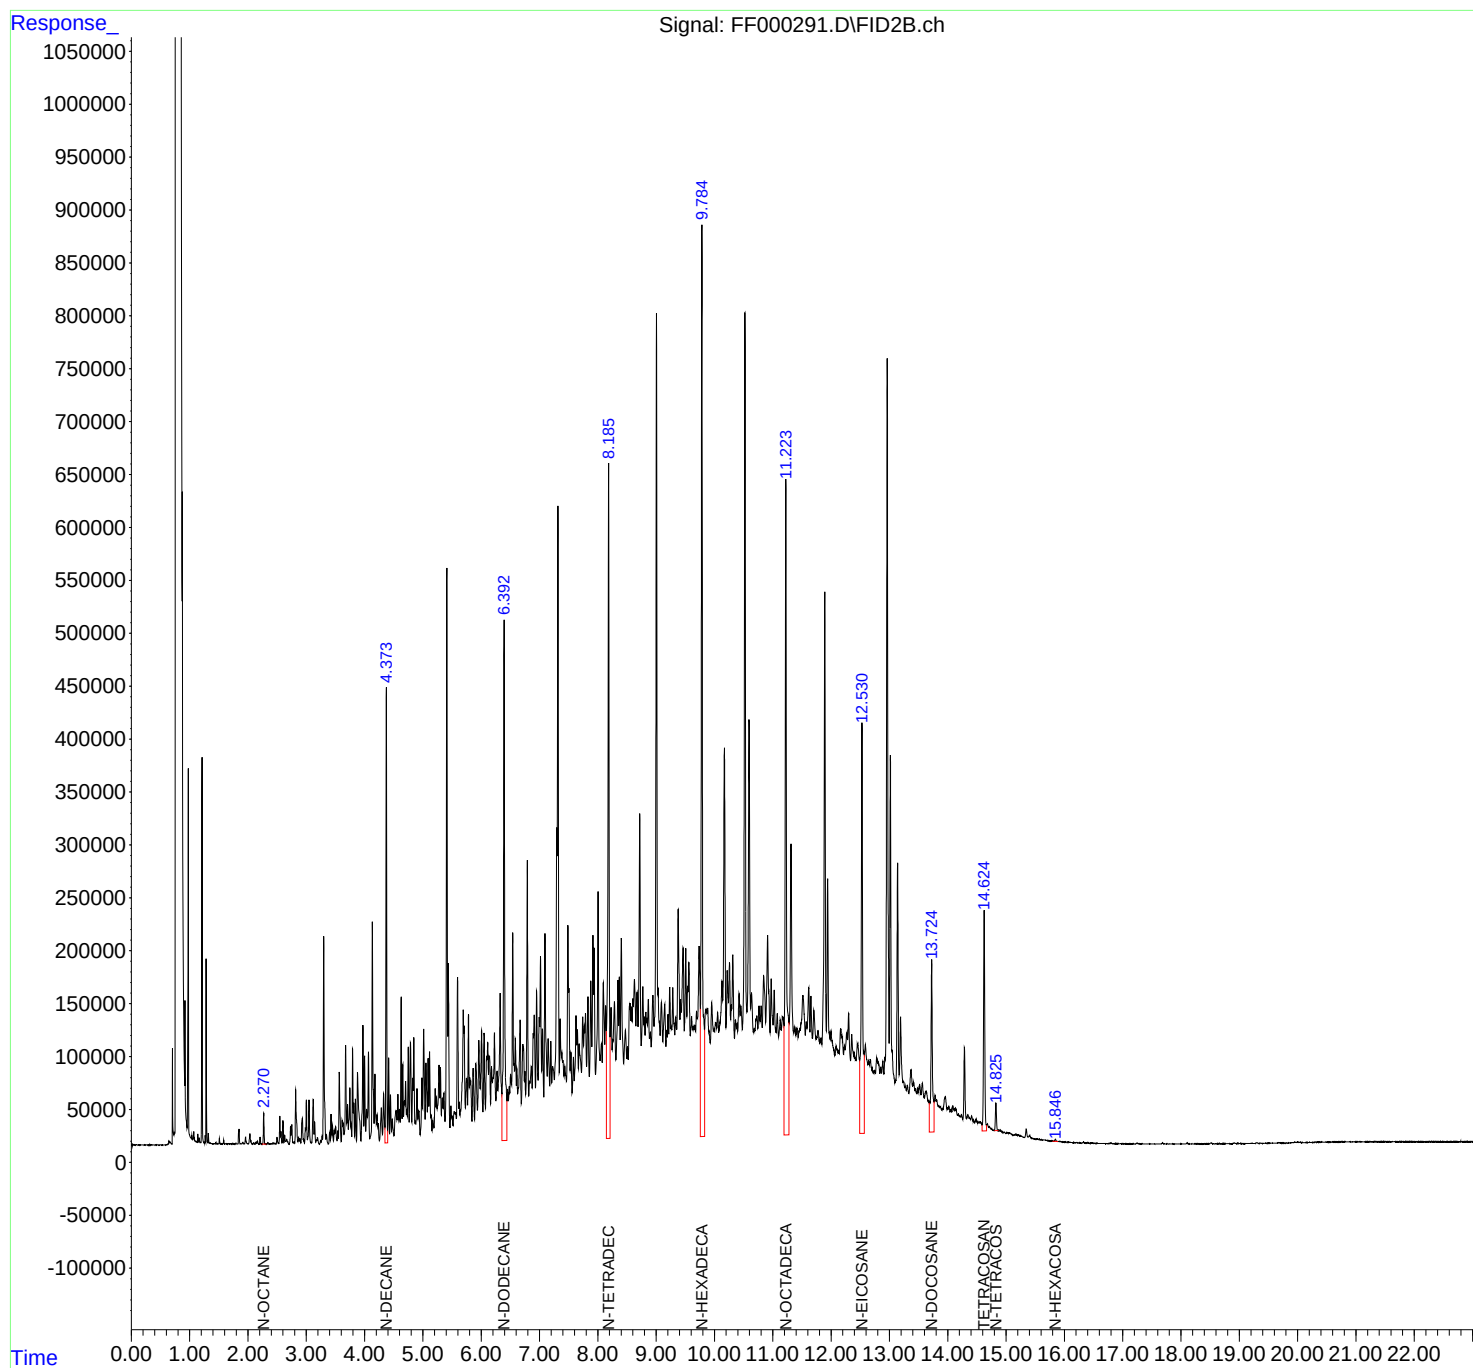


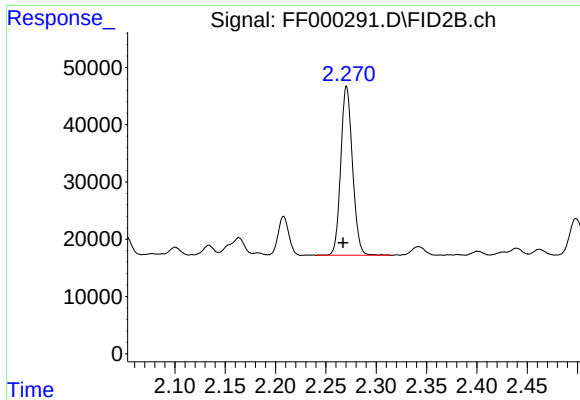

#1 N-OCTANE


R.T.: 2.271 min
Delta R.T.: 0.004 min
Response: 240113
Conc: 2.69 ug/ml

Instrument :
FID_F
ClientSampleId :

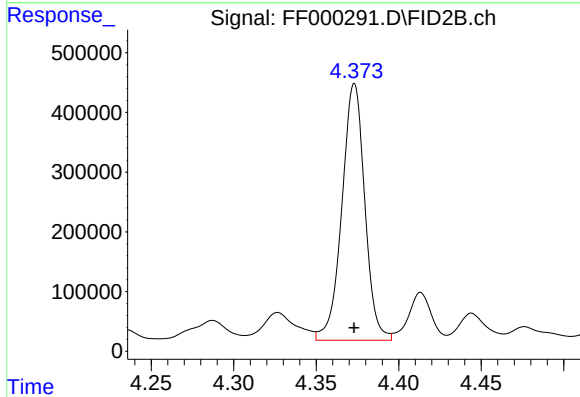


#2 N-DECANE

R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 4160660
Conc: 43.06 ug/ml

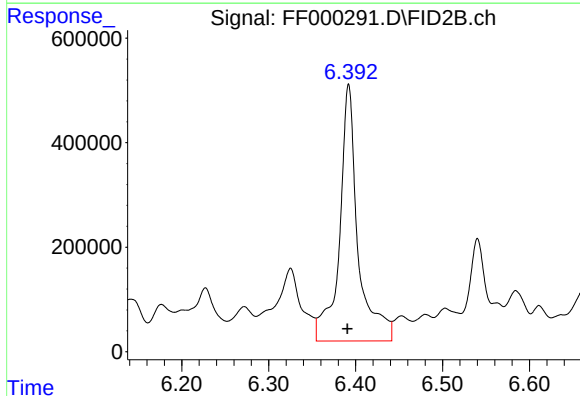


#3 N-DODECANE

R.T.: 6.392 min
Delta R.T.: 0.002 min
Response: 7237764
Conc: 69.82 ug/ml

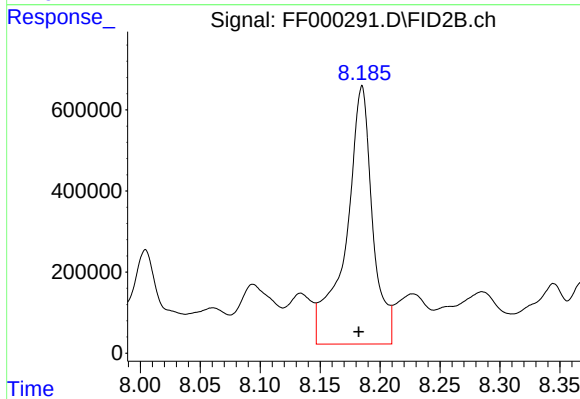

#4 N-TETRADECANE


R.T.: 8.185 min
Delta R.T.: 0.003 min
Response: 9837331
Conc: 86.07 ug/ml

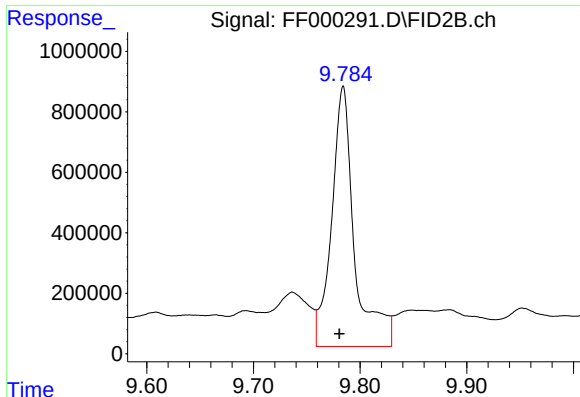

#5 N-HEXADECANE


R.T.: 9.784 min
Delta R.T.: 0.004 min
Response: 12772698
Conc: 105.61 ug/ml

Instrument :
FID_F
ClientSampleId :

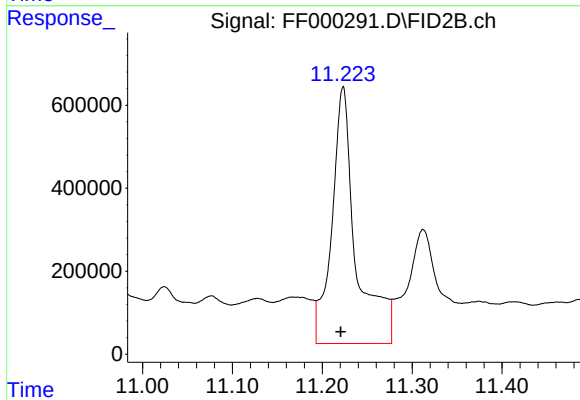


#6 N-OCTADECANE

R.T.: 11.223 min
Delta R.T.: 0.003 min
Response: 11473639
Conc: 90.48 ug/ml

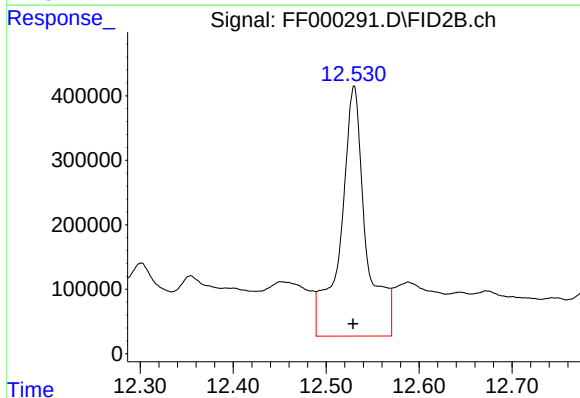


#7 N-EICOSANE

R.T.: 12.530 min
Delta R.T.: 0.000 min
Response: 7312711
Conc: 56.93 ug/ml

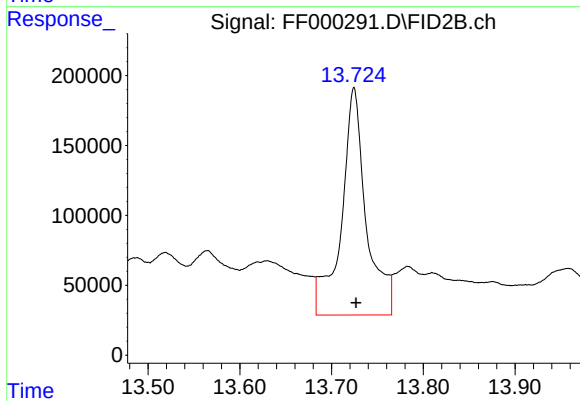

#8 N-DOCOSANE


R.T.: 13.724 min
Delta R.T.: -0.002 min
Response: 3061875
Conc: 23.74 ug/ml

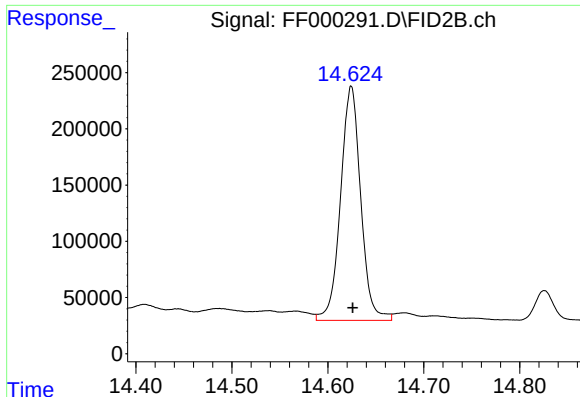

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.624 min
Delta R.T.: -0.001 min
Response: 3049081
Conc: 26.62 ug/ml

Instrument :
FID_F
ClientSampleId :

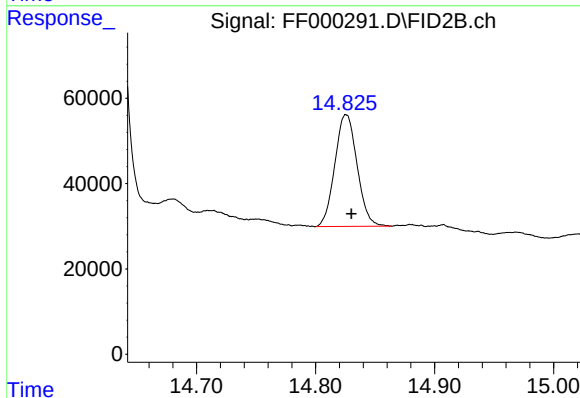

#10 N-TETRACOSANE

R.T.: 14.826 min
Delta R.T.: -0.004 min
Response: 339872
Conc: 2.58 ug/ml

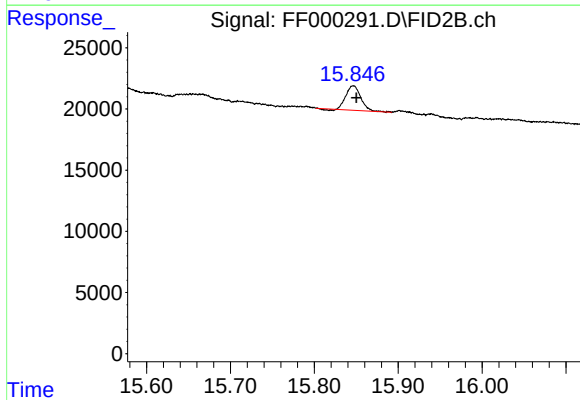

#11 N-HEXACOSANE

R.T.: 15.847 min
Delta R.T.: -0.004 min
Response: 24523
Conc: 0.20 ug/ml