

Data Path : P:\HPCHEM1\FID_F\Data\FF031518\
 Data File : FF000292.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2018 14:59
 Operator : UA\AJ
 Sample : J1888-19 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 15 15:23:01 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF031518.M
 Quant Title :
 QLast Update : Thu Mar 15 11:28:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.622	265123	2.315 ug/ml
Target Compounds			
1) N-OCTANE	2.270	25613	0.287 ug/ml
2) N-DECANE	4.368	394872	4.087 ug/ml
3) N-DODECANE	6.385	559746	5.400 ug/ml
4) N-TETRADECANE	8.176	772765	6.762 ug/ml
5) N-HEXADECANE	9.775	990588	8.191 ug/ml
6) N-OCTADECANE	11.215	754733	5.952 ug/ml
7) N-EICOSANE	12.524	372156	2.897 ug/ml
8) N-DOCOSANE	13.722	155341	1.204 ug/ml
10) N-TETRACOSANE	14.826	28036	0.213 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_F\Data\FF031518\
Data File : FF000292.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2018 14:59
Operator : UA\AJ
Sample : J1888-19 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 15 15:23:01 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF031518.M
Quant Title :
QLast Update : Thu Mar 15 11:28:02 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

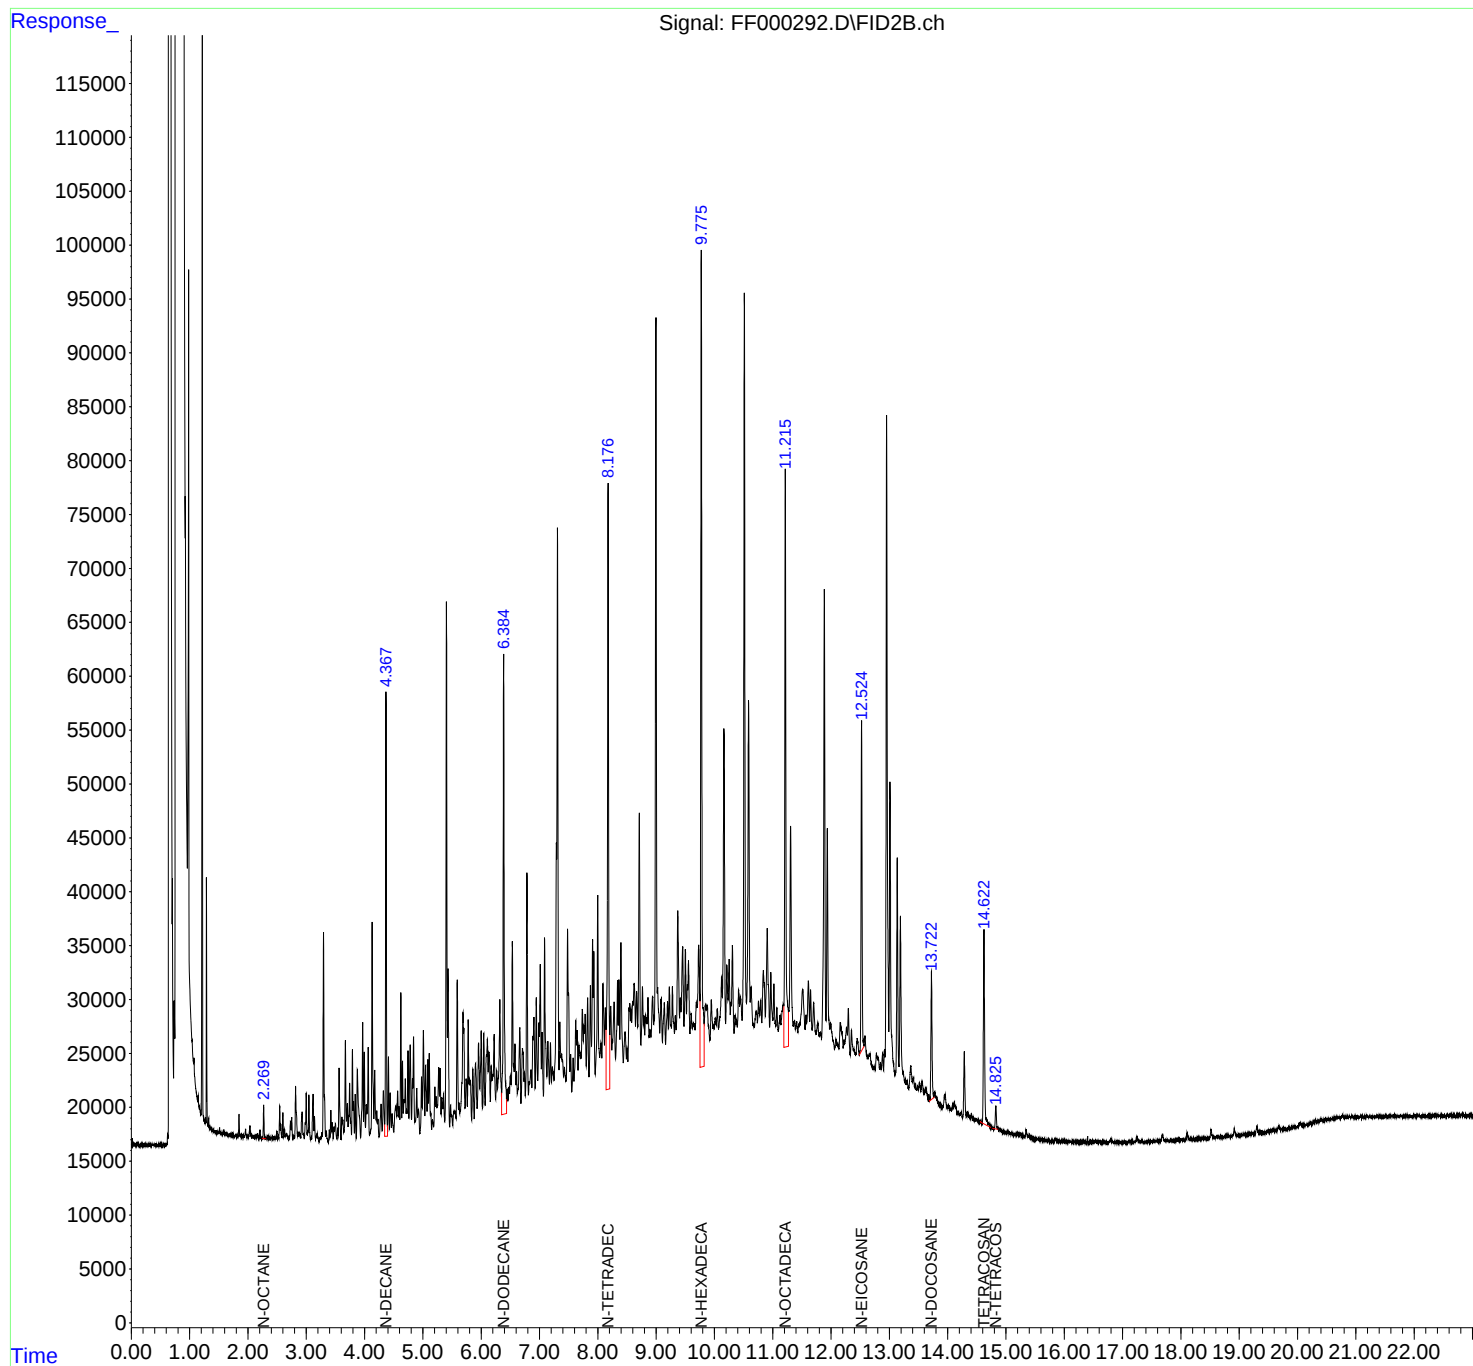


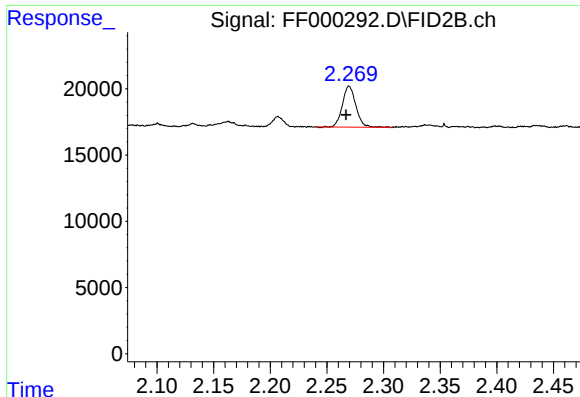

#1 N-OCTANE


R.T.: 2.270 min
Delta R.T.: 0.003 min
Response: 25613
Conc: 0.29 ug/ml

Instrument :
FID_F
ClientSampleId :

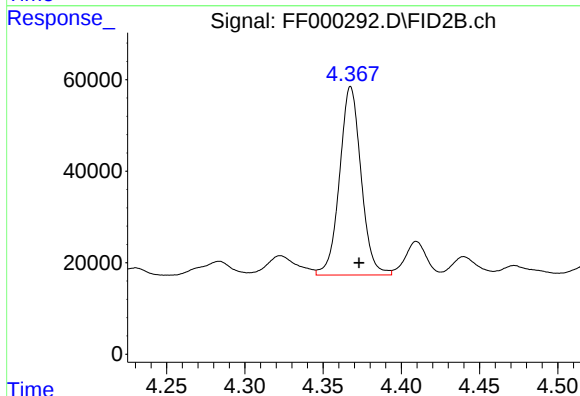


#2 N-DECANE

R.T.: 4.368 min
Delta R.T.: -0.005 min
Response: 394872
Conc: 4.09 ug/ml

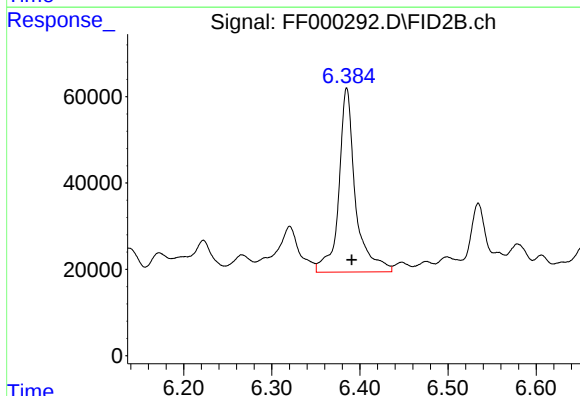


#3 N-DODECANE

R.T.: 6.385 min
Delta R.T.: -0.005 min
Response: 559746
Conc: 5.40 ug/ml

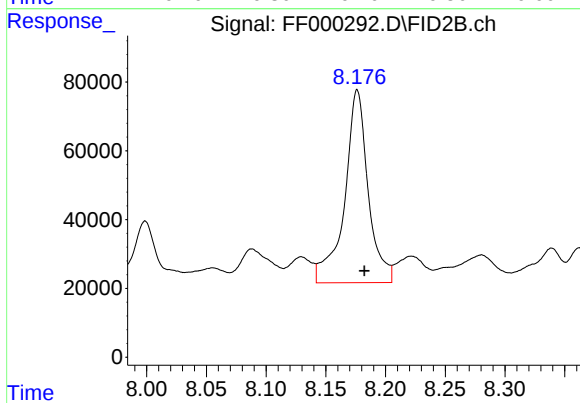

#4 N-TETRADECANE


R.T.: 8.176 min
Delta R.T.: -0.006 min
Response: 772765
Conc: 6.76 ug/ml

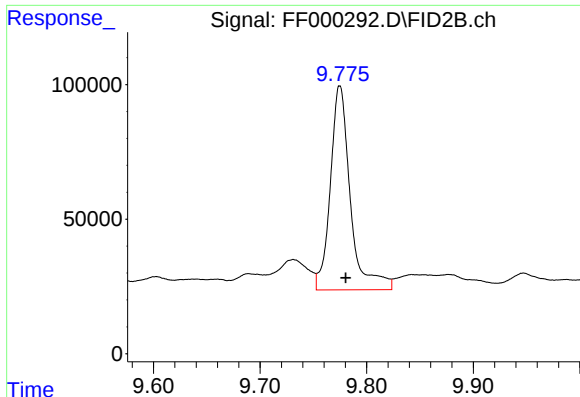

#5 N-HEXADECANE


R.T.: 9.775 min
Delta R.T.: -0.006 min
Response: 990588
Conc: 8.19 ug/ml

Instrument :
FID_F
ClientSampleId :

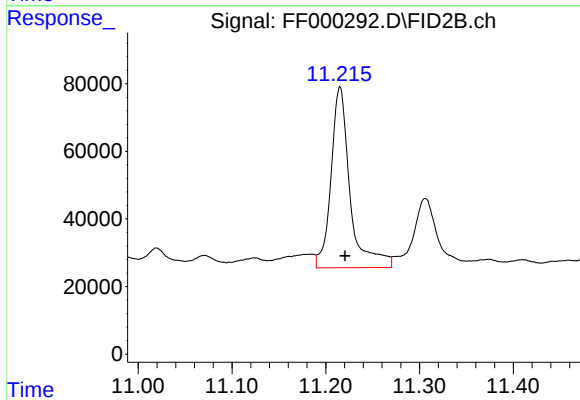


#6 N-OCTADECANE

R.T.: 11.215 min
Delta R.T.: -0.005 min
Response: 754733
Conc: 5.95 ug/ml

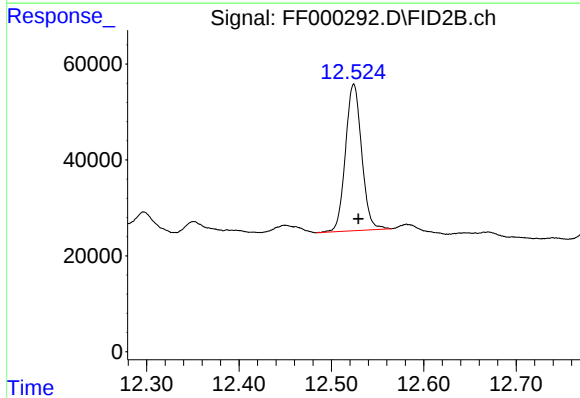


#7 N-EICOSANE

R.T.: 12.524 min
Delta R.T.: -0.005 min
Response: 372156
Conc: 2.90 ug/ml

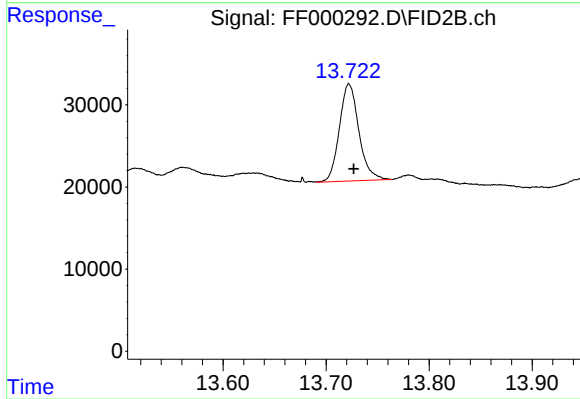

#8 N-DOCOSANE


R.T.: 13.722 min
Delta R.T.: -0.005 min
Response: 155341
Conc: 1.20 ug/ml

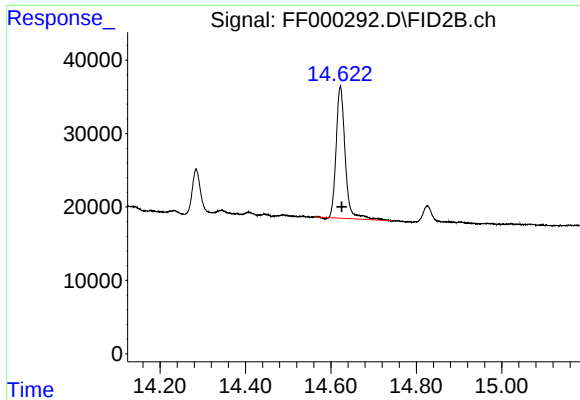

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.622 min
Delta R.T.: -0.004 min
Response: 265123
Conc: 2.31 ug/ml

Instrument :
FID_F
ClientSampleId :

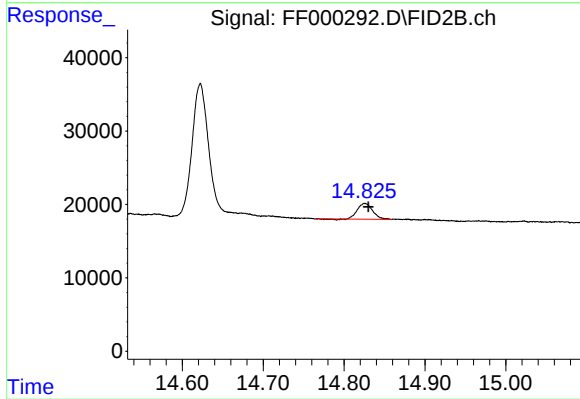

#10 N-TETRACOSANE

R.T.: 14.826 min
Delta R.T.: -0.004 min
Response: 28036
Conc: 0.21 ug/ml