

Data Path : P:\HPCHEM1\FID_F\Data\FF031518\
 Data File : FF000287.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2018 12:33
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Mar 15 14:26:10 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF031518.M
 Quant Title :
 QLast Update : Thu Mar 15 11:28:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.626	6164588	53.825 ug/ml
Target Compounds			
2) N-DECANE	4.369	5286747	54.717 ug/ml
3) N-DODECANE	6.388	5789399	55.851 ug/ml
4) N-TETRADECANE	8.180	6484228	56.736 ug/ml
5) N-HEXADECANE	9.778	6796659	56.199 ug/ml
6) N-OCTADECANE	11.220	6947650	54.788 ug/ml
7) N-EICOSANE	12.528	6891602	53.655 ug/ml
8) N-DOCOSANE	13.727	6934880	53.764 ug/ml
10) N-TETRACOSANE	14.830	7117508	54.024 ug/ml
11) N-HEXACOSANE	15.850	6690595	55.182 ug/ml
12) N-OCTACOSANE	16.800	6143767	56.039 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_F\Data\FF031518\
Data File : FF000287.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2018 12:33
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Mar 15 14:26:10 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF031518.M
Quant Title :
QLast Update : Thu Mar 15 11:28:02 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

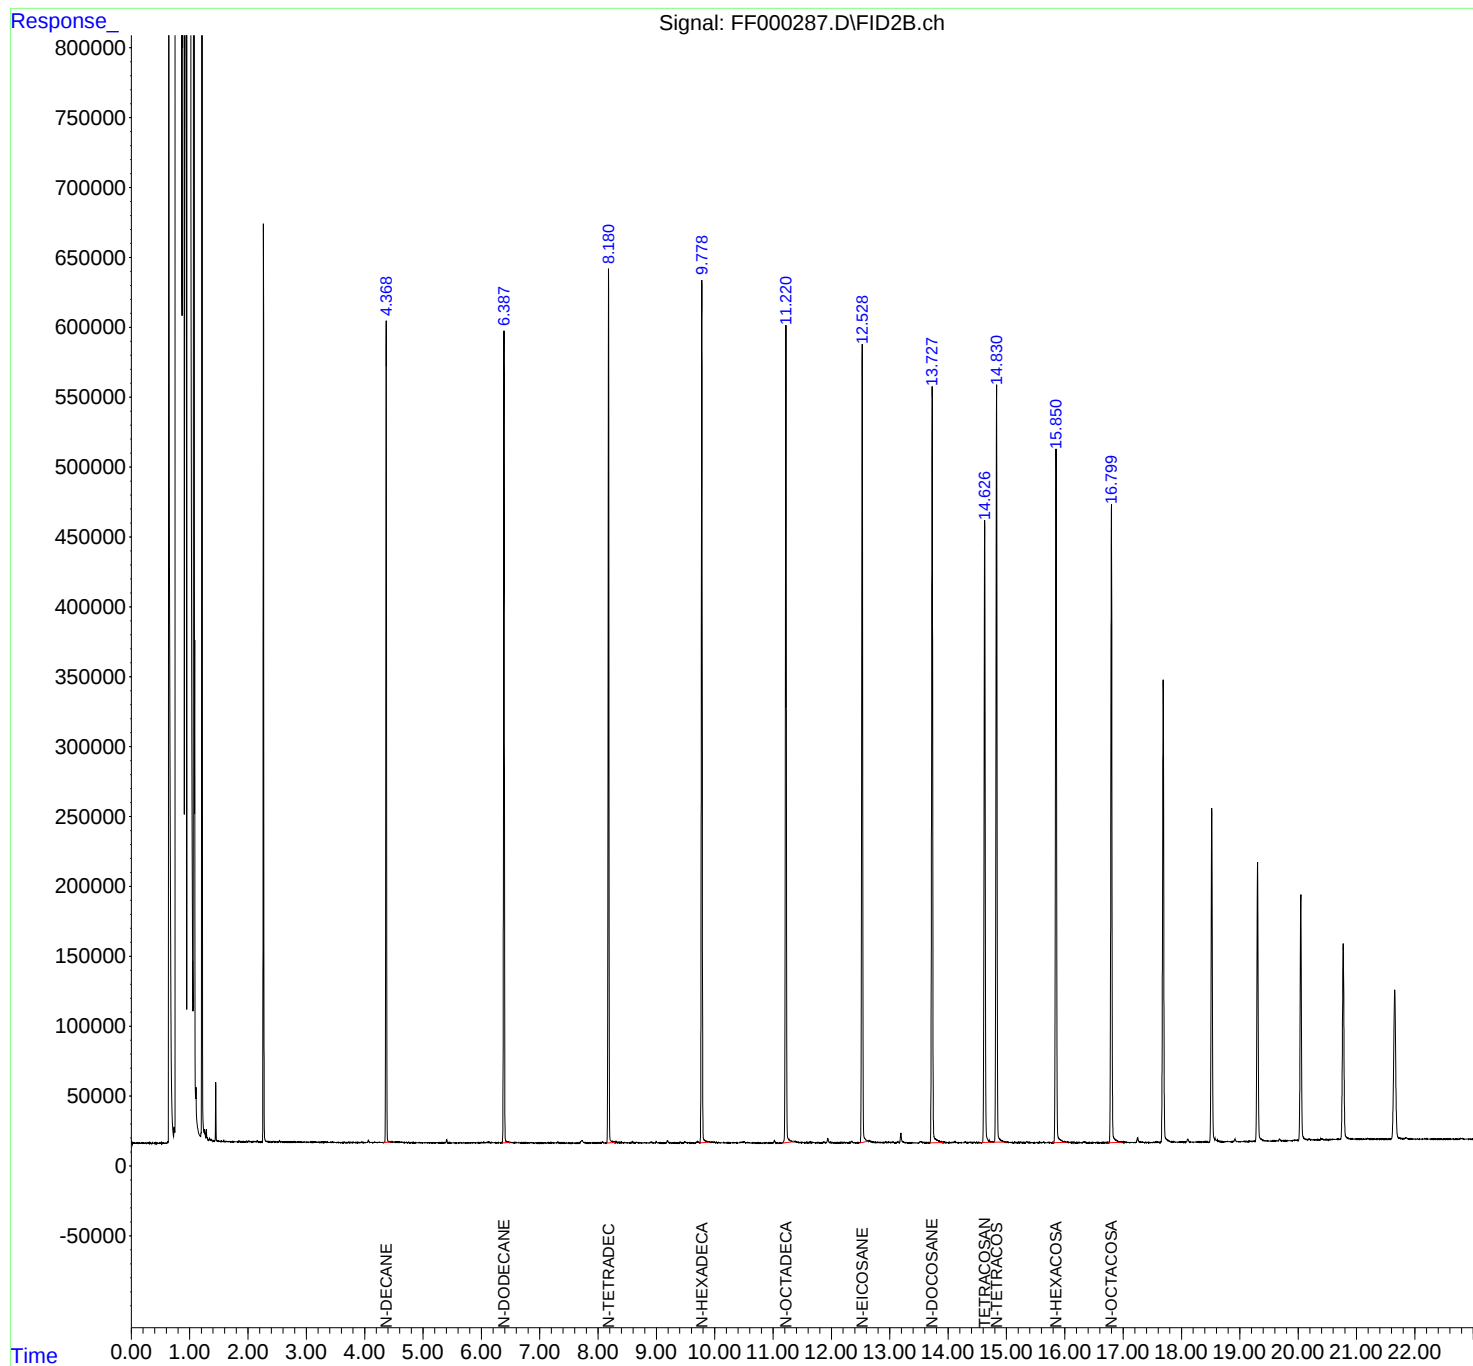


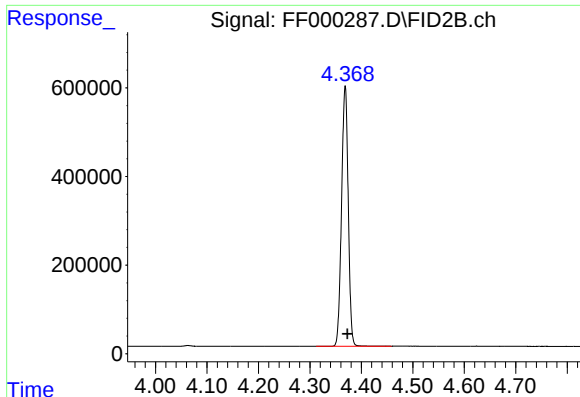

#2 N-DECANE


R.T.: 4.369 min
Delta R.T.: -0.004 min
Response: 5286747
Conc: 54.72 ug/ml

Instrument :
FID_F
ClientSampleId :

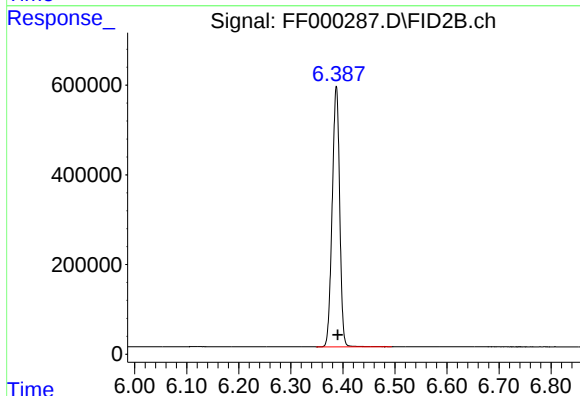


#3 N-DODECANE

R.T.: 6.388 min
Delta R.T.: -0.003 min
Response: 5789399
Conc: 55.85 ug/ml

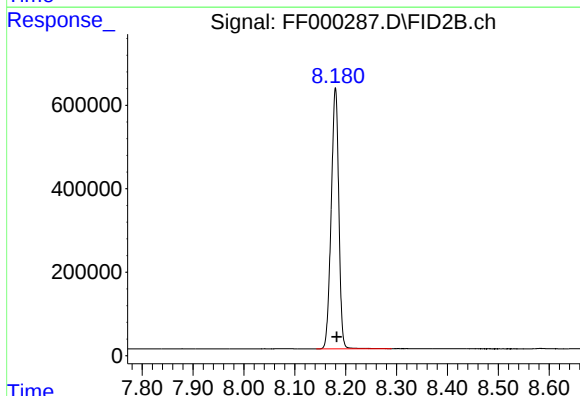


#4 N-TETRADECANE

R.T.: 8.180 min
Delta R.T.: -0.002 min
Response: 6484228
Conc: 56.74 ug/ml

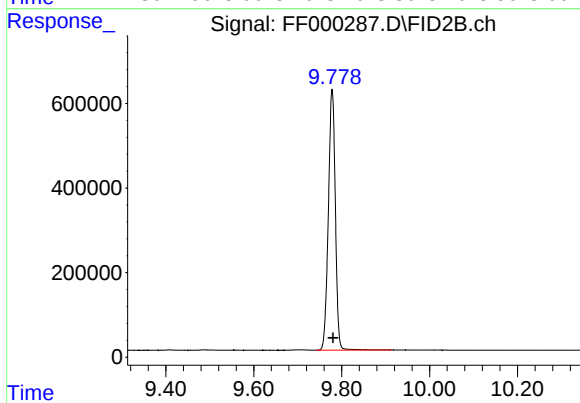

#5 N-HEXADECANE


R.T.: 9.778 min
Delta R.T.: -0.002 min
Response: 6796659
Conc: 56.20 ug/ml

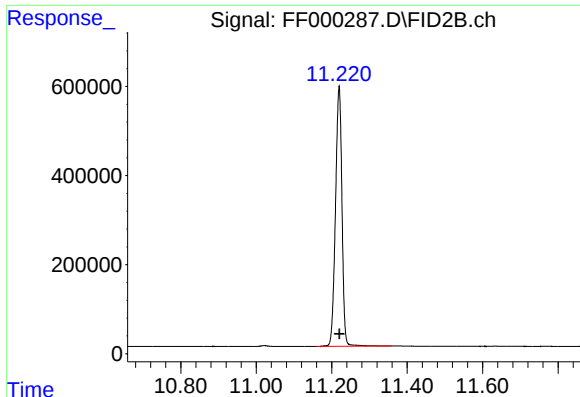

#6 N-OCTADECANE


R.T.: 11.220 min
Delta R.T.: 0.000 min
Response: 6947650
Conc: 54.79 ug/ml

Instrument :
FID_F
ClientSampleId :

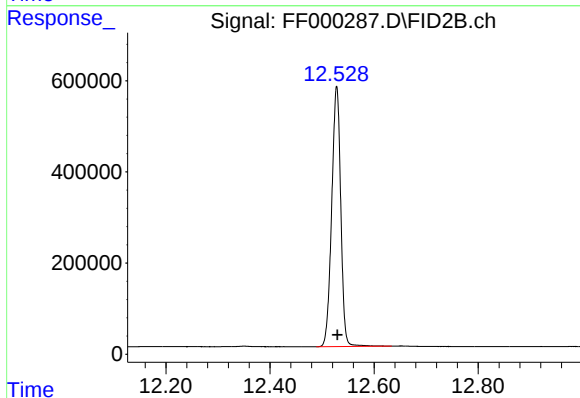


#7 N-EICOSANE

R.T.: 12.528 min
Delta R.T.: -0.001 min
Response: 6891602
Conc: 53.65 ug/ml

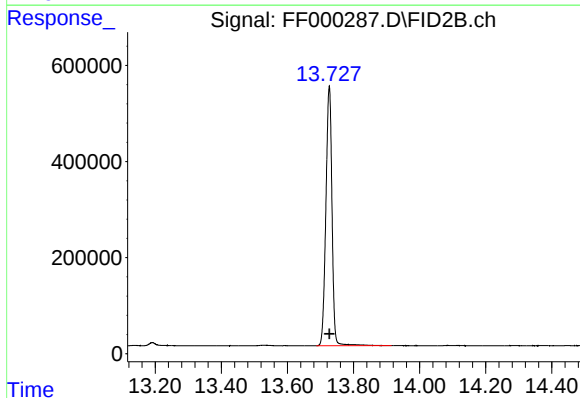


#8 N-DOCOSANE

R.T.: 13.727 min
Delta R.T.: 0.000 min
Response: 6934880
Conc: 53.76 ug/ml

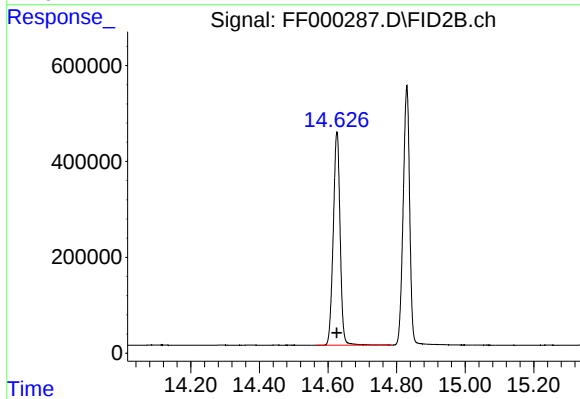

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.626 min
Delta R.T.: 0.000 min
Response: 6164588
Conc: 53.83 ug/ml

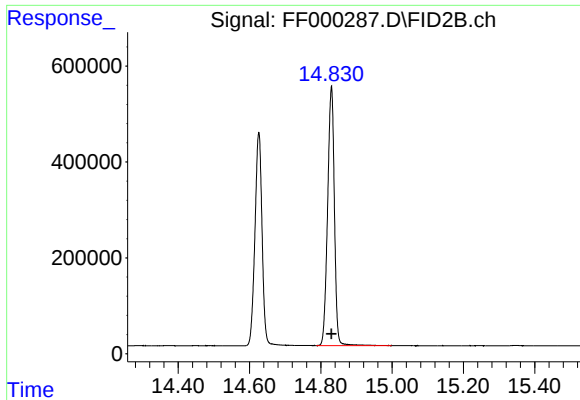

#10 N-TETRACOSANE


R.T.: 14.830 min
Delta R.T.: 0.000 min
Response: 7117508
Conc: 54.02 ug/ml

Instrument :
FID_F
ClientSampleId :

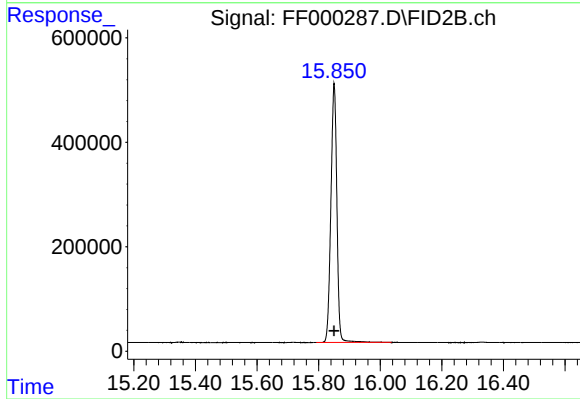

#11 N-HEXACOSANE

R.T.: 15.850 min
Delta R.T.: 0.000 min
Response: 6690595
Conc: 55.18 ug/ml

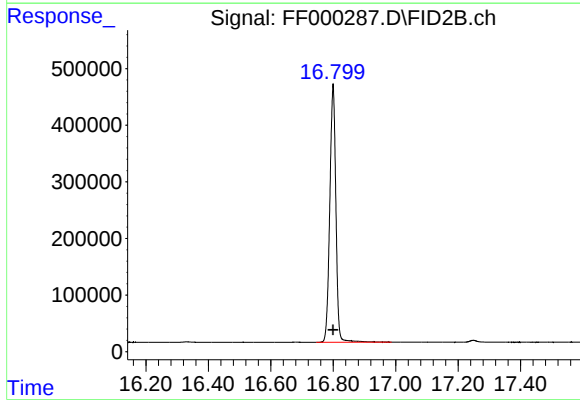

#12 N-OCTACOSANE

R.T.: 16.800 min
Delta R.T.: 0.000 min
Response: 6143767
Conc: 56.04 ug/ml