

Data Path : P:\HPCHEM1\FID_F\Data\FF031518\
 Data File : FF000294.D
 Signal(s) : FID2B.ch
 Acq On : 15 Mar 2018 16:00
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: Sample.e
 Quant Time: Mar 15 16:24:18 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF031518.M
 Quant Title :
 QLast Update : Thu Mar 15 11:28:02 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.625	5710289	49.859 ug/ml
Target Compounds			
2) N-DECANE	4.372	4573771	47.337 ug/ml
3) N-DODECANE	6.390	5041503	48.636 ug/ml
4) N-TETRADECANE	8.181	5711754	49.977 ug/ml
5) N-HEXADECANE	9.780	6051948	50.041 ug/ml
6) N-OCTADECANE	11.220	6251537	49.298 ug/ml
7) N-EICOSANE	12.529	6280390	48.896 ug/ml
8) N-DOCOSANE	13.727	6384311	49.496 ug/ml
10) N-TETRACOSANE	14.829	6622368	50.266 ug/ml
11) N-HEXACOSANE	15.850	6356506	52.426 ug/ml
12) N-OCTACOSANE	16.800	6158779	56.176 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : P:\HPCHEM1\FID_F\Data\FF031518\
Data File : FF000294.D
Signal(s) : FID2B.ch
Acq On : 15 Mar 2018 16:00
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: Sample.e
Quant Time: Mar 15 16:24:18 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF031518.M
Quant Title :
QLast Update : Thu Mar 15 11:28:02 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

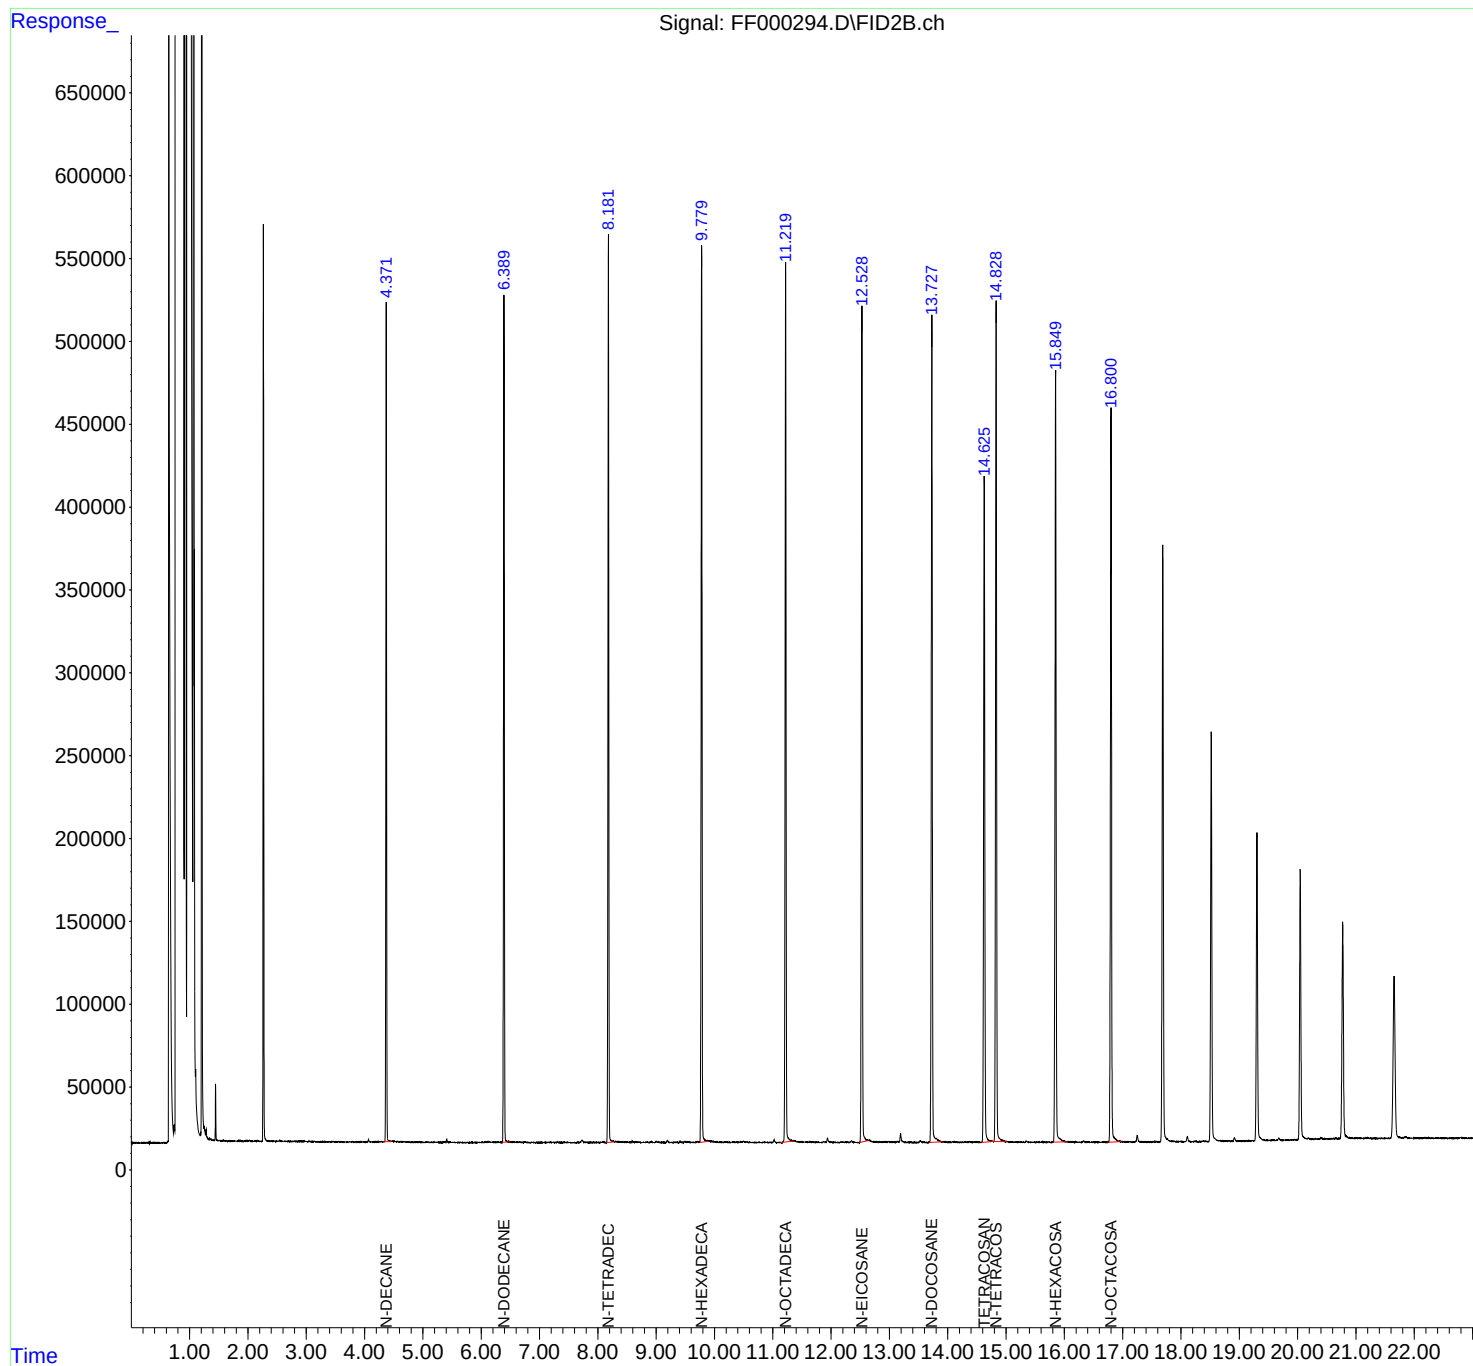


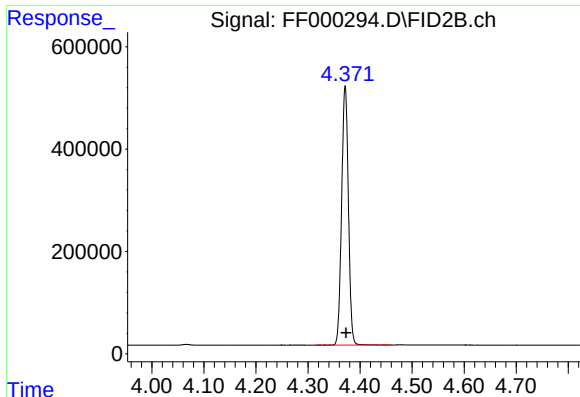

#2 N-DECANE


R.T.: 4.372 min
Delta R.T.: -0.001 min
Response: 4573771
Conc: 47.34 ug/ml

Instrument :
FID_F
ClientSampleId :

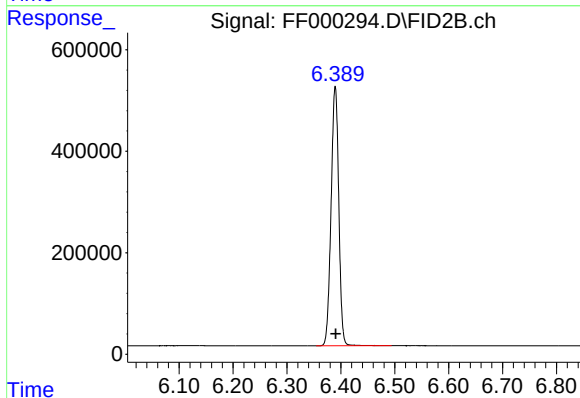


#3 N-DODECANE

R.T.: 6.390 min
Delta R.T.: 0.000 min
Response: 5041503
Conc: 48.64 ug/ml

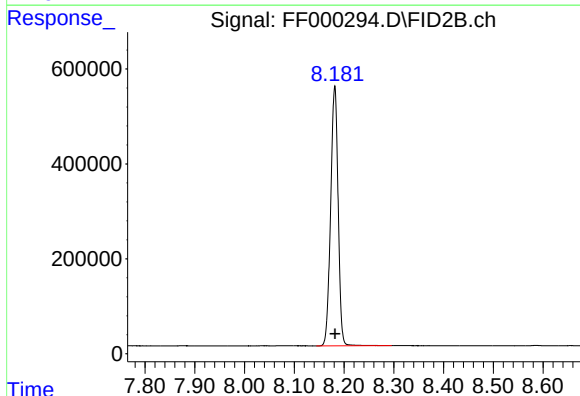


#4 N-TETRADECANE

R.T.: 8.181 min
Delta R.T.: 0.000 min
Response: 5711754
Conc: 49.98 ug/ml

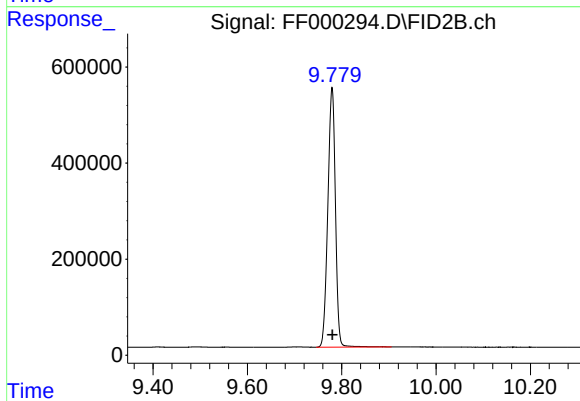

#5 N-HEXADECANE


R.T.: 9.780 min
Delta R.T.: 0.000 min
Response: 6051948
Conc: 50.04 ug/ml

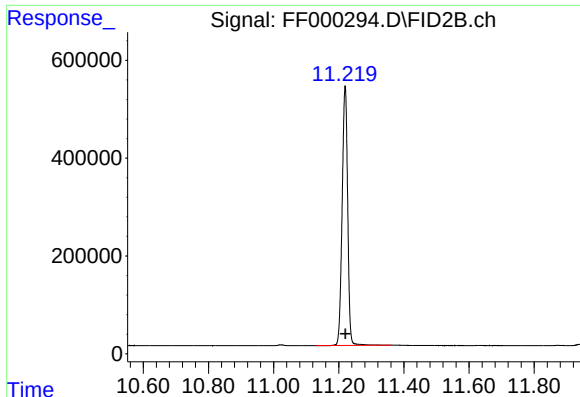

#6 N-OCTADECANE


R.T.: 11.220 min
Delta R.T.: 0.000 min
Response: 6251537
Conc: 49.30 ug/ml

Instrument :
FID_F
ClientSampleId :

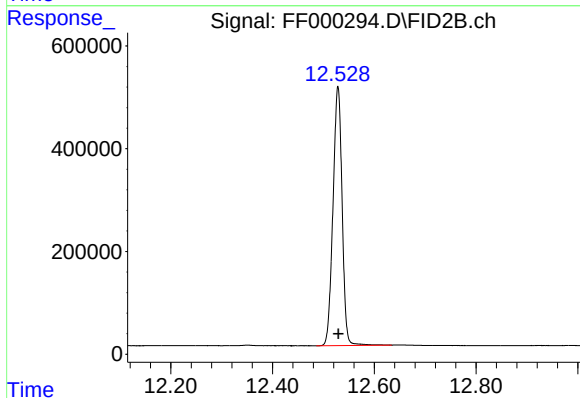


#7 N-EICOSANE

R.T.: 12.529 min
Delta R.T.: 0.000 min
Response: 6280390
Conc: 48.90 ug/ml

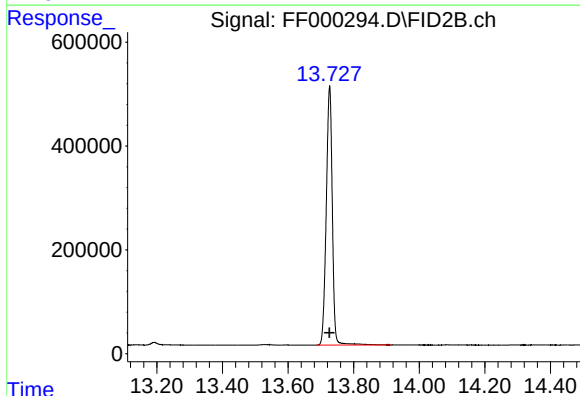


#8 N-DOCOSANE

R.T.: 13.727 min
Delta R.T.: 0.000 min
Response: 6384311
Conc: 49.50 ug/ml

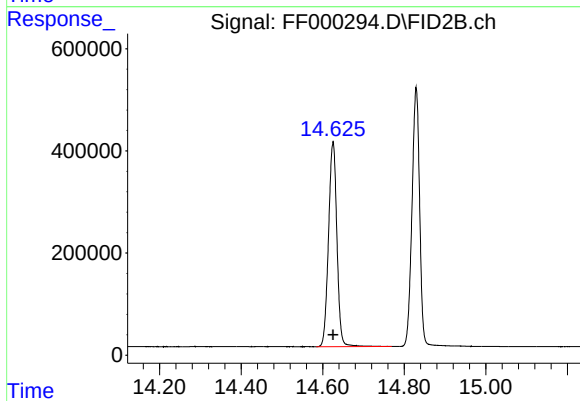

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.625 min
Delta R.T.: 0.000 min
Response: 5710289
Conc: 49.86 ug/ml

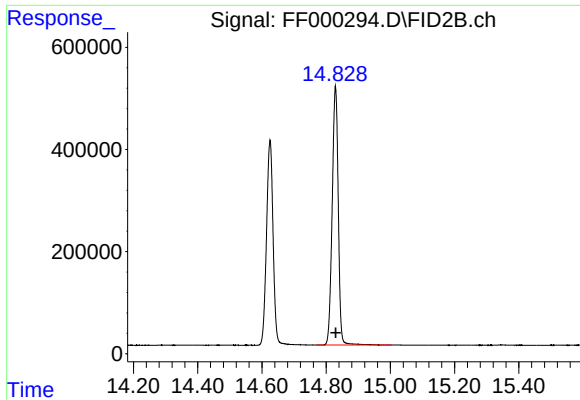

#10 N-TETRACOSANE


R.T.: 14.829 min
Delta R.T.: 0.000 min
Response: 6622368
Conc: 50.27 ug/ml

Instrument :
FID_F
ClientSampleId :

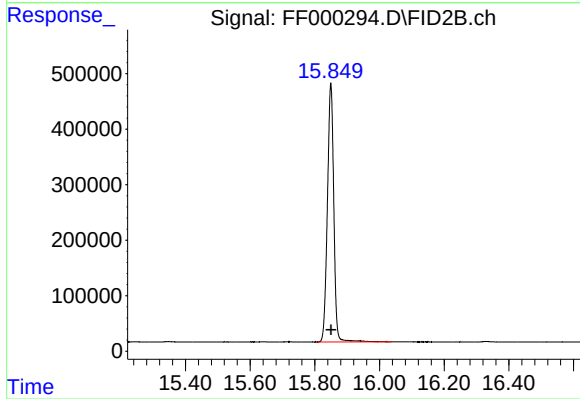

#11 N-HEXACOSANE

R.T.: 15.850 min
Delta R.T.: 0.000 min
Response: 6356506
Conc: 52.43 ug/ml

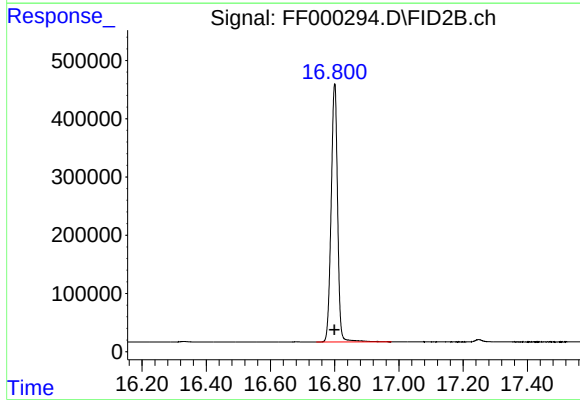

#12 N-OCTACOSANE

R.T.: 16.800 min
Delta R.T.: 0.000 min
Response: 6158779
Conc: 56.18 ug/ml