

Data Path : P:\HPCHEM1\FID_F\Data\FF042518\
 Data File : FF000473.D
 Signal(s) : FID2B.ch
 Acq On : 25 Apr 2018 11:34
 Operator : UA\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 26 04:17:29 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF042318.M
 Quant Title :
 QLast Update : Mon Apr 23 18:07:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.607	7717355	53.825 ug/ml
Target Compounds				
2)	N-DECANE	4.353	8437650	52.981 ug/ml
3)	N-DODECANE	6.369	8561633	53.236 ug/ml
4)	N-TETRADECANE	8.163	8673993	53.383 ug/ml
5)	N-HEXADECANE	9.761	8774425	53.463 ug/ml
6)	N-OCTADECANE	11.202	8836023	53.517 ug/ml
7)	N-EICOSANE	12.511	8784250	53.380 ug/ml
8)	N-DOCOSANE	13.708	8726550	53.464 ug/ml
10)	N-TETRACOSANE	14.810	8641195	53.682 ug/ml
11)	N-HEXACOSANE	15.830	8559330	53.856 ug/ml
12)	N-OCTACOSANE	16.780	8515468	54.094 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_F\Data\FF042518\
Data File : FF000473.D
Signal(s) : FID2B.ch
Acq On : 25 Apr 2018 11:34
Operator : UA\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 26 04:17:29 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF042318.M
Quant Title :
QLast Update : Mon Apr 23 18:07:21 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

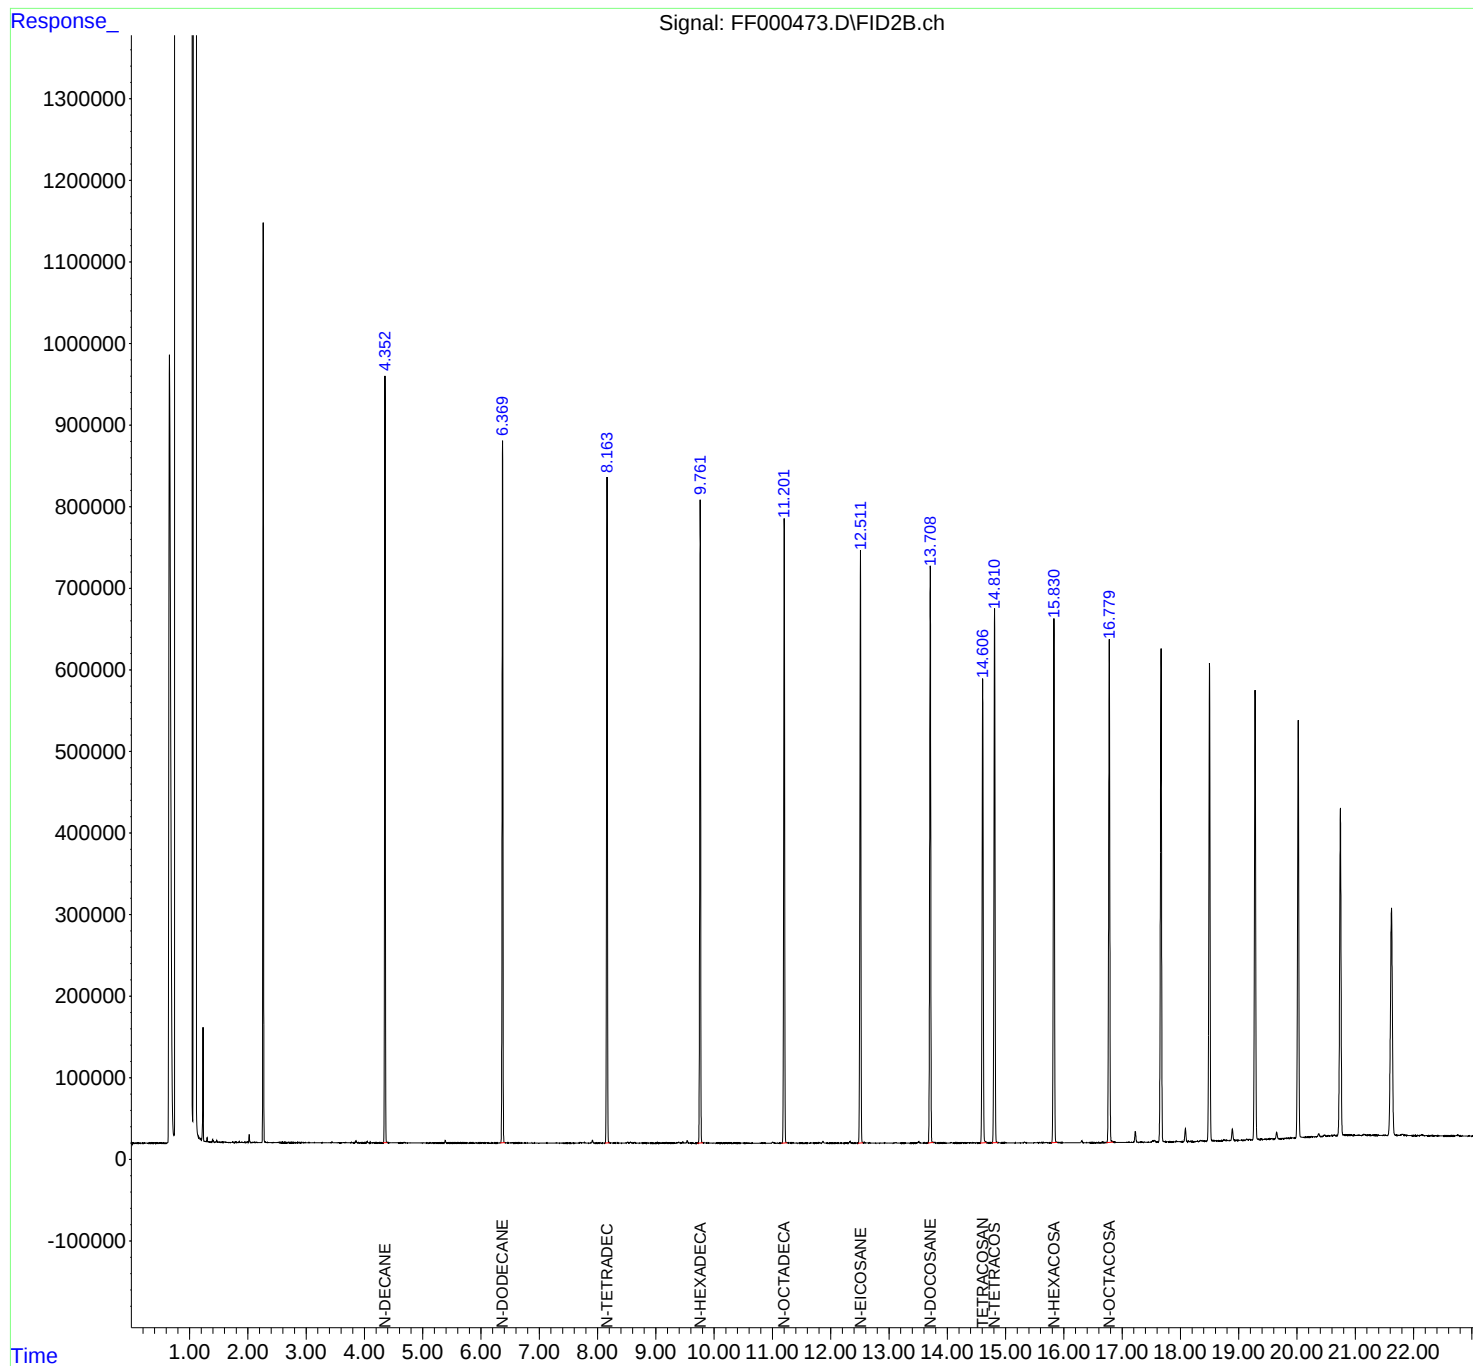

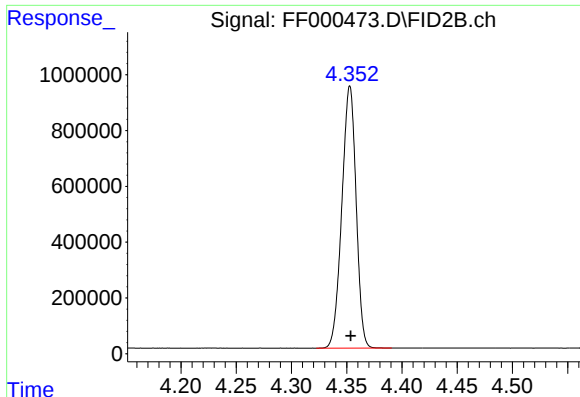


#2 N-DECANE

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 8437650
Conc: 52.98 ug/ml

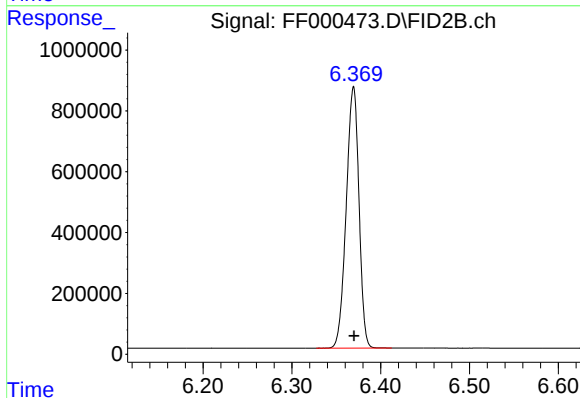


#3 N-DODECANE

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 8561633
Conc: 53.24 ug/ml

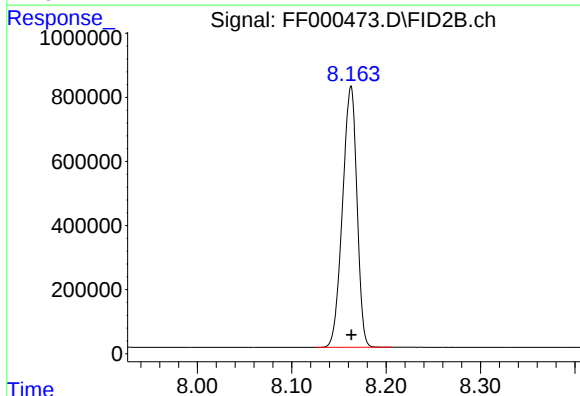


#4 N-TETRADECANE

R.T.: 8.163 min
Delta R.T.: 0.000 min
Response: 8673993
Conc: 53.38 ug/ml

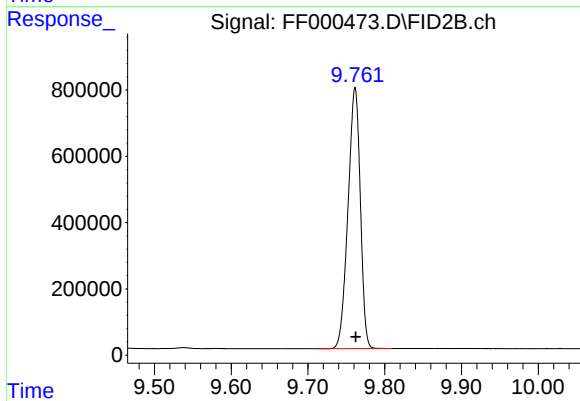


#5 N-HEXADECANE

R.T.: 9.761 min
Delta R.T.: 0.000 min
Response: 8774425
Conc: 53.46 ug/ml

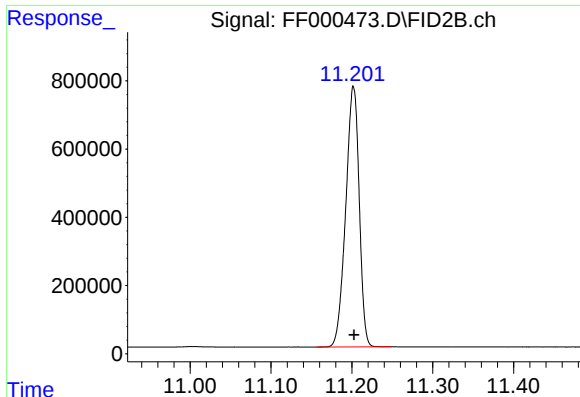


#6 N-OCTADECANE

R.T.: 11.202 min
Delta R.T.: 0.000 min
Response: 8836023
Conc: 53.52 ug/ml

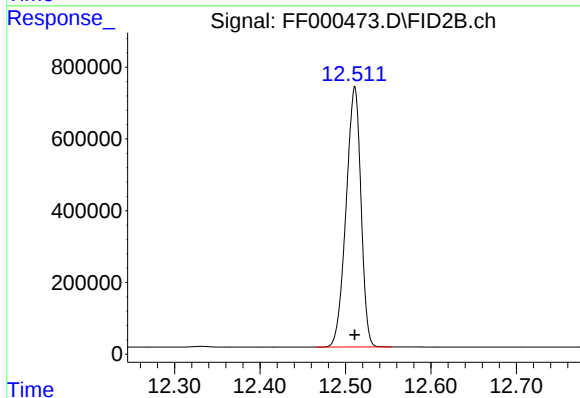


#7 N-EICOSANE

R.T.: 12.511 min
Delta R.T.: 0.000 min
Response: 8784250
Conc: 53.38 ug/ml

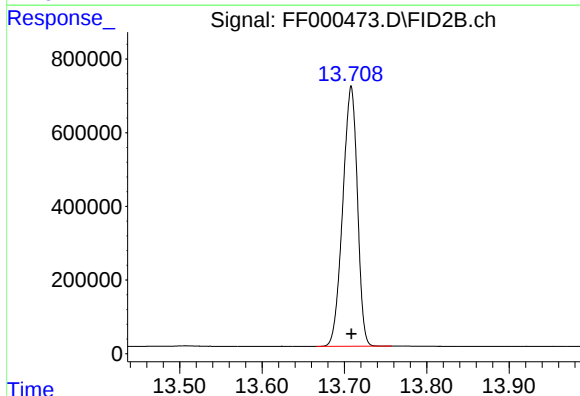


#8 N-DOCOSANE

R.T.: 13.708 min
Delta R.T.: 0.000 min
Response: 8726550
Conc: 53.46 ug/ml

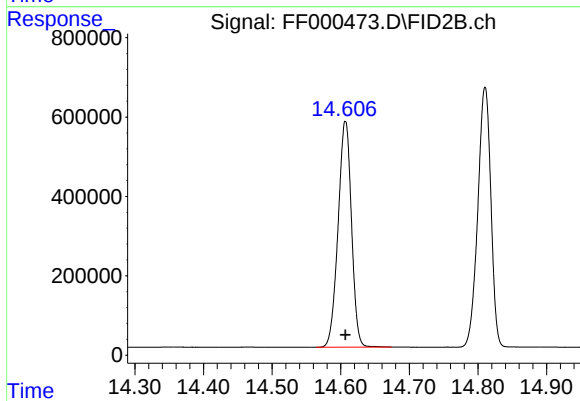


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.607 min
Delta R.T.: 0.000 min
Response: 7717355
Conc: 53.83 ug/ml

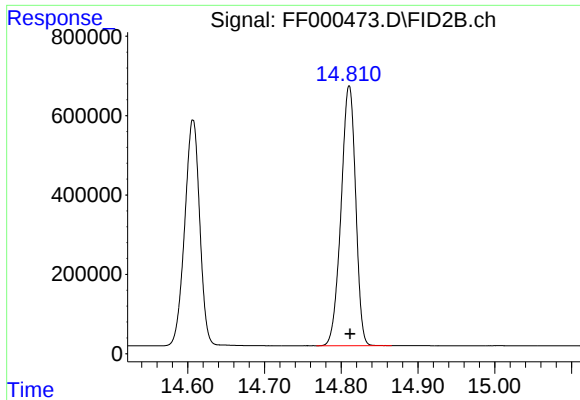


#10 N-TETRACOSANE

R.T.: 14.810 min
Delta R.T.: -0.001 min
Response: 8641195
Conc: 53.68 ug/ml

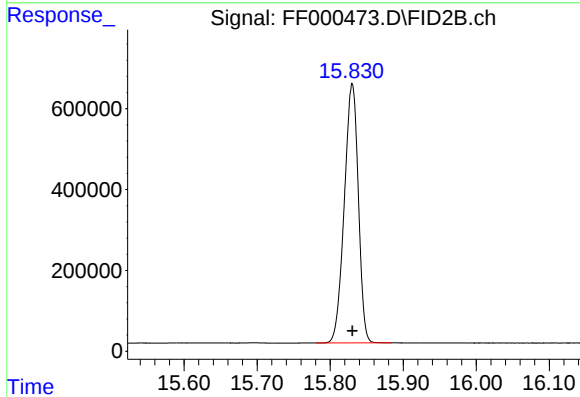

#11 N-HEXACOSANE

R.T.: 15.830 min
Delta R.T.: 0.000 min
Response: 8559330
Conc: 53.86 ug/ml

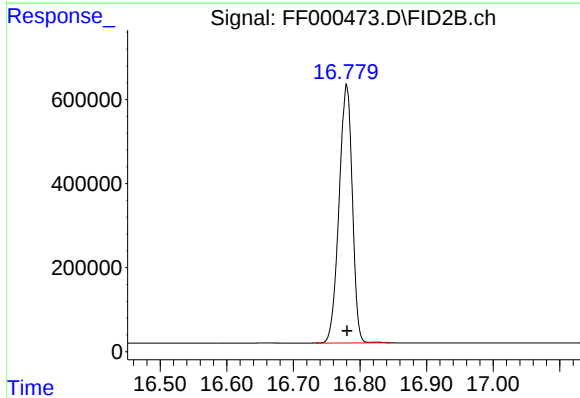

#12 N-OCTACOSANE

R.T.: 16.780 min
Delta R.T.: 0.000 min
Response: 8515468
Conc: 54.09 ug/ml