

Data Path : P:\HPCHEM1\FID_F\Data\FF042518\
 Data File : FF000480.D
 Signal(s) : FID2B.ch
 Acq On : 25 Apr 2018 16:20
 Operator : UA\AJ
 Sample : PB108590BS
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Apr 26 04:19:16 2018
 Quant Method : P:\HPCHEM1\FID_F\Method\FF042318.M
 Quant Title :
 QLast Update : Mon Apr 23 18:07:21 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.608	2392713	16.688 ug/ml
Target Compounds				
2)	N-DECANE	4.353	2873022	18.040 ug/ml
3)	N-DODECANE	6.369	2967392	18.451 ug/ml
4)	N-TETRADECANE	8.162	3035593	18.682 ug/ml
5)	N-HEXADECANE	9.761	3086556	18.807 ug/ml
6)	N-OCTADECANE	11.202	3095874	18.751 ug/ml
7)	N-EICOSANE	12.511	3035663	18.447 ug/ml
8)	N-DOCOSANE	13.709	2958628	18.126 ug/ml
10)	N-TETRACOSANE	14.810	2861331	17.775 ug/ml
11)	N-HEXACOSANE	15.831	2773126	17.449 ug/ml
12)	N-OCTACOSANE	16.781	2680414	17.027 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : P:\HPCHEM1\FID_F\Data\FF042518\
Data File : FF000480.D
Signal(s) : FID2B.ch
Acq On : 25 Apr 2018 16:20
Operator : UA\AJ
Sample : PB108590BS
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Apr 26 04:19:16 2018
Quant Method : P:\HPCHEM1\FID_F\Method\FF042318.M
Quant Title :
QLast Update : Mon Apr 23 18:07:21 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

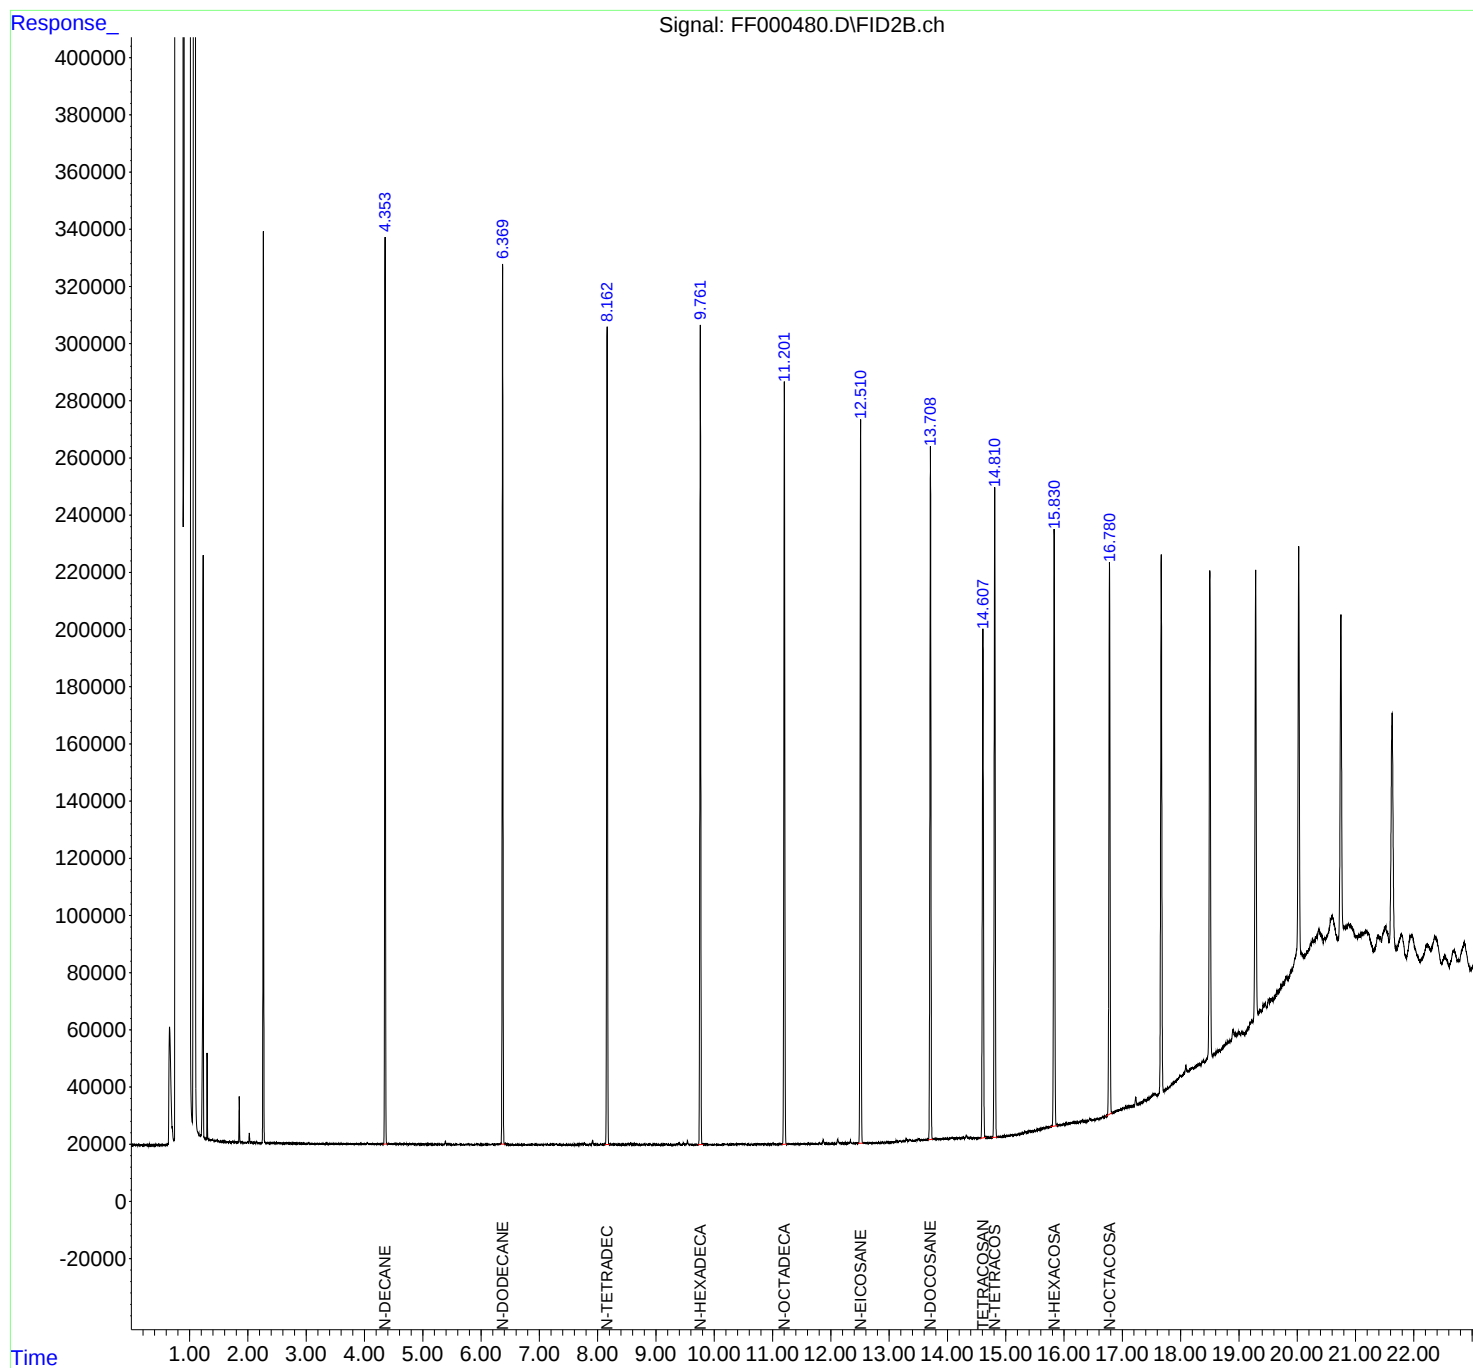

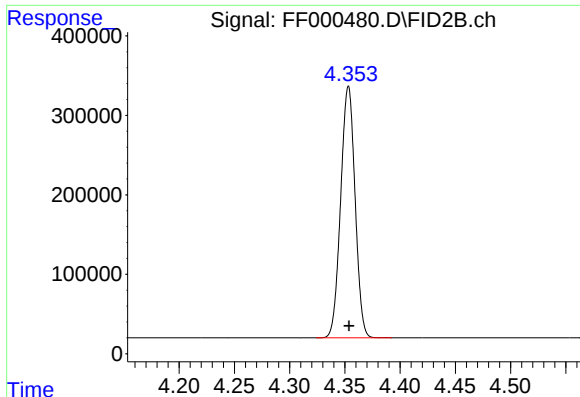


#2 N-DECANE

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 2873022
Conc: 18.04 ug/ml

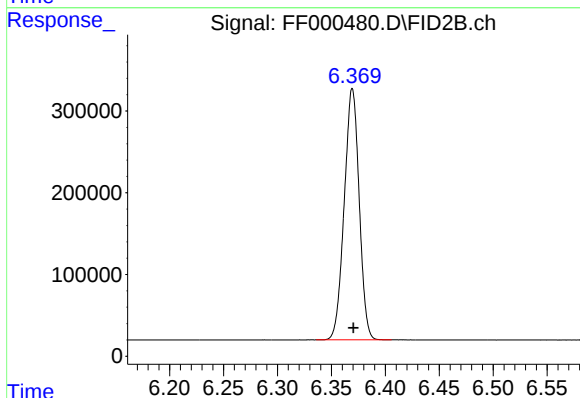


#3 N-DODECANE

R.T.: 6.369 min
Delta R.T.: 0.000 min
Response: 2967392
Conc: 18.45 ug/ml

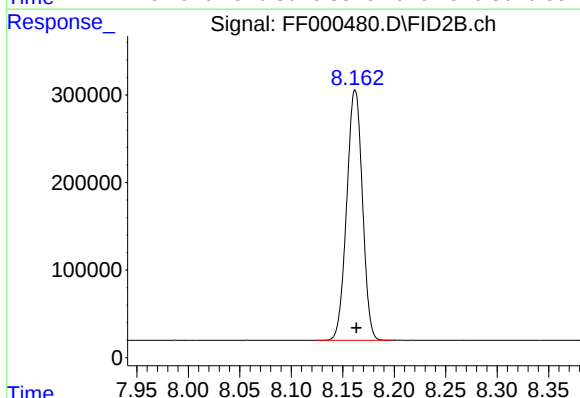


#4 N-TETRADECANE

R.T.: 8.162 min
Delta R.T.: -0.001 min
Response: 3035593
Conc: 18.68 ug/ml

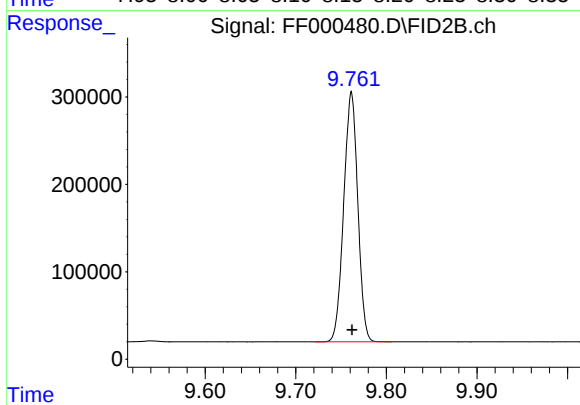


#5 N-HEXADECANE

R.T.: 9.761 min
Delta R.T.: 0.000 min
Response: 3086556
Conc: 18.81 ug/ml

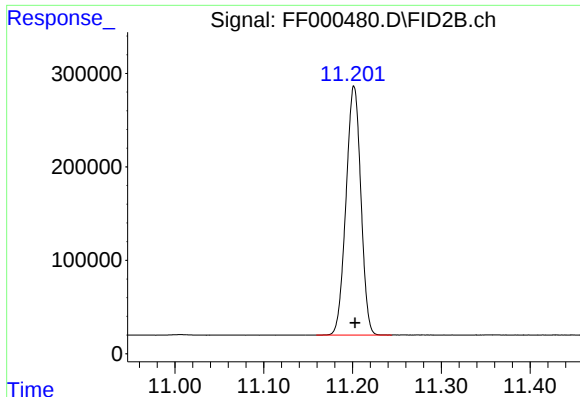


#6 N-OCTADECANE

R.T.: 11.202 min
Delta R.T.: -0.001 min
Response: 3095874
Conc: 18.75 ug/ml

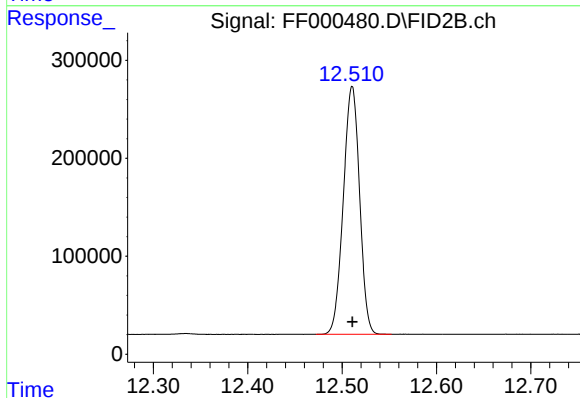


#7 N-EICOSANE

R.T.: 12.511 min
Delta R.T.: 0.000 min
Response: 3035663
Conc: 18.45 ug/ml

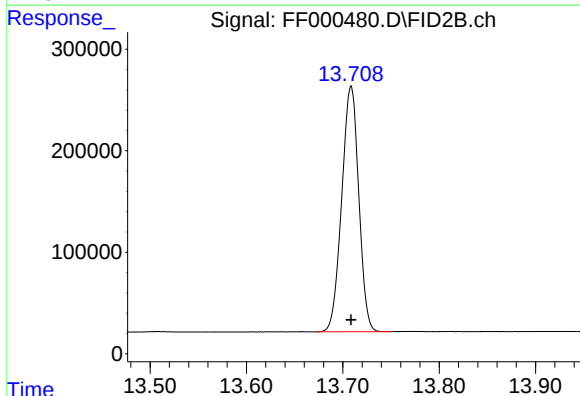


#8 N-DOCOSANE

R.T.: 13.709 min
Delta R.T.: 0.000 min
Response: 2958628
Conc: 18.13 ug/ml

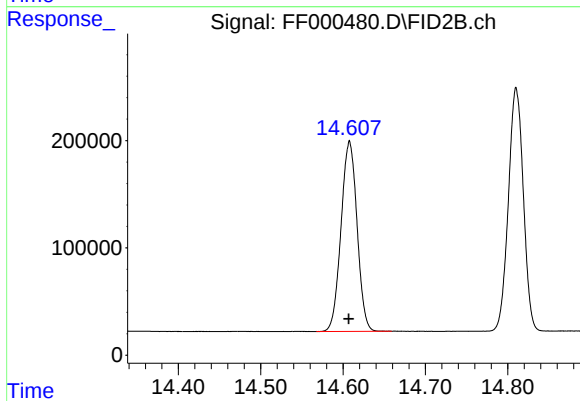


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.608 min
Delta R.T.: 0.000 min
Response: 2392713
Conc: 16.69 ug/ml

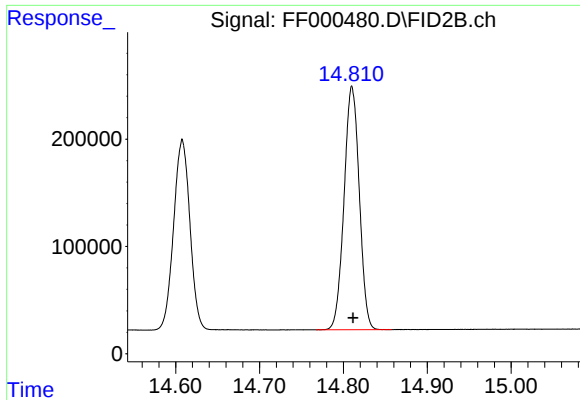


#10 N-TETRACOSANE

R.T.: 14.810 min
Delta R.T.: -0.001 min
Response: 2861331
Conc: 17.78 ug/ml

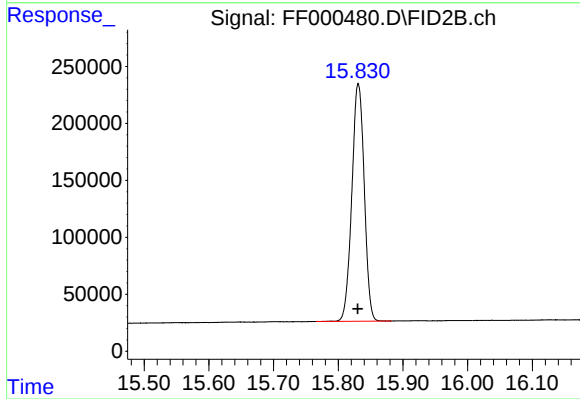

#11 N-HEXACOSANE

R.T.: 15.831 min
Delta R.T.: 0.000 min
Response: 2773126
Conc: 17.45 ug/ml

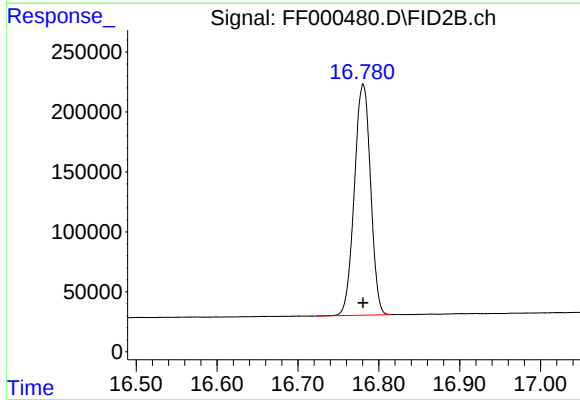

#12 N-OCTACOSANE

R.T.: 16.781 min
Delta R.T.: 0.000 min
Response: 2680414
Conc: 17.03 ug/ml