

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070618\
 Data File : FF001234.D
 Signal(s) : FID2B.ch
 Acq On : 06 Jul 2018 13:22
 Operator : UA\AJ
 Sample : PB110880BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 07 00:55:30 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.469	2215776	20.569 ug/ml
Target Compounds			
2) N-DECANE	4.228	1962224	15.804 ug/ml
3) N-DODECANE	6.241	2254905	17.996 ug/ml
4) N-TETRADECANE	8.030	2553234	20.301 ug/ml
5) N-HEXADECANE	9.628	2664121	21.323 ug/ml
6) N-OCTADECANE	11.066	2701095	21.553 ug/ml
7) N-EICOSANE	12.373	2678412	21.532 ug/ml
8) N-DOCOSANE	13.570	2608763	21.156 ug/ml
10) N-TETRACOSANE	14.671	2647063	21.714 ug/ml
11) N-HEXACOSANE	15.691	2559374	21.115 ug/mlm
12) N-OCTACOSANE	16.640	2512706	20.857 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070618\
Data File : FF001234.D
Signal(s) : FID2B.ch
Acq On : 06 Jul 2018 13:22
Operator : UA\AJ
Sample : PB110880BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 07 00:55:30 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

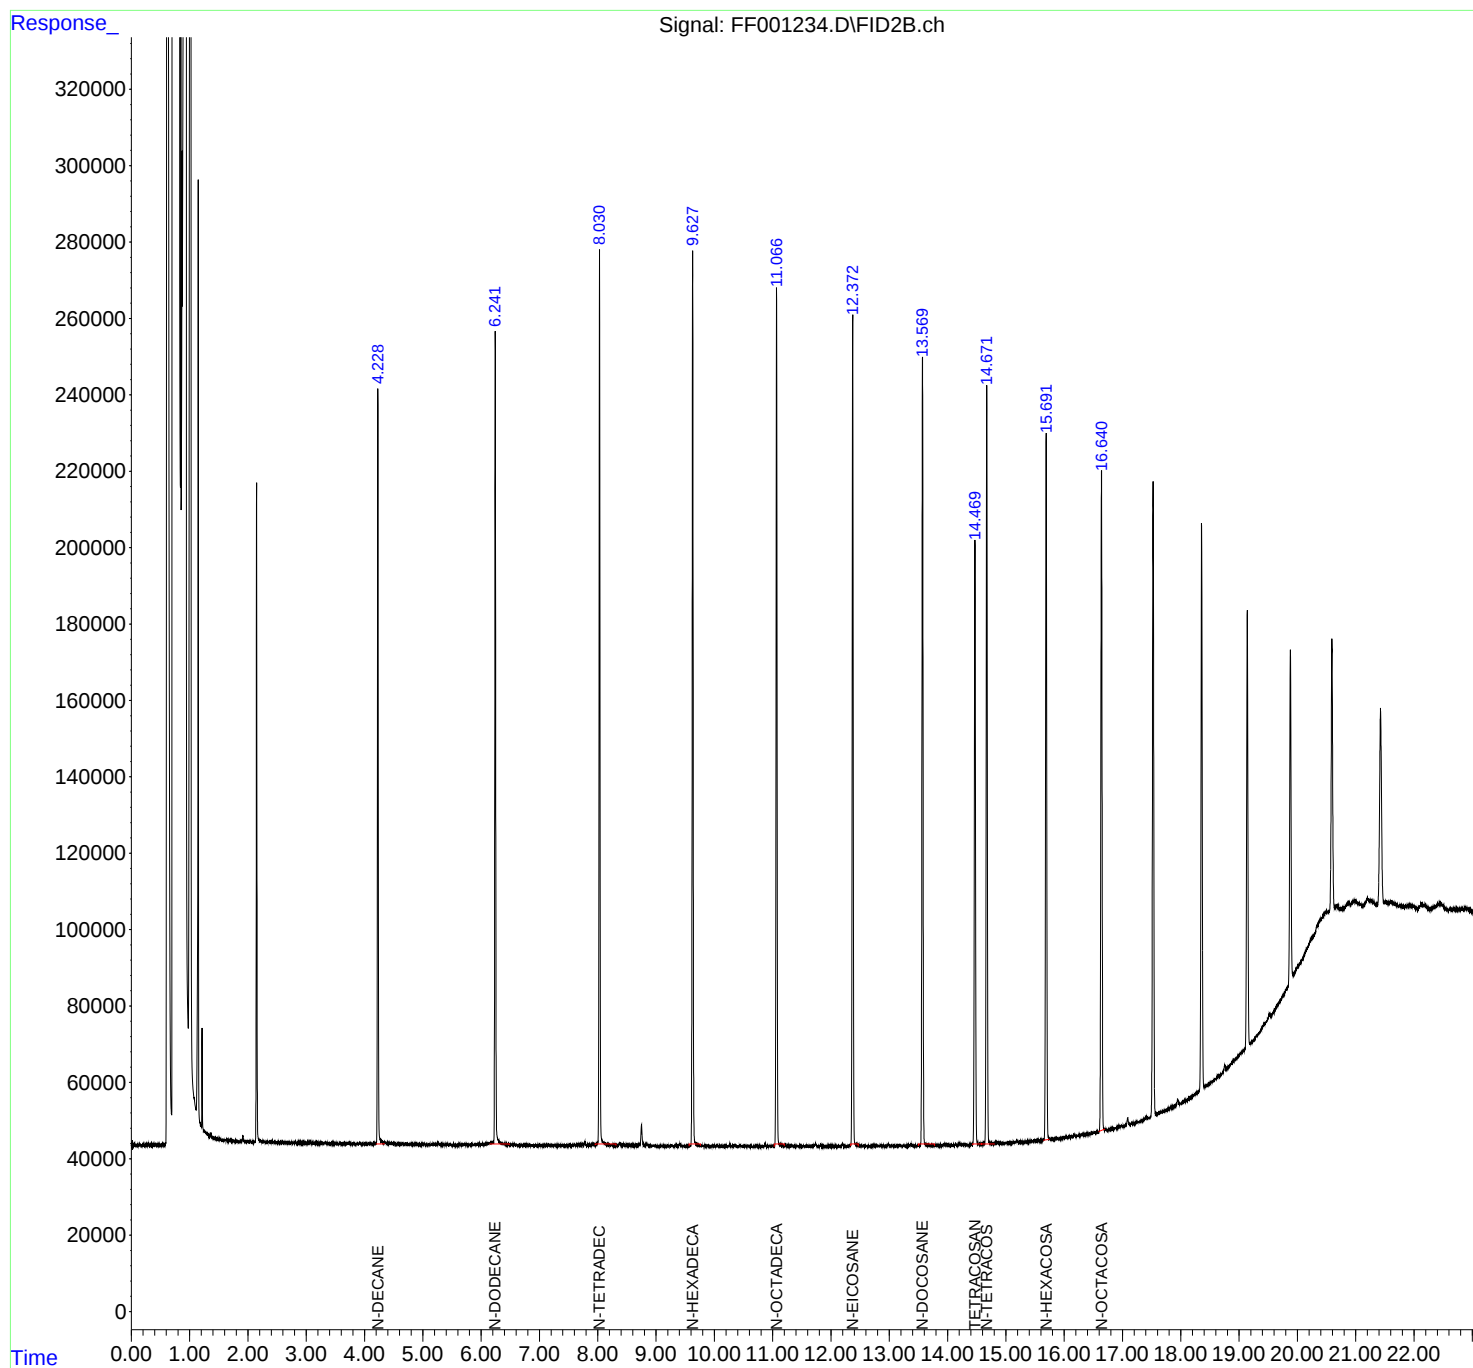

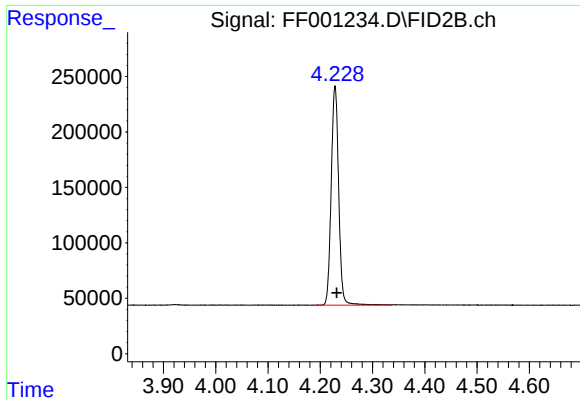


#2 N-DECANE

R.T.: 4.228 min
Delta R.T.: -0.003 min
Response: 1962224
Conc: 15.80 ug/ml

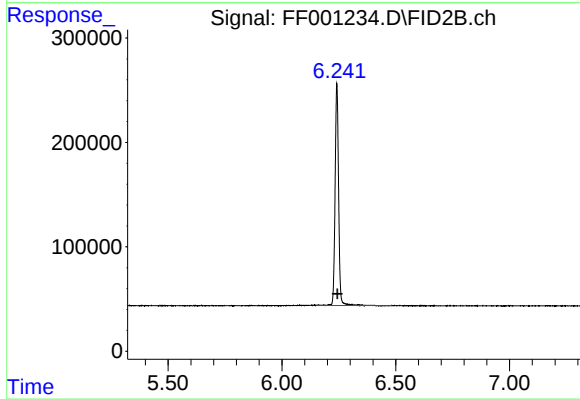


#3 N-DODECANE

R.T.: 6.241 min
Delta R.T.: -0.003 min
Response: 2254905
Conc: 18.00 ug/ml

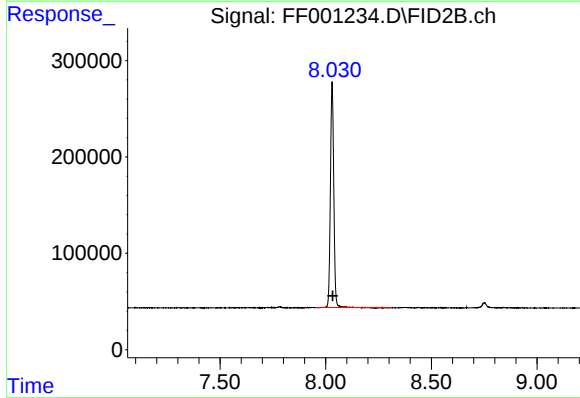


#4 N-TETRADECANE

R.T.: 8.030 min
Delta R.T.: -0.002 min
Response: 2553234
Conc: 20.30 ug/ml

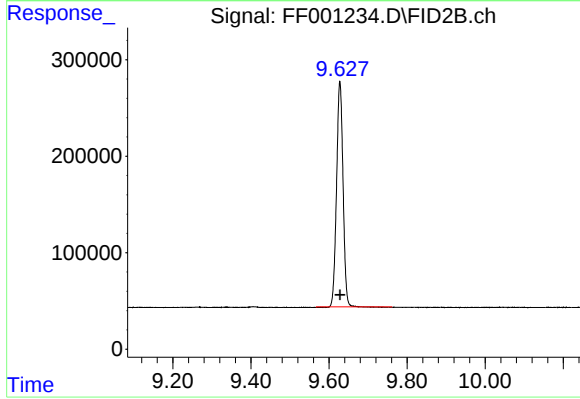


#5 N-HEXADECANE

R.T.: 9.628 min
Delta R.T.: 0.000 min
Response: 2664121
Conc: 21.32 ug/ml

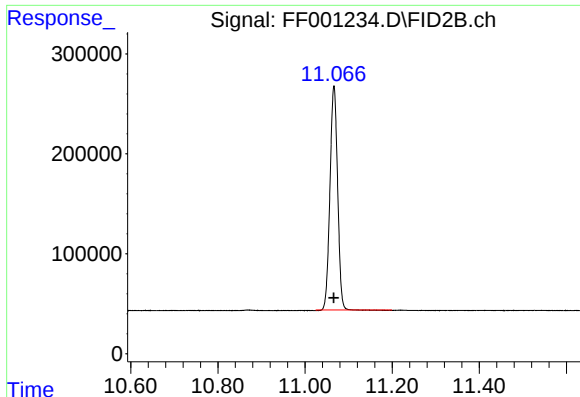


#6 N-OCTADECANE

R.T.: 11.066 min
Delta R.T.: 0.000 min
Response: 2701095
Conc: 21.55 ug/ml

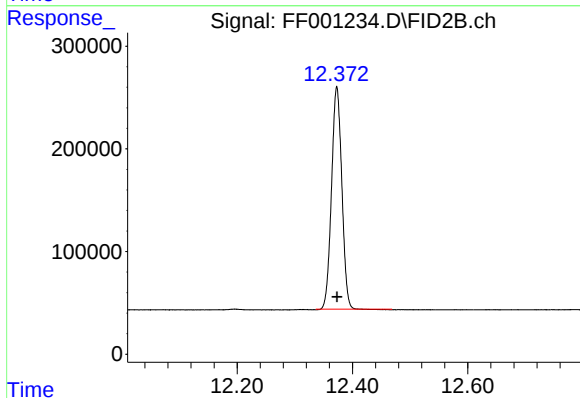


#7 N-EICOSANE

R.T.: 12.373 min
Delta R.T.: 0.000 min
Response: 2678412
Conc: 21.53 ug/ml

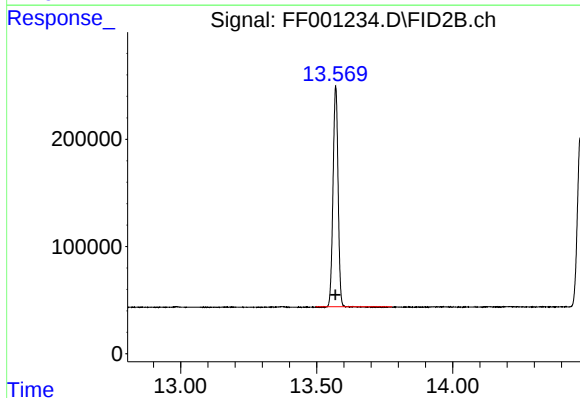


#8 N-DOCOSANE

R.T.: 13.570 min
Delta R.T.: 0.001 min
Response: 2608763
Conc: 21.16 ug/ml

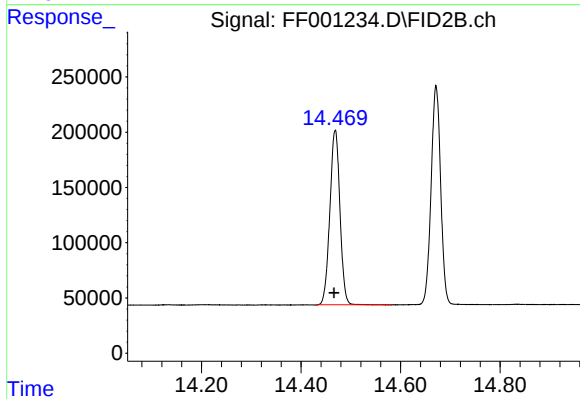


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.469 min
Delta R.T.: 0.002 min
Response: 2215776
Conc: 20.57 ug/ml

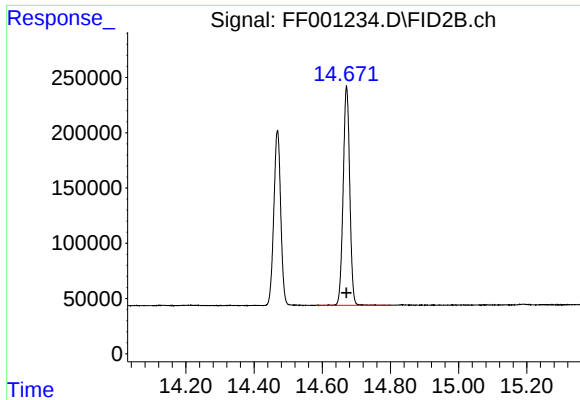


#10 N-TETRACOSANE

R.T.: 14.671 min
Delta R.T.: 0.000 min
Response: 2647063
Conc: 21.71 ug/ml

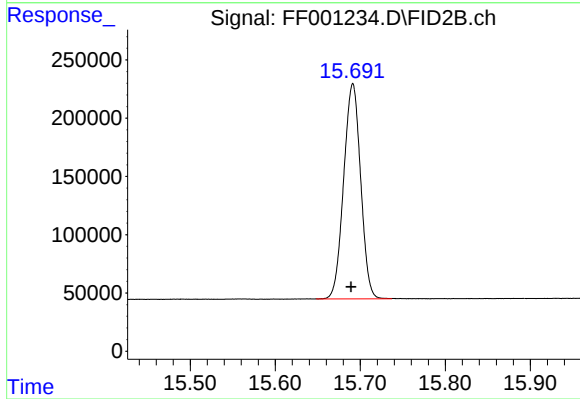

#11 N-HEXACOSANE

R.T.: 15.691 min
Delta R.T.: 0.002 min
Response: 2559374
Conc: 21.11 ug/ml m

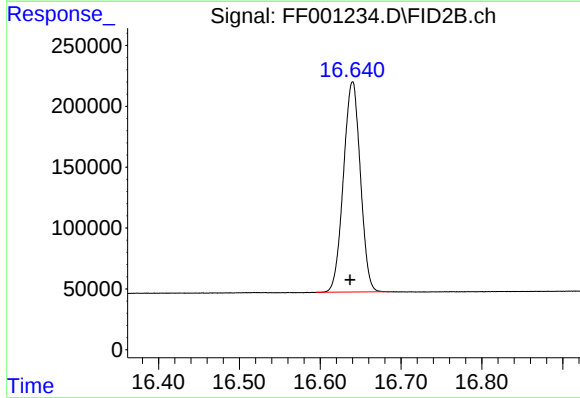

#12 N-OCTACOSANE

R.T.: 16.640 min
Delta R.T.: 0.003 min
Response: 2512706
Conc: 20.86 ug/ml m