

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070618\
 Data File : FF001240.D
 Signal(s) : FID2B.ch
 Acq On : 06 Jul 2018 16:29
 Operator : UA\AJ
 Sample : J3868-02MSD
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 07 00:57:03 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.466	1428175	13.258 ug/mlm
Target Compounds			
2) N-DECANE	4.229	1509806	12.160 ug/ml
3) N-DODECANE	6.242	1520092	12.131 ug/ml
4) N-TETRADECANE	8.030	1571633	12.496 ug/mlm
5) N-HEXADECANE	9.627	1569083	12.558 ug/ml
6) N-OCTADECANE	11.065	1578147	12.593 ug/mlm
7) N-EICOSANE	12.372	1563581	12.570 ug/mlm
8) N-DOCOSANE	13.569	1555859	12.617 ug/mlm
10) N-TETRACOSANE	14.669	1667703	13.680 ug/mlm
11) N-HEXACOSANE	15.689	1651720	13.626 ug/mlm
12) N-OCTACOSANE	16.638	1683893	13.977 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF070618\
Data File : FF001240.D
Signal(s) : FID2B.ch
Acq On : 06 Jul 2018 16:29
Operator : UA\AJ
Sample : J3868-02MSD
Misc :
ALS Vial : 62 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 07 00:57:03 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

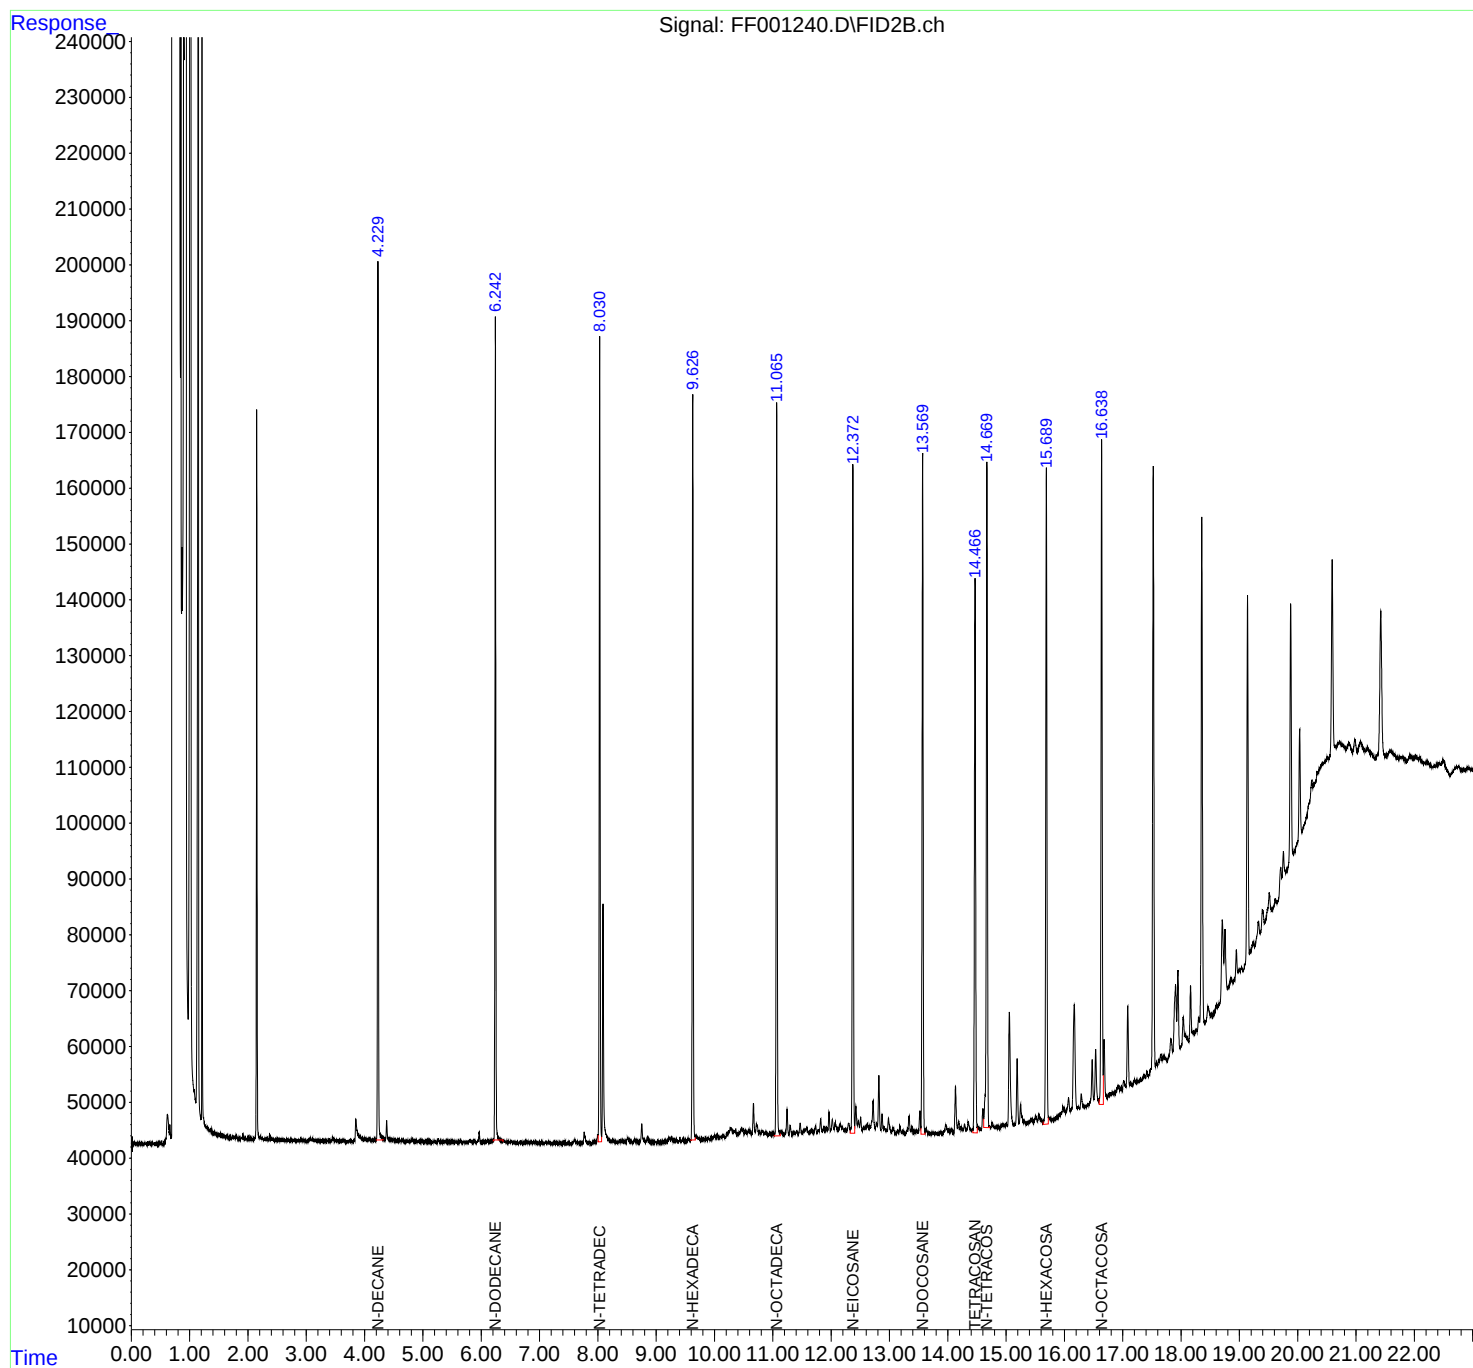

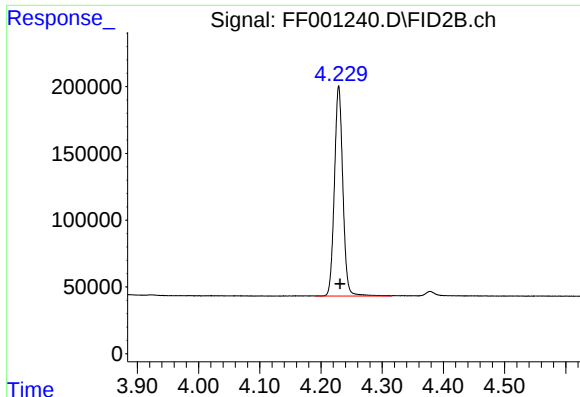


#2 N-DECANE

R.T.: 4.229 min
Delta R.T.: -0.002 min
Response: 1509806
Conc: 12.16 ug/ml

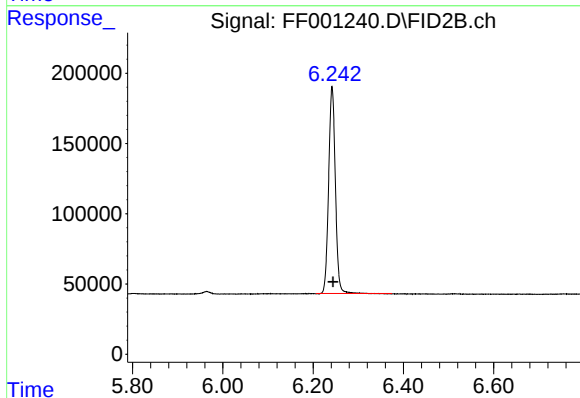


#3 N-DODECANE

R.T.: 6.242 min
Delta R.T.: -0.002 min
Response: 1520092
Conc: 12.13 ug/ml

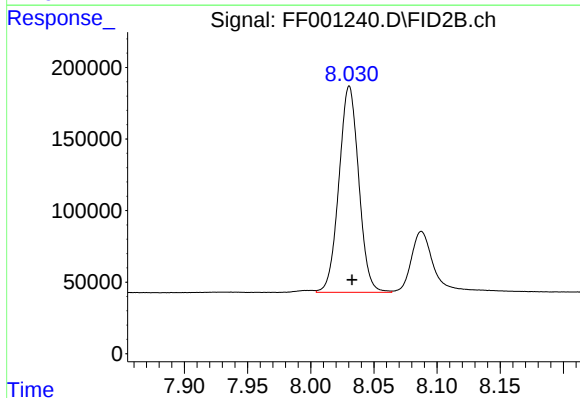


#4 N-TETRADECANE

R.T.: 8.030 min
Delta R.T.: -0.003 min
Response: 1571633
Conc: 12.50 ug/ml m

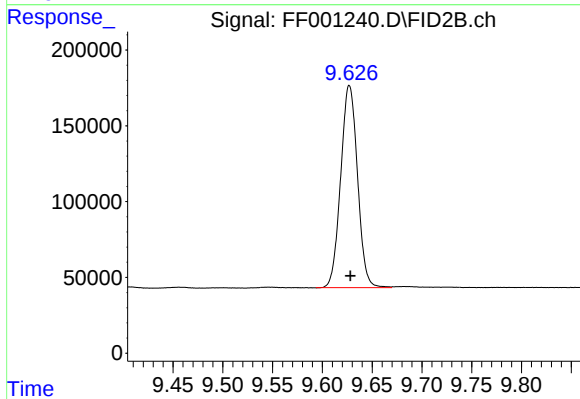


#5 N-HEXADECANE

R.T.: 9.627 min
Delta R.T.: -0.001 min
Response: 1569083
Conc: 12.56 ug/ml

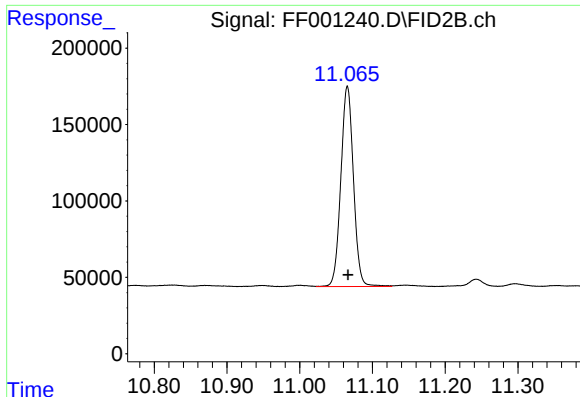


#6 N-OCTADECANE

R.T.: 11.065 min
Delta R.T.: -0.001 min
Response: 1578147
Conc: 12.59 ug/ml m

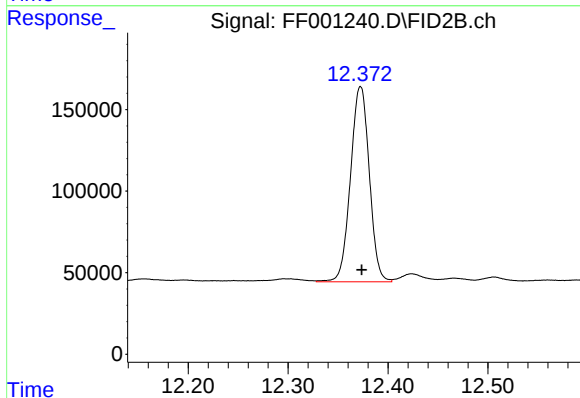


#7 N-EICOSANE

R.T.: 12.372 min
Delta R.T.: -0.002 min
Response: 1563581
Conc: 12.57 ug/ml m

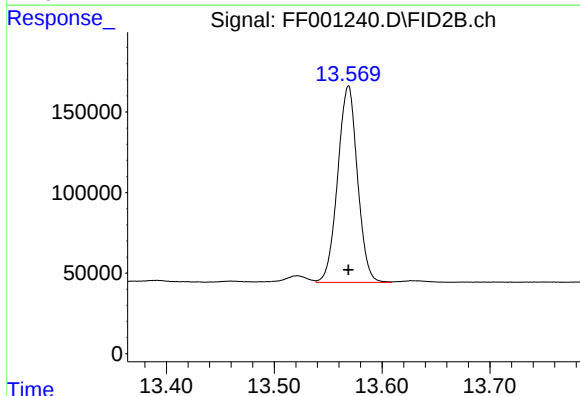


#8 N-DOCOSANE

R.T.: 13.569 min
Delta R.T.: 0.000 min
Response: 1555859
Conc: 12.62 ug/ml m

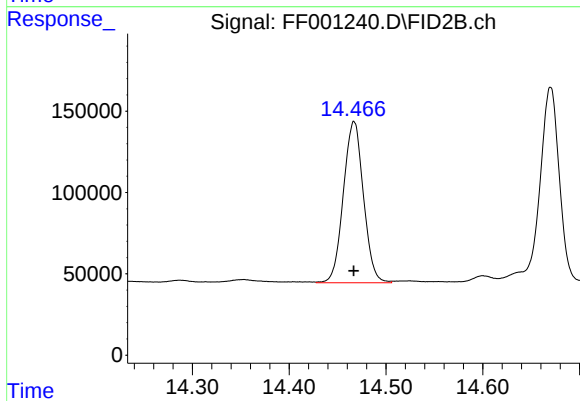


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.466 min
Delta R.T.: 0.000 min
Response: 1428175
Conc: 13.26 ug/ml m

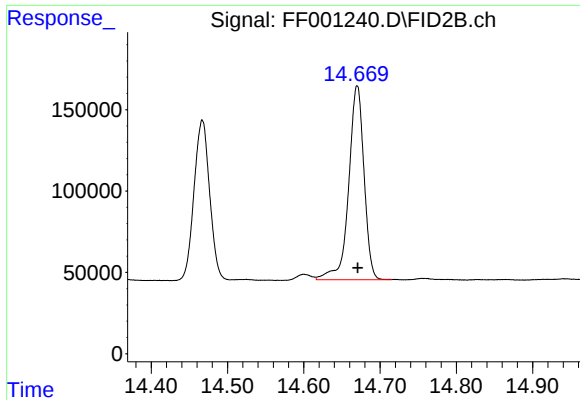


#10 N-TETRACOSANE

R.T.: 14.669 min
Delta R.T.: -0.001 min
Response: 1667703
Conc: 13.68 ug/ml m

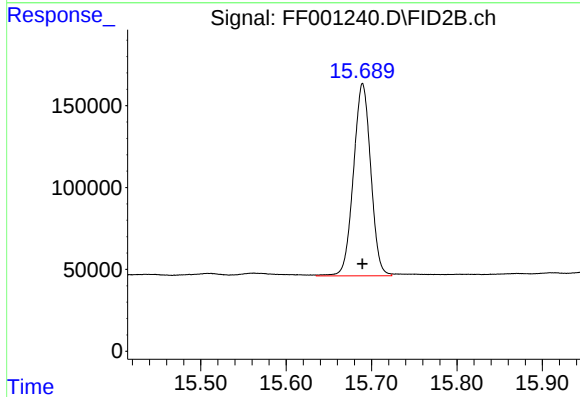

#11 N-HEXACOSANE

R.T.: 15.689 min
Delta R.T.: 0.000 min
Response: 1651720
Conc: 13.63 ug/ml m

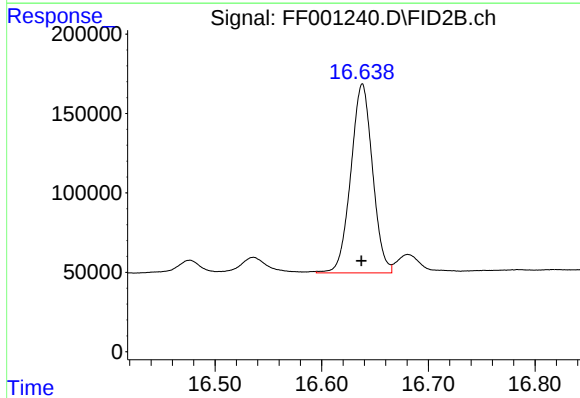

#12 N-OCTACOSANE

R.T.: 16.638 min
Delta R.T.: 0.000 min
Response: 1683893
Conc: 13.98 ug/ml m