

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071718\
 Data File : FF001394.D
 Signal(s) : FID2B.ch
 Acq On : 17 Jul 2018 14:56
 Operator : AJ\SJ
 Sample : PB111135BS
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 17 16:23:19 2018
 Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
 Quant Title :
 QLast Update : Mon Jul 02 13:42:46 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.458	2385910	22.148 ug/ml
Target Compounds			
2) N-DECANE	4.221	2988361	24.069 ug/ml
3) N-DODECANE	6.234	3057934	24.404 ug/ml
4) N-TETRADECANE	8.023	3093628	24.598 ug/ml
5) N-HEXADECANE	9.619	3080555	24.656 ug/ml
6) N-OCTADECANE	11.058	3082187	24.594 ug/ml
7) N-EICOSANE	12.364	3060618	24.605 ug/ml
8) N-DOCOSANE	13.560	3054358	24.770 ug/ml
10) N-TETRACOSANE	14.662	3073249	25.210 ug/ml
11) N-HEXACOSANE	15.682	3039290	25.074 ug/ml
12) N-OCTACOSANE	16.630	3066277	25.452 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF071718\
Data File : FF001394.D
Signal(s) : FID2B.ch
Acq On : 17 Jul 2018 14:56
Operator : AJ\SJ
Sample : PB111135BS
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 17 16:23:19 2018
Quant Method : Z:\PESTPCBSRV\HPCHEM1\FID_F\Method\FF070218.M
Quant Title :
QLast Update : Mon Jul 02 13:42:46 2018
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

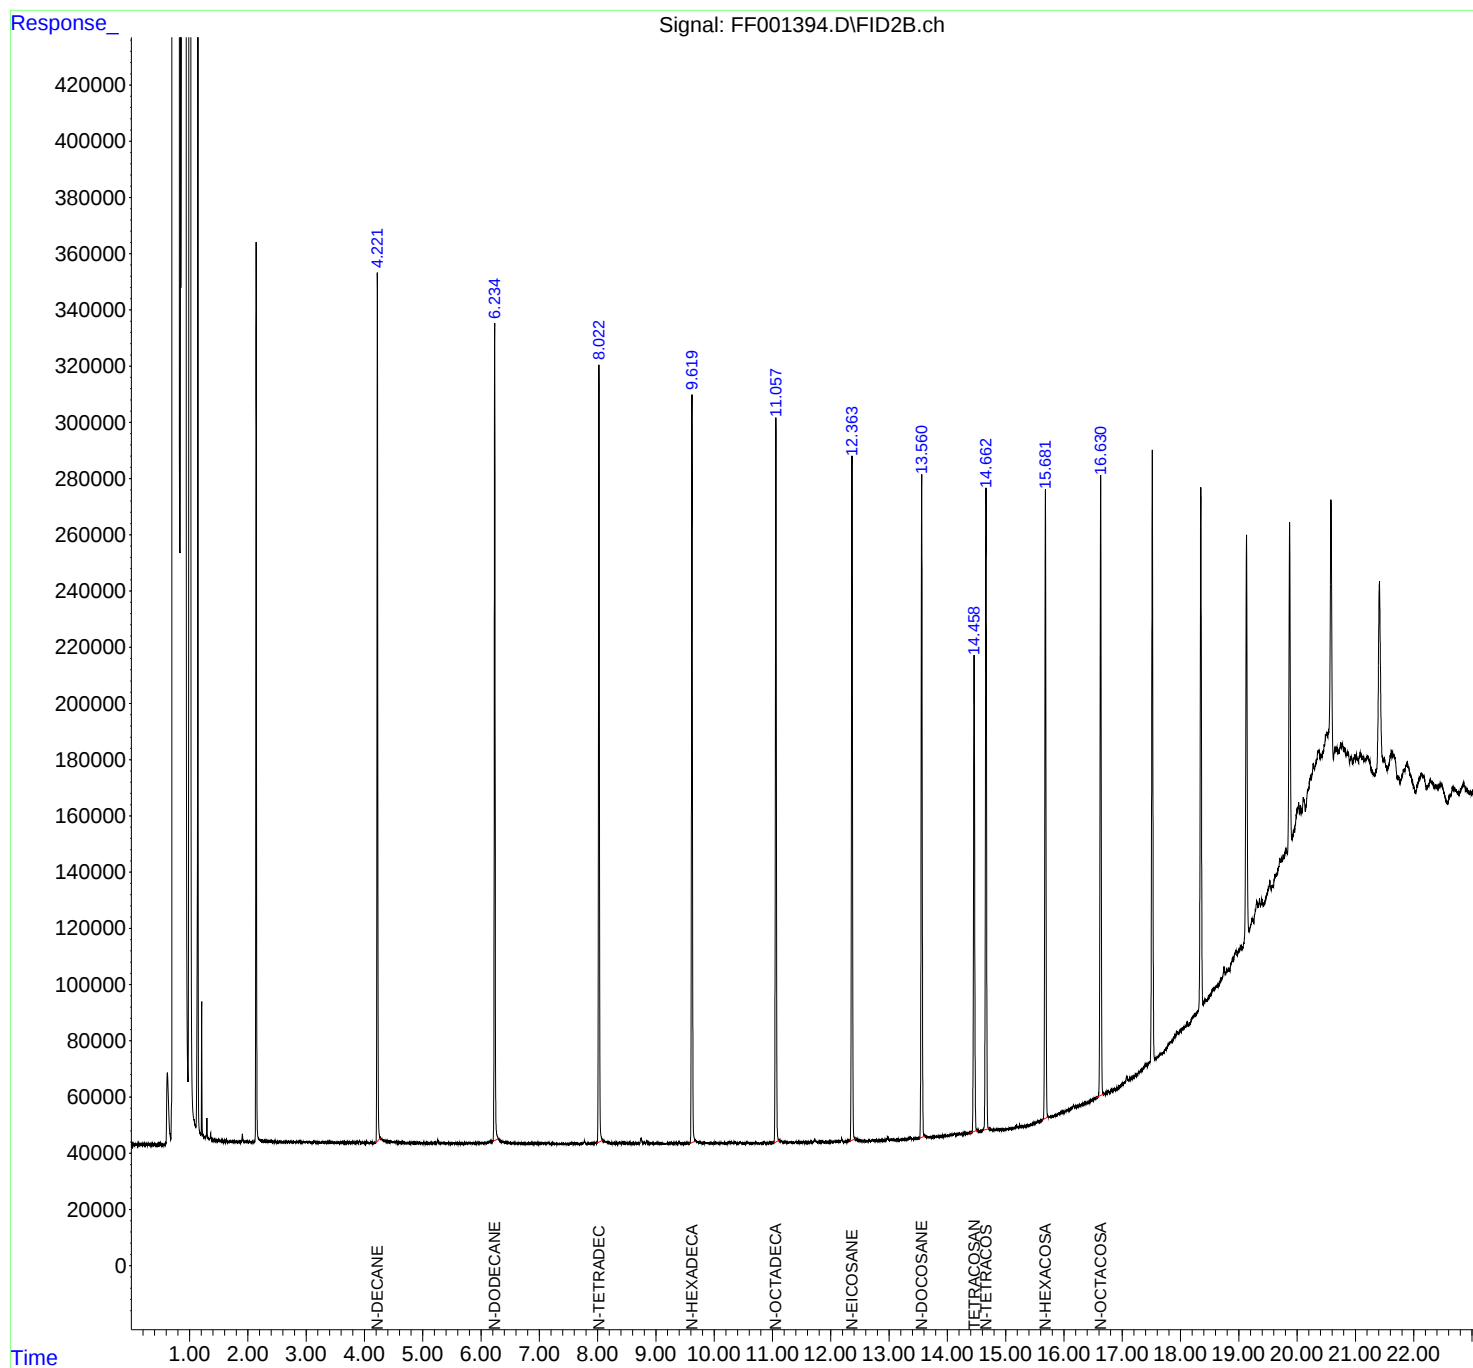

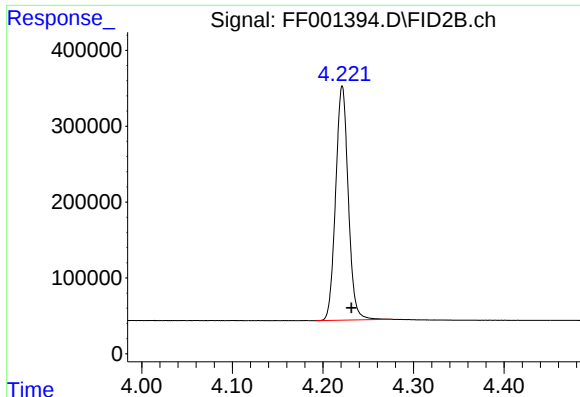


#2 N-DECANE

R.T.: 4.221 min
Delta R.T.: -0.010 min
Response: 2988361
Conc: 24.07 ug/ml

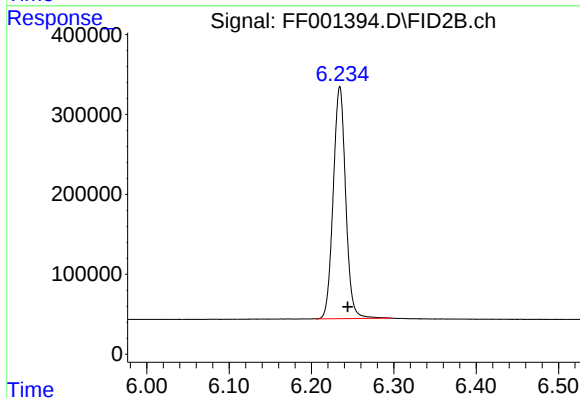


#3 N-DODECANE

R.T.: 6.234 min
Delta R.T.: -0.010 min
Response: 3057934
Conc: 24.40 ug/ml

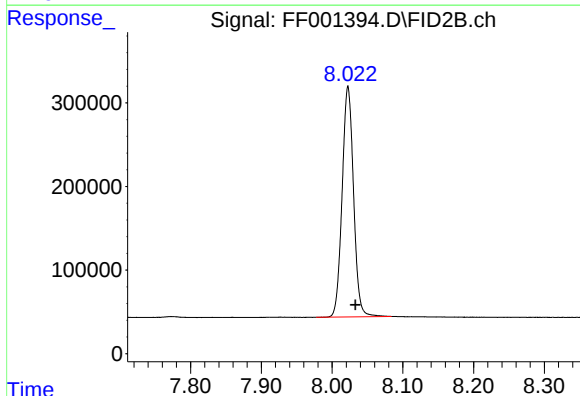


#4 N-TETRADECANE

R.T.: 8.023 min
Delta R.T.: -0.010 min
Response: 3093628
Conc: 24.60 ug/ml

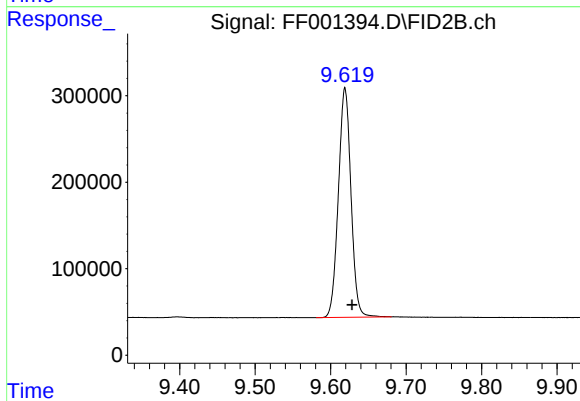


#5 N-HEXADECANE

R.T.: 9.619 min
Delta R.T.: -0.009 min
Response: 3080555
Conc: 24.66 ug/ml

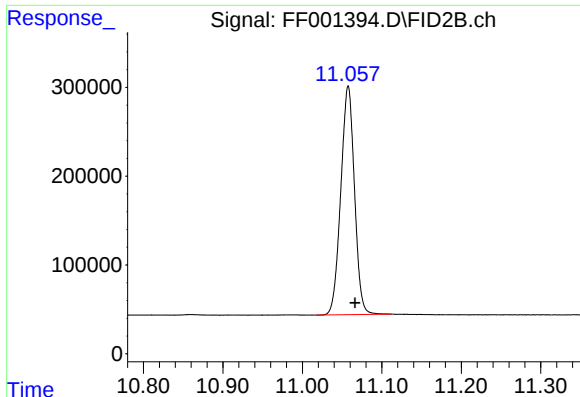


#6 N-OCTADECANE

R.T.: 11.058 min
Delta R.T.: -0.009 min
Response: 3082187
Conc: 24.59 ug/ml

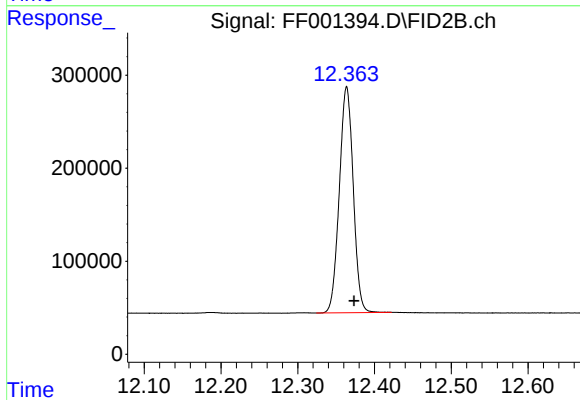


#7 N-EICOSANE

R.T.: 12.364 min
Delta R.T.: -0.010 min
Response: 3060618
Conc: 24.60 ug/ml

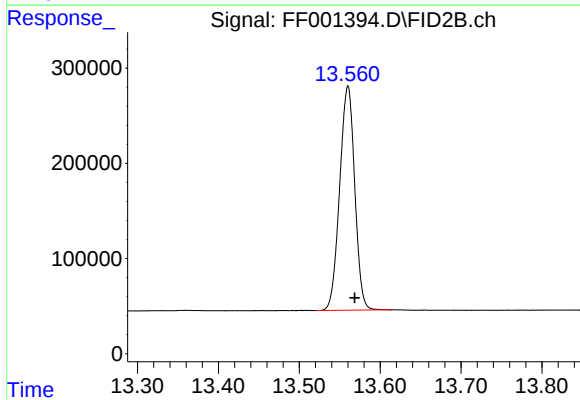


#8 N-DOCOSANE

R.T.: 13.560 min
Delta R.T.: -0.008 min
Response: 3054358
Conc: 24.77 ug/ml

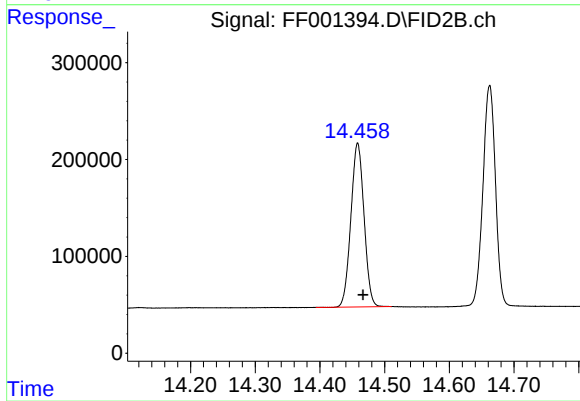


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.458 min
Delta R.T.: -0.008 min
Response: 2385910
Conc: 22.15 ug/ml

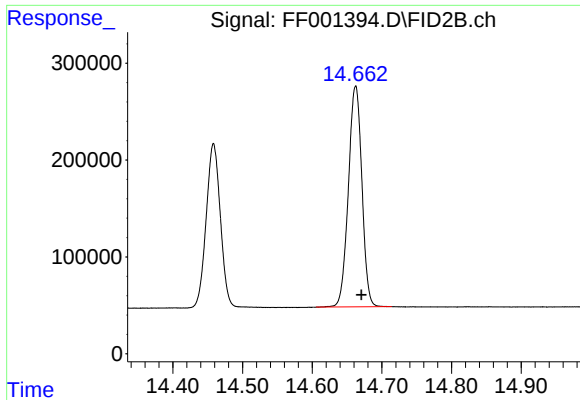


#10 N-TETRACOSANE

R.T.: 14.662 min
Delta R.T.: -0.008 min
Response: 3073249
Conc: 25.21 ug/ml

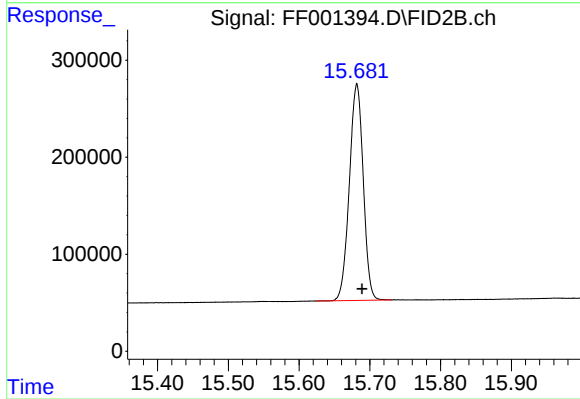

#11 N-HEXACOSANE

R.T.: 15.682 min
Delta R.T.: -0.008 min
Response: 3039290
Conc: 25.07 ug/ml

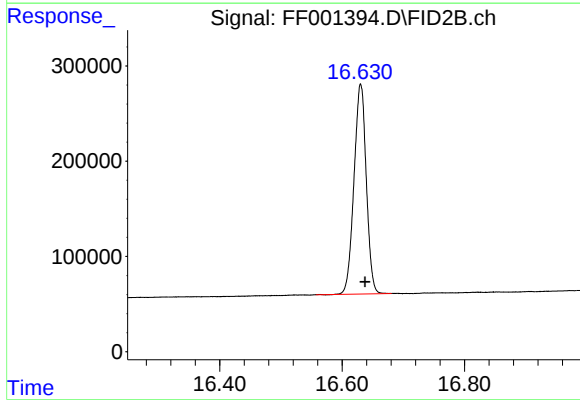

#12 N-OCTACOSANE

R.T.: 16.630 min
Delta R.T.: -0.007 min
Response: 3066277
Conc: 25.45 ug/ml