


L3100131

7470A

INSTRUMENT ID: CYZ

Linear

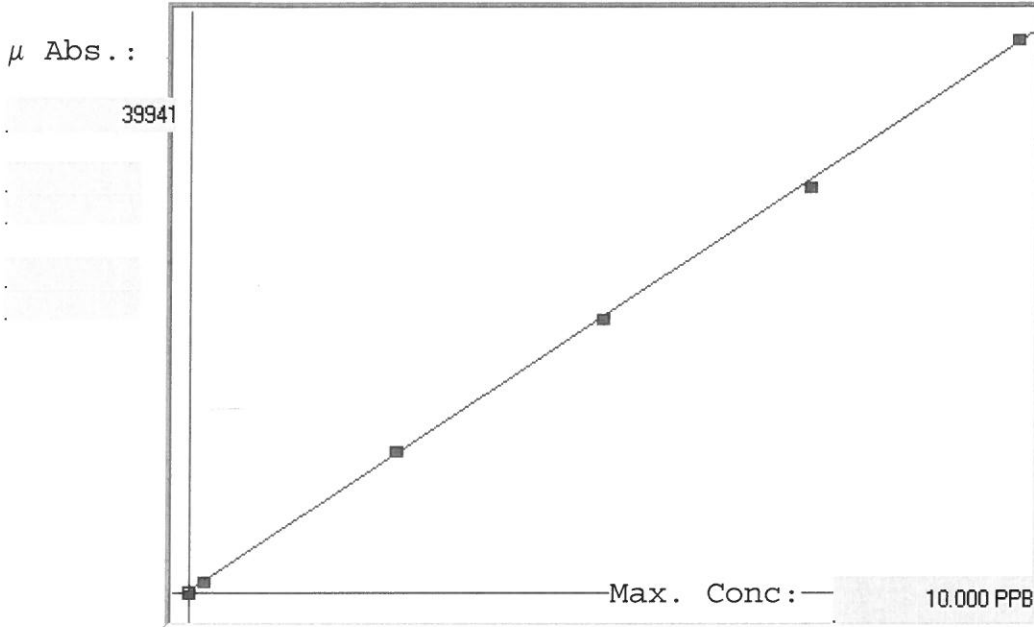

A= 0.0000e+000

B= 2.5257e-004

C= -1.8985e-002

Rho= 0.9998531

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.013	-0.013	25	0.000	25				
0.2	0.200	0.191	-0.009	830	0.0 %	830				
2.5	2.500	2.584	0.084	10307	0.0 %	10307				
5.0	5.000	4.975	-0.025	19774	0.0 %	19774				
7.5	7.500	7.394	-0.106	29349	0.0 %	29349				
10.0	10.000	10.069	0.069	39941	0.0 %	39941	0			

LB100131 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 03 Jan 2019 11:13:48

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	25	-	0.0000	7470A	PPB	03 Jan 2019 11:16:05	S	Std
0.2 - 1	50.2	830	-	0.2000	7470A	PPB	03 Jan 2019 11:18:14	S	Std
2.5 - 1	52.5	10307	-	2.5000	7470A	PPB	03 Jan 2019 11:20:22	S	Std
5.0 - 1	55	19774	-	5.0000	7470A	PPB	03 Jan 2019 11:22:31	S	Std
7.5 - 1	57.5	29349	-	7.5000	7470A	PPB	03 Jan 2019 11:24:39	S	Std
10.0 - 1	51.0	39941	-	10.0000	7470A	PPB	03 Jan 2019 11:26:47	S	Std
ICV49 - 1	ICV49	14969	3.7617	-	7470A	PPB	03 Jan 2019 11:29:30	U	SMPL
ICB49 - 1	ICB49	-32	-0.0271	-	7470A	PPB	03 Jan 2019 11:31:36	U	SMPL
CCV45 - 1	CCV45	19315	4.8594	-	7470A	PPB	03 Jan 2019 11:33:43	U	SMPL
CCB45 - 1	CCB45	-49	-0.0314	-	7470A	PPB	03 Jan 2019 11:35:50	U	SMPL
CRA - 1	CRA	782	0.1785	-	7470A	PPB	03 Jan 2019 11:37:57	U	SMPL
HighStd - 1	HighStd	37517	9.4566	-	7470A	PPB	03 Jan 2019 11:40:04	U	SMPL
ChkStd - 1	ChkStd	27764	6.9933	-	7470A	PPB	03 Jan 2019 11:42:11	U	SMPL
PB116112BL - 1	PBW	-137	-0.0536	-	7470A	PPB	03 Jan 2019 11:48:15	U	SMPL
PB116112BS - 1	LCSW	12923	3.2450	-	7470A	PPB	03 Jan 2019 11:50:22	U	SMPL
J6565-04 - 1	P001-BC010-01	565	0.1237	-	7470A	PPB	03 Jan 2019 11:59:34	U	SMPL
J6565-04DUP - 1	P001-BC010-01DUP	567	0.1242	-	7470A	PPB	03 Jan 2019 12:01:42	U	SMPL
J6565-04MS - 1	P001-BC010-01MS	14655	3.6824	-	7470A	PPB	03 Jan 2019 12:03:51	U	SMPL
J6565-04MSD - 1	P001-BC010-01MSD	14654	3.6822	-	7470A	PPB	03 Jan 2019 12:05:59	U	SMPL
J6565-05 - 1	P001-BC010-02	341	0.0671	-	7470A	PPB	03 Jan 2019 12:08:06	U	SMPL
CCV46 - 1	CCV46	19054	4.7935	-	7470A	PPB	03 Jan 2019 12:10:13	U	SMPL
CCB46 - 1	CCB46	-34	-0.0276	-	7470A	PPB	03 Jan 2019 12:12:20	U	SMPL
J6565-06 - 1	P001-BC011-01	462	0.0977	-	7470A	PPB	03 Jan 2019 12:14:27	U	SMPL
J6566-15 - 1	P001-BC012-01	523	0.1131	-	7470A	PPB	03 Jan 2019 12:16:33	U	SMPL
J6566-16 - 1	P001-BC013-01	559	0.1222	-	7470A	PPB	03 Jan 2019 12:18:40	U	SMPL
J6566-17 - 1	P001-BC014-01	380	0.0770	-	7470A	PPB	03 Jan 2019 12:20:47	U	SMPL
J6566-18 - 1	P001-BC015-01	322	0.0623	-	7470A	PPB	03 Jan 2019 12:22:55	U	SMPL
J6566-19 - 1	P001-BC016-01	344	0.0679	-	7470A	PPB	03 Jan 2019 12:25:03	U	SMPL
J6566-20 - 1	P001-BC017-01	345	0.0682	-	7470A	PPB	03 Jan 2019 12:27:11	U	SMPL
J6566-21 - 1	P001-BC018-01	314	0.0603	-	7470A	PPB	03 Jan 2019 12:29:19	U	SMPL
J6566-22 - 1	P001-BC019-01	346	0.0684	-	7470A	PPB	03 Jan 2019 12:31:28	U	SMPL
J6566-23 - 1	P001-BC020-01	302	0.0573	-	7470A	PPB	03 Jan 2019 12:33:35	U	SMPL
CCV47 - 1	CCV47	19101	4.8053	-	7470A	PPB	03 Jan 2019 12:35:42	U	SMPL
CCB47 - 1	CCB47	-33	-0.0273	-	7470A	PPB	03 Jan 2019 12:37:50	U	SMPL
J6566-24 - 1	P001-BC021-01	266	0.0482	-	7470A	PPB	03 Jan 2019 12:39:57	U	SMPL
J6566-25 - 1	P001-BC022-01	324	0.0628	-	7470A	PPB	03 Jan 2019 12:42:05	U	SMPL
J6566-26 - 1	P001-BC023-01	300	0.0568	-	7470A	PPB	03 Jan 2019 12:44:12	U	SMPL
J6566-27 - 1	P001-BC024-01	281	0.0520	-	7470A	PPB	03 Jan 2019 12:46:19	U	SMPL
J6589-01 - 1	13178	7036	1.7581	-	7470A	PPB	03 Jan 2019 12:48:26	U	SMPL
PB116113BL - 1	PBW	20	-0.0139	-	7470A	PPB	03 Jan 2019 12:50:34	U	SMPL
PB116113BS - 1	LCSW	13371	3.3581	-	7470A	PPB	03 Jan 2019 12:58:42	U	SMPL
J6587-01 - 1	WC-20181227	617	0.1368	-	7470A	PPB	03 Jan 2019 13:00:50	U	SMPL
J6598-01 - 1	MW05_122818	-25	-0.0253	-	7470A	PPB	03 Jan 2019 13:02:59	U	SMPL
J6598-01DUP - 1	MW05_122818DUP	14	-0.0154	-	7470A	PPB	03 Jan 2019 13:05:07	U	SMPL
CCV48 - 1	CCV48	19957	5.0215	-	7470A	PPB	03 Jan 2019 13:14:39	U	SMPL
CCB48 - 1	CCB48	-56	-0.0331	-	7470A	PPB	03 Jan 2019 13:16:46	U	SMPL
J6598-01MS - 1	MW05_122818MS	15515	3.8996	-	7470A	PPB	03 Jan 2019 13:21:20	U	SMPL
J6598-01MSD - 1	MW05_122818MSD	16339	4.1077	-	7470A	PPB	03 Jan 2019 13:23:27	U	SMPL
J6598-02 - 1	B3_122818	80	0.0012	-	7470A	PPB	03 Jan 2019 13:25:34	U	SMPL
J6598-06 - 1	MW05_122818	49	-0.0066	-	7470A	PPB	03 Jan 2019 13:27:42	U	SMPL
J6598-07 - 1	B3_122818	-35	-0.0278	-	7470A	PPB	03 Jan 2019 13:29:49	U	SMPL
PB116112TB - 1	PB116067TB	421	0.0873	-	7470A	PPB	03 Jan 2019 13:31:57	U	SMPL
J6565-04LX5 - 1		100	0.0063	-	7470A	PPB	03 Jan 2019 13:34:05	U	SMPL
J6565-04A - 1		15697	3.9456	-	7470A	PPB	03 Jan 2019 13:36:13	U	SMPL
J6598-01LX5 - 1		-40	-0.0291	-	7470A	PPB	03 Jan 2019 13:38:22	U	SMPL
J6598-01A - 1		16353	4.1113	-	7470A	PPB	03 Jan 2019 13:40:29	U	SMPL
CCV49 - 1	CCV49	19859	4.9968	-	7470A	PPB	03 Jan 2019 13:42:37	U	SMPL
CCB49 - 1	CCB49	-77	-0.0384	-	7470A	PPB	03 Jan 2019 13:44:44	U	SMPL