


LB 100174

ISM02.4

INSTRUMENT ID: CV1

Linear

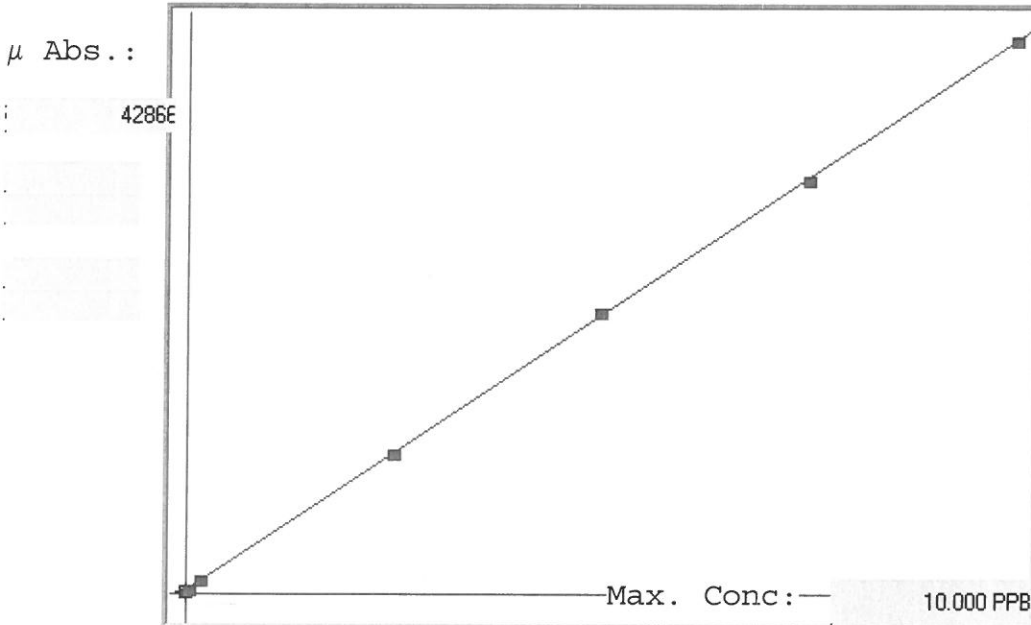

A= 0.0000e+000

B= 2.3433e-004

C= -5.4612e-002

Rho= 0.9999636

Accept=Accepted

*Slope
γ = 1.000036*

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%CD
0.00	0.000	-0.012	-0.012	183	0.000	183					-
0.05	0.050	0.035	-0.015	382	0.0 %	382					-30
0.2	0.200	0.192	-0.008	1051	0.0 %	1051					-4
2.5	2.500	2.514	0.014	10962	0.0 %	10962					1
5.0	5.000	5.069	0.069	21866	0.0 %	21866					-1
7.5	7.500	7.461	-0.039	32074	0.0 %	32074					-1
10.0	10.000	9.990	-0.010	42866	0.0 %	42866					0

*0.00
1/4/19*

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	183	-		0 ISM02.4	PPB	1/4/2019 17:07	Std
	0.05 S0.05	382	-		0.05 ISM02.4	PPB	1/4/2019 17:09	Std
	0.2 S0.2	1051	-		0.2 ISM02.4	PPB	1/4/2019 17:11	Std
	2.5 S2.5	10962	-		2.5 ISM02.4	PPB	1/4/2019 17:14	Std
	5 S5	21866	-		5 ISM02.4	PPB	1/4/2019 17:16	Std
	7.5 S7.5	32074	-		7.5 ISM02.4	PPB	1/4/2019 17:18	Std
	10 S10	42866	-		10 ISM02.4	PPB	1/4/2019 17:24	Std
ICV	ICV	17013	3.9321 -		ISM02.4	PPB	1/4/2019 17:27	SMPL
ICB	ICB	233	0 -		ISM02.4	PPB	1/4/2019 17:32	SMPL
CCV074	CCV074	21597	5.0063 -		ISM02.4	PPB	1/4/2019 17:34	SMPL
CCB074	CCB074	171	-0.0145 -		ISM02.4	PPB	1/4/2019 17:36	SMPL
PB116182BL	PBW182	145	-0.0206 -		ISM02.4	PPB	1/4/2019 17:39	SMPL
J6537-01	MBE803	84543	19.7566 -		ISM02.4	PPB	1/4/2019 17:41	SMPL
J6537-02	MBE803D	77347	18.0703 -		ISM02.4	PPB	1/4/2019 17:43	SMPL
J6537-03	MBE803S	81383	19.0161 -		ISM02.4	PPB	1/4/2019 17:56	SMPL
PB116183BL	PBW183	318	0.0199 -		ISM02.4	PPB	1/4/2019 18:05	SMPL
CCV075	CCV075	21526	4.9896 -		ISM02.4	PPB	1/4/2019 18:14	SMPL
CCB075	CCB075	252	0.0044 -		ISM02.4	PPB	1/4/2019 18:19	SMPL
J6538-01	MBE809	-113	-0.0811 -		ISM02.4	PPB	1/4/2019 18:21	SMPL
J6538-02	MBE809D	-236	-0.1099 -		ISM02.4	PPB	1/4/2019 18:23	SMPL
J6538-03	MBE809S	2058	0.4276 -		ISM02.4	PPB	1/4/2019 18:26	SMPL
J6537-01DLX5	MBE803	42086	9.8075 -		ISM02.4	PPB	1/4/2019 18:28	SMPL
J6537-02DLX5	MBE803D	41560	9.6843 -		ISM02.4	PPB	1/4/2019 18:30	SMPL
J6537-03DLX5	MBE803S	45149	10.5253 -		ISM02.4	PPB	1/4/2019 18:33	SMPL
CCV076	CCV076	20741	4.8057 -		ISM02.4	PPB	1/4/2019 18:35	SMPL
CCB076	CCB076	264	0.0073 -		ISM02.4	PPB	1/4/2019 18:40	SMPL
J6537-01DL2X10	MBE803S	23343	5.4154 -		ISM02.4	PPB	1/4/2019 18:43	SMPL
J6537-02DL2X10	MBE803S	23186	5.3786 -		ISM02.4	PPB	1/4/2019 18:45	SMPL
J6537-03DL2X10	MBE803S	25071	5.8204 -		ISM02.4	PPB	1/4/2019 18:47	SMPL
CCV077	CCV077	21082	4.8856 -		ISM02.4	PPB	1/4/2019 18:50	SMPL
CCB077	CCB077	239	0.0014 -		ISM02.4	PPB	1/4/2019 18:52	SMPL