

LB100222 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin


Date of Analysis: 09 Jan 2019 14:15:10

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	-10	-	0.0000	7471B	PPB	09 Jan 2019 14:21:55	S	Std
0.2 - 1	50.2	1097	-	0.2000	7471B	PPB	09 Jan 2019 14:24:12	S	Std
2.5 - 1	52.5	13485	-	2.5000	7471B	PPB	09 Jan 2019 14:26:30	S	Std
5.0 - 1	55.0	26735	-	5.0000	7471B	PPB	09 Jan 2019 14:28:47	S	Std
7.5 - 1	57.5	40178	-	7.5000	7471B	PPB	09 Jan 2019 14:31:05	S	Std
10.0 - 1	510.0	53022	-	10.0000	7471B	PPB	09 Jan 2019 14:33:22	S	Std
ICV55 - 1	ICV55	20565	3.8514	-	7471B	PPB	09 Jan 2019 14:36:40	U	SMPL
ICB55 - 1	ICB55	-100	-0.0365	-	7471B	PPB	09 Jan 2019 14:38:56	U	SMPL
CCV05 - 1	CCV05	26256	4.9221	-	7471B	PPB	09 Jan 2019 14:41:12	U	SMPL
CCB05 - 1	CCB05	-101	-0.0366	-	7471B	PPB	09 Jan 2019 14:43:28	U	SMPL
CRA - 1	CRA	1058	0.1814	-	7471B	PPB	09 Jan 2019 14:45:45	U	SMPL
HighStd - 1	HighStd	52747	9.9061	-	7471B	PPB	09 Jan 2019 14:48:01	U	SMPL
ChkStd - 1	ChkStd	37472	7.0323	-	7471B	PPB	09 Jan 2019 14:50:17	U	SMPL
PB116252BL - 1	PBS	-101	-0.0366	-	7471B	PPB	09 Jan 2019 14:52:35	U	SMPL
PB116252BS - 1	LCSS	18144	3.3959	-	7471B	PPB	09 Jan 2019 14:54:54	U	SMPL
K1006-01 - 1	JC-03-010819-A	4291	0.7897	-	7471B	PPB	09 Jan 2019 14:57:11	U	SMPL
K1006-03 - 1	JC-03-010819-B	8500	1.5815	-	7471B	PPB	09 Jan 2019 14:59:28	U	SMPL
K1006-05 - 1	JC-03-010819-C	10046	1.8724	-	7471B	PPB	09 Jan 2019 15:01:46	U	SMPL
K1006-07 - 1	JC-03-010819-D	14340	2.6803	-	7471B	PPB	09 Jan 2019 15:04:05	U	SMPL
K1006-09 - 1	JC-03-010819-E	5519	1.0207	-	7471B	PPB	09 Jan 2019 15:06:20	U	SMPL
CCV06 - 1	CCV06	25403	4.7616	-	7471B	PPB	09 Jan 2019 15:08:36	U	SMPL
CCB06 - 1	CCB06	-130	-0.0421	-	7471B	PPB	09 Jan 2019 15:10:52	U	SMPL
K1006-11 - 1	JC-03-010819-F	11274	2.1034	-	7471B	PPB	09 Jan 2019 15:13:10	U	SMPL
K1006-13 - 1	JC-03-010819-G	20844	3.9039	-	7471B	PPB	09 Jan 2019 15:15:26	U	SMPL
K1006-15 - 1	JC-03-010819-H	13136	2.4537	-	7471B	PPB	09 Jan 2019 15:17:42	U	SMPL
K1006-17 - 1	JC-03-010819-I	9974	1.8588	-	7471B	PPB	09 Jan 2019 15:19:59	U	SMPL
K1006-19 - 1	JC-03-010819-J	8405	1.5637	-	7471B	PPB	09 Jan 2019 15:22:16	U	SMPL
K1006-19DUP - 1	JC-03-010819-JDUP	7806	1.4510	-	7471B	PPB	09 Jan 2019 15:24:33	U	SMPL
K1006-19MS - 1	JC-03-010819-JMS	30868	5.7898	-	7471B	PPB	09 Jan 2019 15:33:26	U	SMPL
K1006-19MSD - 1	JC-03-010819-JMSD	29932	5.6137	-	7471B	PPB	09 Jan 2019 15:35:43	U	SMPL
PB116253BL - 1	PBS	-126	-0.0413	-	7471B	PPB	09 Jan 2019 15:38:02	U	SMPL
PB116253BS - 1	LCSS	19636	3.6766	-	7471B	PPB	09 Jan 2019 15:40:19	U	SMPL
CCV07 - 1	CCV07	28380	5.3217	-	7471B	PPB	09 Jan 2019 15:42:35	U	SMPL
CCB07 - 1	CCB07	-114	-0.0391	-	7471B	PPB	09 Jan 2019 15:44:52	U	SMPL
K1008-01 - 1	HD-02-010819	1392	0.2442	-	7471B	PPB	09 Jan 2019 15:47:10	U	SMPL
K1081-04 - 1	SUP-3B-C-1-010819	436	0.0644	-	7471B	PPB	09 Jan 2019 15:49:26	U	SMPL
K1082-01 - 1	SP-1-1	17272	3.2319	-	7471B	PPB	09 Jan 2019 15:51:42	U	SMPL
K1082-03 - 1	SP-1-2	2484	0.4497	-	7471B	PPB	09 Jan 2019 15:53:58	U	SMPL
K1082-05 - 1	SP-1-3	2134	0.3838	-	7471B	PPB	09 Jan 2019 15:56:16	U	SMPL
K1082-07 - 1	SP-1-4	1979	0.3547	-	7471B	PPB	09 Jan 2019 15:58:33	U	SMPL
K1082-09 - 1	SP-1-5	2745	0.4988	-	7471B	PPB	09 Jan 2019 16:00:50	U	SMPL
K1082-11 - 1	SP-1-6	3164	0.5776	-	7471B	PPB	09 Jan 2019 16:03:08	U	SMPL
K1083-01 - 1	OILY-STONES	556	0.0870	-	7471B	PPB	09 Jan 2019 16:05:26	U	SMPL
K1087-01 - 1	MH-448-C	619	0.0988	-	7471B	PPB	09 Jan 2019 16:07:43	U	SMPL
CCV08 - 1	CCV08	29065	5.4506	-	7471B	PPB	09 Jan 2019 16:09:59	U	SMPL
CCB08 - 1	CCB08	-105	-0.0374	-	7471B	PPB	09 Jan 2019 16:12:16	U	SMPL
K1087-01DUP - 1	MH-448-CDUP	725	0.1188	-	7471B	PPB	09 Jan 2019 16:14:33	U	SMPL
K1087-01MS - 1	MH-448-CMS	20873	3.9094	-	7471B	PPB	09 Jan 2019 16:16:49	U	SMPL
K1087-01MSD - 1	MH-448-CMSD	21225	3.9756	-	7471B	PPB	09 Jan 2019 16:19:05	U	SMPL
K1087-05 - 1	MH-447-C	589	0.0932	-	7471B	PPB	09 Jan 2019 16:21:22	U	SMPL
K1087-09 - 1	MH-445-C	1188	0.2059	-	7471B	PPB	09 Jan 2019 16:23:39	U	SMPL
K1006-19LX5 - 1		1806	0.3221	-	7471B	PPB	09 Jan 2019 16:25:56	U	SMPL
K1006-19A - 1		33220	6.2323	-	7471B	PPB	09 Jan 2019 16:28:14	U	SMPL
K1087-01LX5 - 1		-4	-0.0184	-	7471B	PPB	09 Jan 2019 16:30:31	U	SMPL
K1087-01A - 1		24147	4.5253	-	7471B	PPB	09 Jan 2019 16:32:50	U	SMPL
CCV09 - 1	CCV09	28685	5.3791	-	7471B	PPB	09 Jan 2019 16:35:06	U	SMPL
CCB09 - 1	CCB09	-117	-0.0397	-	7471B	PPB	09 Jan 2019 16:37:23	U	SMPL
IDOC1 - 1	IDOC1	18283	3.4221	-	7471B	PPB	09 Jan 2019 16:39:41	U	SMPL
IDOC2 - 1	IDOC2	19475	3.6463	-	7471B	PPB	09 Jan 2019 16:41:57	U	SMPL
IDOC3 - 1	IDOC3	19558	3.6620	-	7471B	PPB	09 Jan 2019 16:44:14	U	SMPL
IDOC4 - 1	IDOC4	18971	3.5515	-	7471B	PPB	09 Jan 2019 16:46:31	U	SMPL
CCV10 - 1	CCV10	29231	5.4818	-	7471B	PPB	09 Jan 2019 16:48:47	U	SMPL
CCB10 - 1	CCB10	-110	-0.0383	-	7471B	PPB	09 Jan 2019 16:51:05	U	SMPL

PS 01/09/19

LB100222 INSTRUMENT ID-CV1

7471B

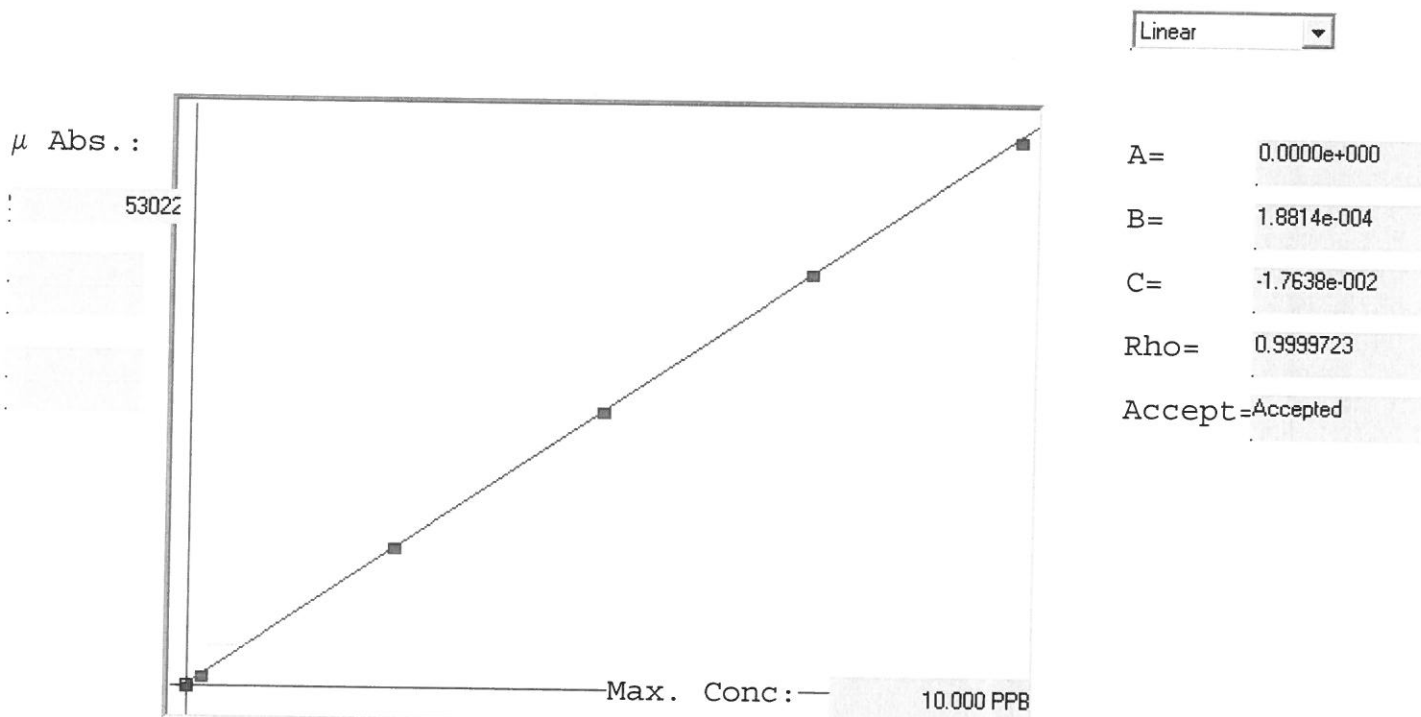

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.020	-0.020	-10	0.000	-10				
0.2	0.200	0.189	-0.011	1097	0.0 %	1097				
2.5	2.500	2.519	0.019	13485	0.0 %	13485				
5.0	5.000	5.012	0.012	26735	0.0 %	26735				
7.5	7.500	7.541	0.041	40178	0.0 %	40178				
10.0	10.000	9.958	-0.042	53022	0.0 %	53022				