


LB 100445
INSTRUMENT ID: CV1

7471B

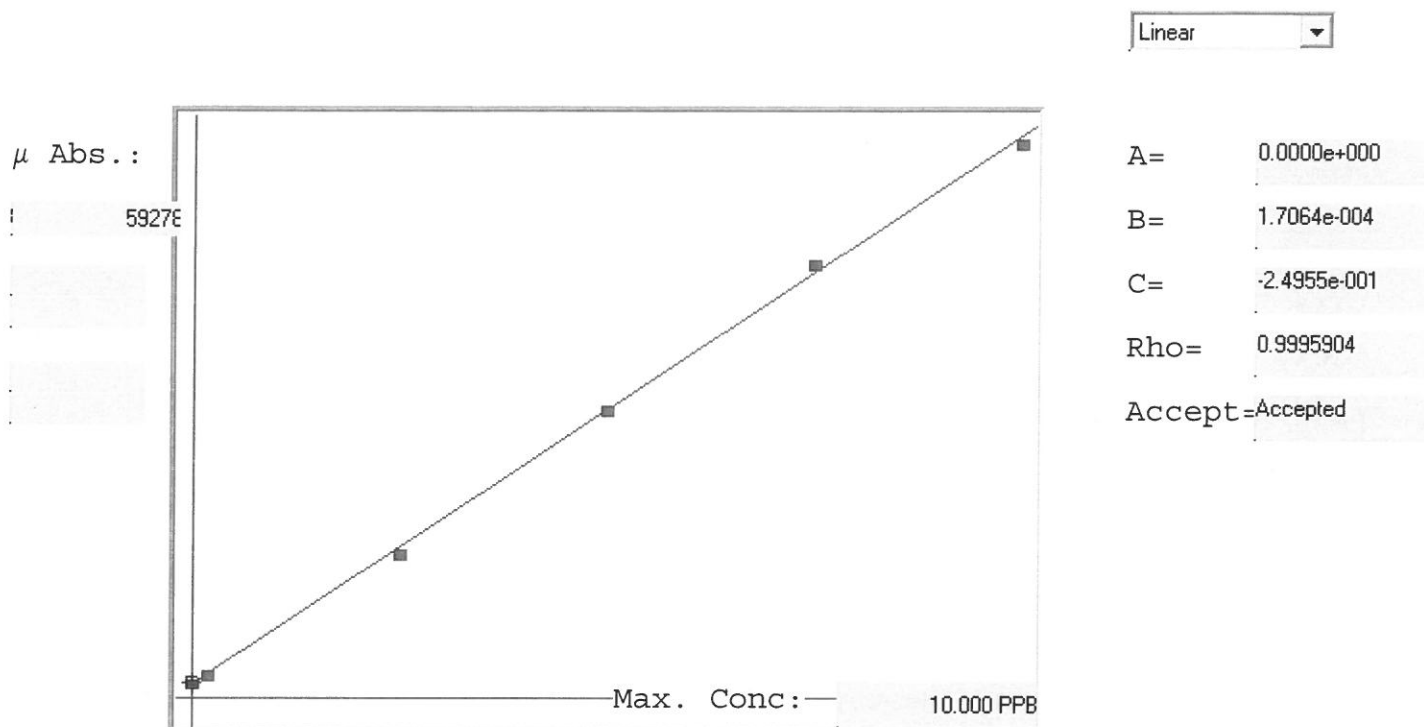

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.036	0.036	1673	0.000	1673				
0.2	0.200	0.190	-0.010	2576	0.0 %	2576				
2.5	2.500	2.391	-0.109	15473	0.0 %	15473				
5.0	5.000	5.032	0.032	30953	0.0 %	30953				
7.5	7.500	7.686	0.186	46503	0.0 %	46503				
10.0	10.000	9.866	-0.134	59278	0.0 %	59278				

LB100445 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 23 Jan 2019 09:04:01

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	1673	-	0.0000	7471B	PPB	23 Jan 2019 09:09:25	S	Std
0.2 - 1	50.2	2576	-	0.2000	7471B	PPB	23 Jan 2019 09:11:43	S	Std
2.5 - 1	52.5	15473	-	2.5000	7471B	PPB	23 Jan 2019 09:14:01	S	Std
5.0 - 1	55	30953	-	5.0000	7471B	PPB	23 Jan 2019 09:16:18	S	Std
7.5 - 1	57.5	46503	-	7.5000	7471B	PPB	23 Jan 2019 09:18:36	S	Std
10.0 - 1	510	59278	-	10.0000	7471B	PPB	23 Jan 2019 09:20:54	S	Std
ICV76 - 1	ICV76	24815	3.9848	-	7471B	PPB	23 Jan 2019 09:23:47	U	SMPL
ICB76 - 1	ICB76	1470	0.0013	-	7471B	PPB	23 Jan 2019 09:26:03	U	SMPL
CCV01 - 1	CCV01	30788	5.0040	-	7471B	PPB	23 Jan 2019 09:28:20	U	SMPL
CCB01 - 1	CCB01	1489	0.0045	-	7471B	PPB	23 Jan 2019 09:30:37	U	SMPL
CRA - 1	CRA	2541	0.1840	-	7471B	PPB	23 Jan 2019 09:32:55	U	SMPL
HighStd - 1	HighStd	58482	9.7297	-	7471B	PPB	23 Jan 2019 09:35:11	U	SMPL
ChkStd - 1	ChkStd	42509	7.0041	-	7471B	PPB	23 Jan 2019 09:37:28	U	SMPL
PB116576BL - 1	PBS	998	-0.0793	-	7471B	PPB	23 Jan 2019 09:39:46	U	SMPL
PB116576BS - 1	LCSS	21439	3.4088	-	7471B	PPB	23 Jan 2019 09:42:04	U	SMPL
K1210-01 - 1	RT-1495	1314	-0.0253	-	7471B	PPB	23 Jan 2019 09:44:21	U	SMPL
K1216-01 - 1	MULCH-1	6082	0.7883	-	7471B	PPB	23 Jan 2019 09:46:39	U	SMPL
K1219-01 - 1	390110753	6094	0.7903	-	7471B	PPB	23 Jan 2019 09:48:57	U	SMPL
K1220-01 - 1	S-1	3568	0.3593	-	7471B	PPB	23 Jan 2019 09:51:15	U	SMPL
CCV02 - 1	CCV02	30498	4.9546	-	7471B	PPB	23 Jan 2019 09:53:31	U	SMPL
CCB02 - 1	CCB02	1489	0.0045	-	7471B	PPB	23 Jan 2019 09:55:47	U	SMPL
K1220-03 - 1	T-1	14635	2.2477	-	7471B	PPB	23 Jan 2019 10:05:16	U	SMPL
K1220-03DUP - 1	T-1DUP	14925	2.2972	-	7471B	PPB	23 Jan 2019 10:07:32	U	SMPL
K1220-03MS - 1	T-1MS	40009	6.5775	-	7471B	PPB	23 Jan 2019 10:09:48	U	SMPL
K1220-03MSD - 1	T-1MSD	39598	6.5074	-	7471B	PPB	23 Jan 2019 10:12:05	U	SMPL
K1220-03LX5 - 1		3903	0.4164	-	7471B	PPB	23 Jan 2019 10:14:23	U	SMPL
K1220-03A - 1		38248	6.2770	-	7471B	PPB	23 Jan 2019 10:16:42	U	SMPL
CCV03 - 1	CCV03	30665	4.9831	-	7471B	PPB	23 Jan 2019 10:18:59	U	SMPL
CCB03 - 1	CCB03	1307	-0.0265	-	7471B	PPB	23 Jan 2019 10:21:19	U	SMPL