


LB100485
INSTRUMENT ID : CV1

7470A

μ Abs. :

44450

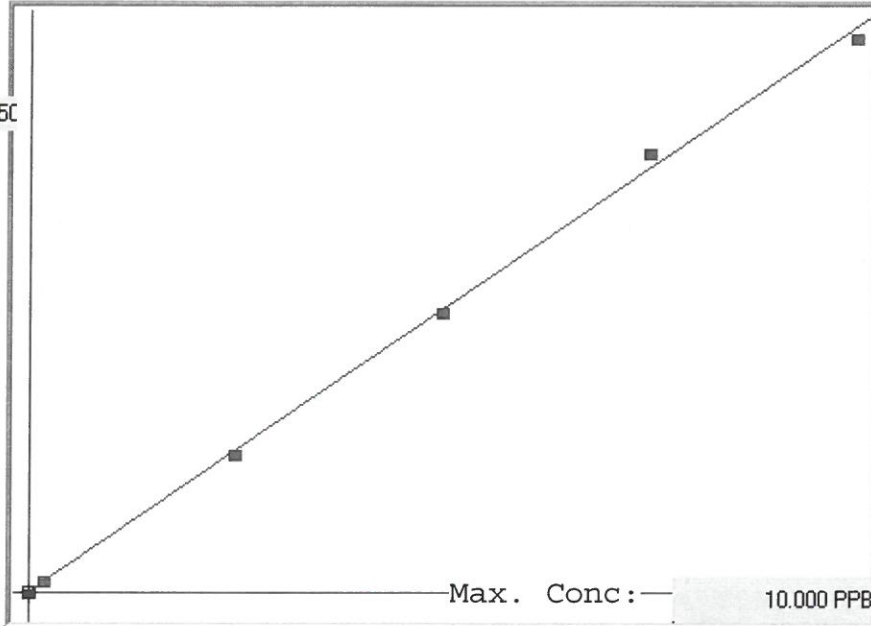

Linear

A= 0.0000e+000

B= 2.2080e-004

C= -8.2388e-003

Rho= 0.9992750

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.001	-0.001	34	0.000	34				
0.2	0.200	0.199	-0.001	937	0.0 %	937				
2.5	2.500	2.441	-0.059	11093	0.0 %	11093				
5.0	5.000	4.978	-0.022	22581	0.0 %	22581				
7.5	7.500	7.777	0.277	35261	0.0 %	35261				
10.0	10.000	9.806	-0.194	44450	0.0 %	44450	0			

LB100485 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 25 Jan 2019 14:51:05

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	34	-	0.0000	7470A	PPB	25 Jan 2019 14:53:41	S	Std
0.2 - 1	50-2	937	-	0.2000	7470A	PPB	25 Jan 2019 14:55:49	S	Std
2.5 - 1	52-5	11093	-	2.5000	7470A	PPB	25 Jan 2019 14:57:58	S	Std
5.0 - 1	55-0	22581	-	5.0000	7470A	PPB	25 Jan 2019 15:00:06	S	Std
7.5 - 1	57-5	35261	-	7.5000	7470A	PPB	25 Jan 2019 15:07:42	S	Std
10.0 - 1	510-0	44450	-	10.0000	7470A	PPB	25 Jan 2019 15:09:49	S	Std
ICV80 - 1	ICV80	16689	3.6766	-	7470A	PPB	25 Jan 2019 15:14:08	U	SMPL
ICB80 - 1	ICB80	-23	-0.0133	-	7470A	PPB	25 Jan 2019 15:16:15	U	SMPL
CCV17 - 1	CCV17	22688	5.0012	-	7470A	PPB	25 Jan 2019 15:18:21	U	SMPL
CCB17 - 1	CCB17	-17	-0.0120	-	7470A	PPB	25 Jan 2019 15:20:28	U	SMPL
CRA - 1	CRA	916	0.1940	-	7470A	PPB	25 Jan 2019 15:22:34	U	SMPL
HighStd - 1	HighStd	45889	10.1239	-	7470A	PPB	25 Jan 2019 15:24:41	U	SMPL
ChkStd - 1	ChkStd	32730	7.2184	-	7470A	PPB	25 Jan 2019 15:26:49	U	SMPL
PB116611BL - 1	PBW	-73	-0.0244	-	7470A	PPB	25 Jan 2019 15:28:56	U	SMPL
PB116611BS - 1	LCSW	16820	3.7056	-	7470A	PPB	25 Jan 2019 15:34:34	U	SMPL
K1003-02 - 1	BU-02-012319	-37	-0.0164	-	7470A	PPB	25 Jan 2019 15:36:42	U	SMPL
K1003-02DUP - 1	BU-02-012319DUP	0	-0.0082	-	7470A	PPB	25 Jan 2019 15:38:50	U	SMPL
K1003-02MS - 1	BU-02-012319MS	16648	3.6676	-	7470A	PPB	25 Jan 2019 15:40:59	U	SMPL
K1003-02MSD - 1	BU-02-012319MSD	16697	3.6784	-	7470A	PPB	25 Jan 2019 15:43:07	U	SMPL
K1016-04 - 1	TR-05-RO-1-012319	-36	-0.0162	-	7470A	PPB	25 Jan 2019 15:45:14	U	SMPL
CCV18 - 1	CCV18	22704	5.0047	-	7470A	PPB	25 Jan 2019 15:47:21	U	SMPL
CCB18 - 1	CCB18	-38	-0.0166	-	7470A	PPB	25 Jan 2019 15:49:28	U	SMPL
K1016-06 - 1	TR-05-RO-2-012319	-4	-0.0091	-	7470A	PPB	25 Jan 2019 15:51:35	U	SMPL
K1016-08 - 1	TR-05-RO-3-012319	5	-0.0071	-	7470A	PPB	25 Jan 2019 15:53:41	U	SMPL
K1016-10 - 1	TR-05-RO-4-012319	1	-0.0080	-	7470A	PPB	25 Jan 2019 15:55:48	U	SMPL
PB116611TB - 1	PB116588TB	27	-0.0023	-	7470A	PPB	25 Jan 2019 15:57:55	U	SMPL
K1003-02LX5 - 1		15	-0.0049	-	7470A	PPB	25 Jan 2019 16:00:03	U	SMPL
K1003-02A - 1		15710	3.4605	-	7470A	PPB	25 Jan 2019 16:02:11	U	SMPL
CCV19 - 1	CCV19	22354	4.9275	-	7470A	PPB	25 Jan 2019 16:04:19	U	SMPL
CCB19 - 1	CCB19	-28	-0.0144	-	7470A	PPB	25 Jan 2019 16:06:27	U	SMPL