

LB100566


INSTRUMENT ID: CU1

7471B

Linear

 μ Abs.:

53531

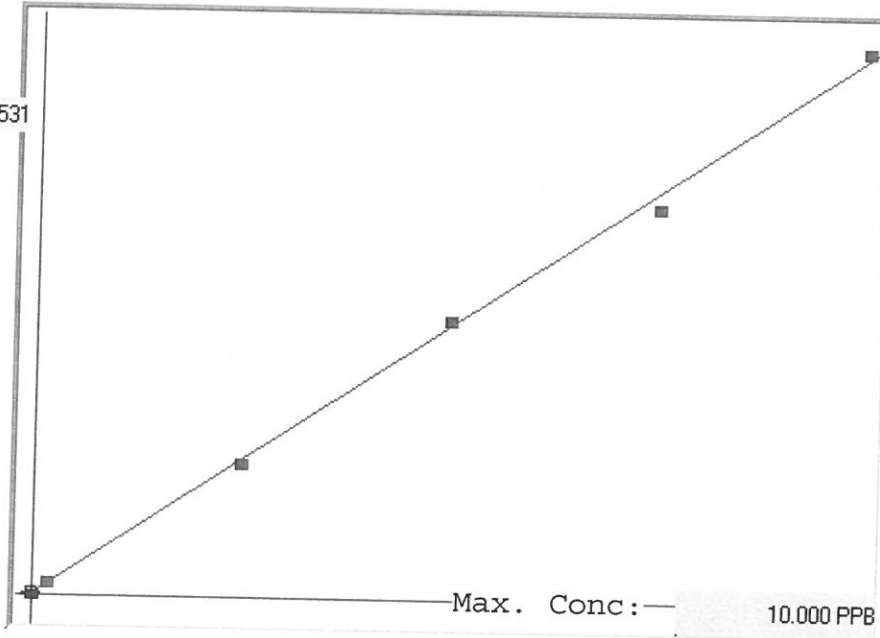

A= 0.0000e+000

B= 1.9008e-004

C= -2.6549e-002

Rho= 0.9993009

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.042	0.042	360	0.000	360				
0.2	0.200	0.221	0.021	1300	0.0 %	1300				
2.5	2.500	2.447	-0.053	13014	0.0 %	13014				
5.0	5.000	5.114	0.114	27046	0.0 %	27046				
7.5	7.500	7.228	-0.272	38165	0.0 %	38165				
10.0	10.000	10.148	0.148	53531	0.0 %	53531				

LB100566 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 31 Jan 2019 09:42:30

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	360	-	0.0000	7471B	PPB	31 Jan 2019 09:44:26	S	Std
0.2 - 1	50-2	1300	-	0.2000	7471B	PPB	31 Jan 2019 09:46:43	S	Std
2.5 - 1	52-5	13014	-	2.5000	7471B	PPB	31 Jan 2019 09:49:00	S	Std
5.0 - 1	55-0	27046	-	5.0000	7471B	PPB	31 Jan 2019 09:51:17	S	Std
7.5 - 1	57-5	38165	-	7.5000	7471B	PPB	31 Jan 2019 09:57:03	S	Std
10.0 - 1	510-0	53531	-	10.0000	7471B	PPB	31 Jan 2019 10:02:45	S	Std
ICV88 - 1	ICV88	21288	4.0198	-	7471B	PPB	31 Jan 2019 10:06:08	U	SMPL
ICB88 - 1	ICB88	184	0.0084	-	7471B	PPB	31 Jan 2019 10:08:25	U	SMPL
CCV49 - 1	CCV49	27056	5.1162	-	7471B	PPB	31 Jan 2019 10:10:42	U	SMPL
CCB49 - 1	CCB49	191	0.0098	-	7471B	PPB	31 Jan 2019 10:12:57	U	SMPL
CRA - 1	CRA	1299	0.2204	-	7471B	PPB	31 Jan 2019 10:15:13	U	SMPL
HighStd - 1	HighStd	54152	10.2665	-	7471B	PPB	31 Jan 2019 10:17:28	U	SMPL
ChkStd - 1	ChkStd	36782	6.9649	-	7471B	PPB	31 Jan 2019 10:19:44	U	SMPL
PB116734BL - 1	PBS	202	0.0118	-	7471B	PPB	31 Jan 2019 10:22:02	U	SMPL
PB116734BS - 1	LCSS	18113	3.4163	-	7471B	PPB	31 Jan 2019 10:27:37	U	SMPL
K1291-01 - 1	390124047	29704	5.6195	-	7471B	PPB	31 Jan 2019 10:29:53	U	SMPL
K1292-01 - 1	WC-1	1210	0.2034	-	7471B	PPB	31 Jan 2019 10:32:11	U	SMPL
K1292-01DUP - 1	WC-1DUP	1329	0.2261	-	7471B	PPB	31 Jan 2019 10:34:30	U	SMPL
K1292-01MS - 1	WC-1MS	19674	3.7130	-	7471B	PPB	31 Jan 2019 10:36:48	U	SMPL
K1292-01MSD - 1	WC-1MSD	19675	3.7132	-	7471B	PPB	31 Jan 2019 10:39:04	U	SMPL
CCV50 - 1	CCV50	26678	5.0443	-	7471B	PPB	31 Jan 2019 10:41:20	U	SMPL
CCB50 - 1	CCB50	177	0.0071	-	7471B	PPB	31 Jan 2019 10:43:37	U	SMPL
K1291-01LX5 - 1		410	0.0514	-	7471B	PPB	31 Jan 2019 10:45:53	U	SMPL
K1291-01A - 1		21813	4.1196	-	7471B	PPB	31 Jan 2019 10:48:09	U	SMPL
CCV51 - 1	CCV51	26835	5.0742	-	7471B	PPB	31 Jan 2019 10:50:25	U	SMPL
CCB51 - 1	CCB51	284	0.0274	-	7471B	PPB	31 Jan 2019 10:52:42	U	SMPL