

LB100569


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

38272

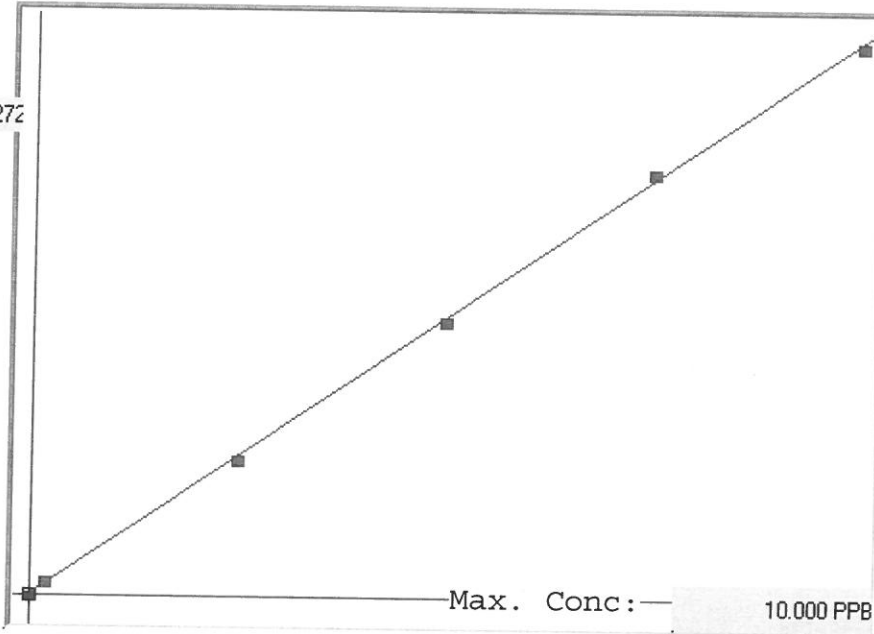

A= 0.0000e+000

B= 2.5968e-004

C= -1.7483e-002

Rho= 0.9998089

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.010	-0.010	27	0.000	27				
0.2	0.200	0.232	0.032	959	0.0 %	959				
2.5	2.500	2.457	-0.043	9529	0.0 %	9529				
5.0	5.000	4.959	-0.041	19163	0.0 %	19163				
7.5	7.500	7.642	0.142	29498	0.0 %	29498				
10.0	10.000	9.921	-0.079	38272	0.0 %	38272				

LB100569 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 31 Jan 2019 11:47:59

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	27	-	0.00007470A	PPB		31 Jan 2019 11:51:28	S	Std
0.2 - 1	50-2	959	-	0.20007470A	PPB		31 Jan 2019 11:53:36	S	Std
2.5 - 1	52-5	9529	-	2.50007470A	PPB		31 Jan 2019 11:55:44	S	Std
5.0 - 1	55-0	19163	-	5.00007470A	PPB		31 Jan 2019 11:57:52	S	Std
7.5 - 1	57-5	29498	-	7.50007470A	PPB		31 Jan 2019 12:07:07	S	Std
10.0 - 1	50-0	38272	-	10.00007470A	PPB		31 Jan 2019 12:09:13	S	Std
ICV89 - 1	ICV89	14642	3.7847	-7470A	PPB		31 Jan 2019 12:12:30	U	SMPL
ICB89 - 1	ICB89	174	0.0277	-7470A	PPB		31 Jan 2019 12:14:37	U	SMPL
CCV52 - 1	CCV52	19068	4.9340	-7470A	PPB		31 Jan 2019 12:16:43	U	SMPL
CCB52 - 1	CCB52	-32	-0.0258	-7470A	PPB		31 Jan 2019 12:18:48	U	SMPL
CRA - 1	CRA	941	0.2269	-7470A	PPB		31 Jan 2019 12:20:54	U	SMPL
HighStd - 1	HighStd	38530	9.9878	-7470A	PPB		31 Jan 2019 12:23:00	U	SMPL
ChkStd - 1	ChkStd	28681	7.4303	-7470A	PPB		31 Jan 2019 12:25:06	U	SMPL
PB116735BL - 1	PBW	234	0.0433	-7470A	PPB		31 Jan 2019 12:27:13	U	SMPL
PB116735BS - 1	LCSW	14883	3.8473	-7470A	PPB		31 Jan 2019 12:29:21	U	SMPL
K1277-04 - 1	FRAC-TANK-1-2	259	0.0498	-7470A	PPB		31 Jan 2019 12:38:00	U	SMPL
K1277-04DUP - 1	FRAC-TANK-1-2DUP	263	0.0508	-7470A	PPB		31 Jan 2019 12:40:07	U	SMPL
K1277-04MS - 1	FRAC-TANK-1-2MS	14568	3.7655	-7470A	PPB		31 Jan 2019 12:42:15	U	SMPL
K1277-04MSD - 1	FRAC-TANK-1-2MSD	14772	3.8184	-7470A	PPB		31 Jan 2019 12:44:23	U	SMPL
K1282-36 - 1	TPW1	294	0.0589	-7470A	PPB		31 Jan 2019 12:46:30	U	SMPL
PB116736BL - 1	PBW	24	-0.0113	-7470A	PPB		31 Jan 2019 12:56:43	U	SMPL
PB116736BS - 1	LCSW	15175	3.9231	-7470A	PPB		31 Jan 2019 12:58:49	U	SMPL
K1276-01 - 1	WASTE-OIL	458	0.1014	-7470A	PPB		31 Jan 2019 13:00:55	U	SMPL
K1282-04 - 1	TP-1	301	0.0607	-7470A	PPB		31 Jan 2019 13:03:01	U	SMPL
K1282-04DUP - 1	TP-1DUP	298	0.0599	-7470A	PPB		31 Jan 2019 13:05:08	U	SMPL
K1282-04MS - 1	TP-1MS	13677	3.5341	-7470A	PPB		31 Jan 2019 13:07:15	U	SMPL
K1282-04MSD - 1	TP-1MSD	14303	3.6967	-7470A	PPB		31 Jan 2019 13:09:22	U	SMPL
K1282-08 - 1	TP-2	917	0.2206	-7470A	PPB		31 Jan 2019 13:11:31	U	SMPL
K1282-12 - 1	TP-3	465	0.1033	-7470A	PPB		31 Jan 2019 13:13:39	U	SMPL
K1282-16 - 1	TP-4	375	0.0799	-7470A	PPB		31 Jan 2019 13:15:45	U	SMPL
CCV54 - 1	CCV54	16574	4.2864	-7470A	PPB		31 Jan 2019 13:17:52	U	SMPL
CCB54 - 1	CCB54	0	-0.0175	-7470A	PPB		31 Jan 2019 13:19:58	U	SMPL
CCV54 - 1	CCV54	17861	4.6206	-7470A	PPB		31 Jan 2019 13:21:43	U	SMPL
CCB54 - 1	CCB54	164	0.0251	-7470A	PPB		31 Jan 2019 13:23:49	U	SMPL
K1282-20 - 1	TP-5	214	0.0381	-7470A	PPB		31 Jan 2019 13:25:56	U	SMPL
K1282-24 - 1	TP-6	392	0.0843	-7470A	PPB		31 Jan 2019 13:28:03	U	SMPL
K1282-28 - 1	TP-7	330	0.0682	-7470A	PPB		31 Jan 2019 13:30:09	U	SMPL
K1282-32 - 1	TP-8	292	0.0583	-7470A	PPB		31 Jan 2019 13:32:15	U	SMPL
PB116735TB - 1	PB116702TB	372	0.0791	-7470A	PPB		31 Jan 2019 13:34:22	U	SMPL
PB116736TB - 1	PB116700TB	382	0.0817	-7470A	PPB		31 Jan 2019 13:40:43	U	SMPL
K1277-04LX5 - 1		191	0.0321	-7470A	PPB		31 Jan 2019 13:42:50	U	SMPL
K1277-04A - 1		13568	3.5058	-7470A	PPB		31 Jan 2019 13:44:58	U	SMPL
K1282-04LX5 - 1		17	-0.0131	-7470A	PPB		31 Jan 2019 13:47:06	U	SMPL
K1282-04A - 1		13654	3.5281	-7470A	PPB		31 Jan 2019 13:49:13	U	SMPL
CCV55 - 1	CCV55	17481	4.5219	-7470A	PPB		31 Jan 2019 13:51:20	U	SMPL
CCB55 - 1	CCB55	-6	-0.0190	-7470A	PPB		31 Jan 2019 13:53:27	U	SMPL