


LB100588

245.1

INSTRUMENT ID: CV1

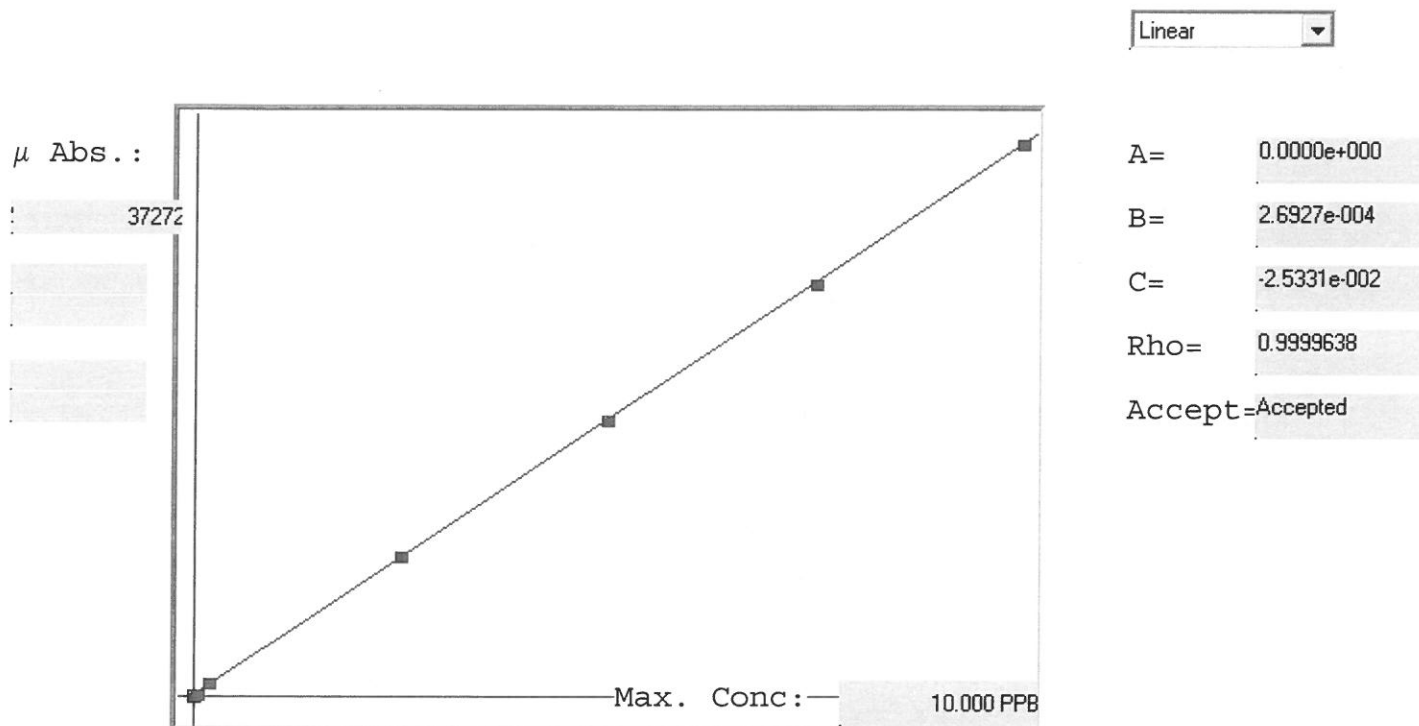

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.049	-0.049	-88	0.000	-88				
0.05	0.050	0.043	-0.007	255	0.0 %	255				
0.2	0.200	0.227	0.027	936	0.0 %	936				
2.5	2.500	2.545	0.045	9547	0.0 %	9547				
5.0	5.000	5.012	0.012	18707	0.0 %	18707				
7.5	7.500	7.461	-0.039	27803	0.0 %	27803				
10.0	10.000	10.011	0.011	37272	0.0 %	37272				

LB100588 INSTRUMENT ID : CV1

Method: 245.1		Operator: Admin		Date of Analysis: 01 Feb 2019 09:49:21					
Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	-88	-	0.0000	245.1	PPB	01 Feb 2019 10:27:13	S	Std
0.05 - 1	50.05	255	-	0.0500	245.1	PPB	01 Feb 2019 10:29:30	S	Std
0.2 - 1	50.2	936	-	0.2000	245.1	PPB	01 Feb 2019 10:31:47	S	Std
2.5 - 1	52.5	9547	-	2.5000	245.1	PPB	01 Feb 2019 10:34:04	S	Std
5.0 - 1	55.0	18707	-	5.0000	245.1	PPB	01 Feb 2019 10:36:21	S	Std
7.5 - 1	57.5	27803	-	7.5000	245.1	PPB	01 Feb 2019 10:38:36	S	Std
10.0 - 1	510.0	37272	-	10.0000	245.1	PPB	01 Feb 2019 10:47:39	S	Std
ICV90 - 1	ICV90	14436	3.8618	-245.1		PPB	01 Feb 2019 10:52:55	U	SMPL
ICB90 - 1	ICB90	234	0.0377	-245.1		PPB	01 Feb 2019 10:55:11	U	SMPL
CCV56 - 1	CCV56	19801	5.3064	-245.1		PPB	01 Feb 2019 10:57:27	U	SMPL
CCB56 - 1	CCB56	26	-0.0183	-245.1		PPB	01 Feb 2019 10:59:41	U	SMPL
CRA - 1	CRA	606	0.1378	-245.1		PPB	01 Feb 2019 11:06:12	U	SMPL
HighStd - 1	HighStd	37601	10.0993	-245.1		PPB	01 Feb 2019 11:08:27	U	SMPL
ChkStd - 1	ChkStd	27459	7.3684	-245.1		PPB	01 Feb 2019 11:10:42	U	SMPL
PB116737BL - 1	PBW	218	0.0334	-245.1		PPB	01 Feb 2019 11:13:00	U	SMPL
PB116737BS - 1	LCSW	14913	3.9902	-245.1		PPB	01 Feb 2019 11:15:18	U	SMPL
K1239-01 - 1	EFF-DAY-1-METAL	222	0.0344	-245.1		PPB	01 Feb 2019 11:17:35	U	SMPL
K1239-01DUP - 1	EFF-DAY-1-METALDUP	280	0.0501	-245.1		PPB	01 Feb 2019 11:19:51	U	SMPL
K1239-01MS - 1	EFF-DAY-1-METALMS	15170	4.0594	-245.1		PPB	01 Feb 2019 11:22:08	U	SMPL
K1239-01MSD - 1	EFF-DAY-1-METALMSD	15638	4.1854	-245.1		PPB	01 Feb 2019 11:24:26	U	SMPL
CCV57 - 1	CCV57	19097	5.1168	-245.1		PPB	01 Feb 2019 11:40:04	U	SMPL
CCB57 - 1	CCB57	9	-0.0229	-245.1		PPB	01 Feb 2019 11:42:20	U	SMPL
PB116755BL - 1	PBW	147	0.0143	-245.1		PPB	01 Feb 2019 12:23:08	U	SMPL
PB116755BS - 1	LCSW	15560	4.1644	-245.1		PPB	01 Feb 2019 12:25:25	U	SMPL
K1307-01 - 1	013019-SIDI-E-U-B	175	0.0218	-245.1		PPB	01 Feb 2019 12:27:42	U	SMPL
K1307-01DUP - 1	013019-SIDI-E-U-BDUP	225	0.0353	-245.1		PPB	01 Feb 2019 12:29:59	U	SMPL
K1307-01MS - 1	013019-SIDI-E-U-BMS	16938	4.5355	-245.1		PPB	01 Feb 2019 12:32:15	U	SMPL
CCV59 - 1 CCV58	eev59 CCV58	19645	5.2644	-245.1		PPB	01 Feb 2019 12:34:31	U	SMPL
CCB59 - 1 CCB58	eeb59 CCB58	-41	-0.0364	-245.1		PPB	01 Feb 2019 12:36:47	U	SMPL
K1307-01MSD - 1	013019-SIDI-E-U-BMSD	17094	4.5775	-245.1		PPB	01 Feb 2019 12:39:02	U	SMPL
K1307-02 - 1	013019-SIDI-E-U-M	171	0.0207	-245.1		PPB	01 Feb 2019 12:41:18	U	SMPL
K1307-03 - 1	013019-SIDI-E-U-S	224	0.0350	-245.1		PPB	01 Feb 2019 12:43:34	U	SMPL
K1307-04 - 1	013019-SIDI-E-D-B	187	0.0250	-245.1		PPB	01 Feb 2019 12:45:50	U	SMPL
K1307-05 - 1	013019-SIDI-E-D-M	174	0.0215	-245.1		PPB	01 Feb 2019 12:48:05	U	SMPL
K1307-06 - 1	013019-SIDI-E-D-S	182	0.0237	-245.1		PPB	01 Feb 2019 12:50:22	U	SMPL
K1239-01LX5 - 1		59	-0.0094	-245.1		PPB	01 Feb 2019 12:52:39	U	SMPL
K1239-01A - 1		16178	4.3309	-245.1		PPB	01 Feb 2019 12:54:55	U	SMPL
K1307-01LX5 - 1		-16	-0.0296	-245.1		PPB	01 Feb 2019 12:57:13	U	SMPL
K1307-01A - 1		17887	4.7910	-245.1		PPB	01 Feb 2019 13:05:28	U	SMPL
CCV60 - 1 CCV59	eev60 CCV59	18943	5.0754	-245.1		PPB	01 Feb 2019 13:07:44	U	SMPL
CCB60 - 1 CCB59	eeb60 CCB59	-54	-0.0399	-245.1		PPB	01 Feb 2019 13:09:59	U	SMPL