

LB100734


INSTRUMENT ID: CV1

7470A

Linear

 μ Abs.:

41322

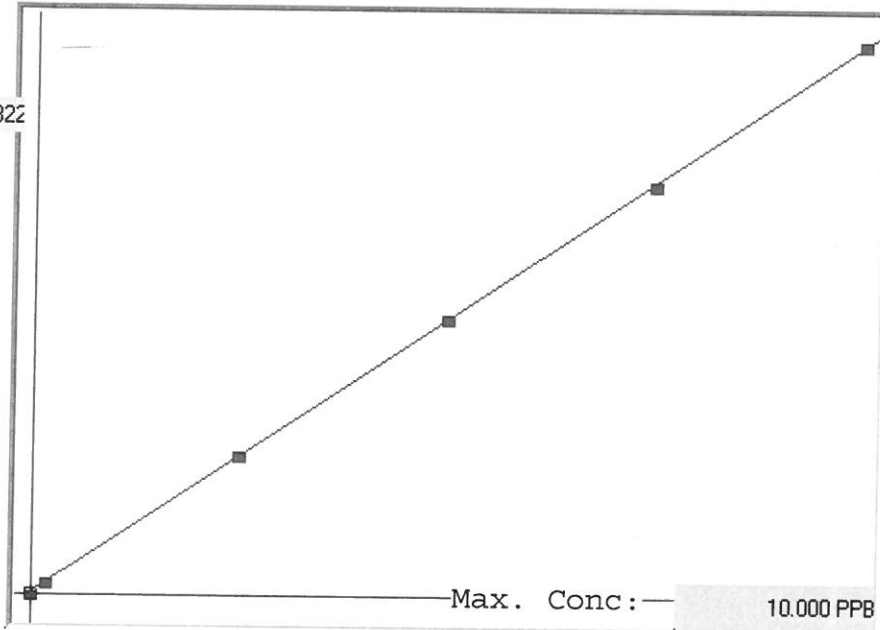

A= 0.0000e+000

B= 2.4333e-004

C= -3.5578e-002

Rho= 0.9999829

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.002	-0.002	136	0.000	136				
0.2	0.200	0.197	-0.003	955	0.0 %	955				
2.5	2.500	2.508	0.008	10452	0.0 %	10452				
5.0	5.000	5.022	0.022	20784	0.0 %	20784				
7.5	7.500	7.457	-0.043	30791	0.0 %	30791				
10.0	10.000	10.019	0.019	41322	0.0 %	41322				

LB100734 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 08 Feb 2019 14:55:48

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	136	-	0.0000	7470A	PPB	08 Feb 2019 15:02:51	S	Std
0.2 - 1	50-2	955	-	0.2000	7470A	PPB	08 Feb 2019 15:04:59	S	Std
2.5 - 1	52-5	10452	-	2.5000	7470A	PPB	08 Feb 2019 15:07:06	S	Std
5.0 - 1	55-0	20784	-	5.0000	7470A	PPB	08 Feb 2019 15:09:14	S	Std
7.5 - 1	57-5	30791	-	7.5000	7470A	PPB	08 Feb 2019 15:11:22	S	Std
10.0 - 1	510-0	41322	-	10.0000	7470A	PPB	08 Feb 2019 15:13:28	S	Std
ICV02 - 1	ICV02	16759	4.0424	-	7470A	PPB	08 Feb 2019 15:15:59	U	SMPL
ICB02 - 1	ICB02	-56	-0.0492	-	7470A	PPB	08 Feb 2019 15:18:05	U	SMPL
CCV04 - 1	CCV04	21394	5.1702	-	7470A	PPB	08 Feb 2019 15:20:10	U	SMPL
CCB04 - 1	CCB04	-27	-0.0421	-	7470A	PPB	08 Feb 2019 15:22:16	U	SMPL
CRA - 1	CRA	952	0.1961	-	7470A	PPB	08 Feb 2019 15:24:21	U	SMPL
HighStd - 1	HighStd	41372	10.0315	-	7470A	PPB	08 Feb 2019 15:26:28	U	SMPL
ChkStd - 1	ChkStd	29027	7.0276	-	7470A	PPB	08 Feb 2019 15:28:33	U	SMPL
PB116963BL - 1	PBW	79	-0.0164	-	7470A	PPB	08 Feb 2019 15:30:41	U	SMPL
PB116963BS - 1	LCSW	16059	3.8721	-	7470A	PPB	08 Feb 2019 15:32:48	U	SMPL
K1389-22 - 1	M-7	232	0.0209	-	7470A	PPB	08 Feb 2019 15:34:55	U	SMPL
K1396-02 - 1	COMP-1	139	-0.0018	-	7470A	PPB	08 Feb 2019 15:37:03	U	SMPL
K1396-02DUP - 1	COMP-1DUP	137	-0.0022	-	7470A	PPB	08 Feb 2019 15:39:10	U	SMPL
K1396-02MS - 1	COMP-1MS	17015	4.1047	-	7470A	PPB	08 Feb 2019 15:41:18	U	SMPL
K1396-02MSD - 1	COMP-1MSD	16907	4.0784	-	7470A	PPB	08 Feb 2019 15:43:24	U	SMPL
CCV05 - 1	CCV05	20752	5.0140	-	7470A	PPB	08 Feb 2019 15:45:30	U	SMPL
CCB05 - 1	CCB05	-68	-0.0521	-	7470A	PPB	08 Feb 2019 15:47:36	U	SMPL
PB116964BL - 1	PBW	236	0.0218	-	7470A	PPB	08 Feb 2019 15:49:42	U	SMPL
PB116964BS - 1	LCSW	15724	3.7906	-	7470A	PPB	08 Feb 2019 15:51:49	U	SMPL
K1385-08 - 1	98-WC-S-01-2-57	247	0.0245	-	7470A	PPB	08 Feb 2019 15:53:55	U	SMPL
K1385-08DUP - 1	98-WC-S-01-2-57DUP	289	0.0347	-	7470A	PPB	08 Feb 2019 15:56:01	U	SMPL
K1385-08MS - 1	98-WC-S-01-2-57MS	16905	4.0779	-	7470A	PPB	08 Feb 2019 15:58:08	U	SMPL
K1385-08MSD - 1	98-WC-S-01-2-57MSD	16817	4.0565	-	7470A	PPB	08 Feb 2019 16:00:15	U	SMPL
K1389-04 - 1	M-4	240	0.0228	-	7470A	PPB	08 Feb 2019 16:02:22	U	SMPL
K1389-08 - 1	M-6	270	0.0301	-	7470A	PPB	08 Feb 2019 16:04:29	U	SMPL
K1389-12 - 1	M-5S	318	0.0418	-	7470A	PPB	08 Feb 2019 16:06:38	U	SMPL
K1389-16 - 1	M-5-D	300	0.0374	-	7470A	PPB	08 Feb 2019 16:08:44	U	SMPL
CCV06 - 1	CCV06	20848	5.0374	-	7470A	PPB	08 Feb 2019 16:10:50	U	SMPL
CCB06 - 1	CCB06	-43	-0.0460	-	7470A	PPB	08 Feb 2019 16:12:57	U	SMPL
K1389-20 - 1	M-7-S	220	0.0180	-	7470A	PPB	08 Feb 2019 16:15:04	U	SMPL
K1394-01 - 1	ISW	224	0.0189	-	7470A	PPB	08 Feb 2019 16:17:10	U	SMPL
K1394-03 - 1	ISF	237	0.0221	-	7470A	PPB	08 Feb 2019 16:19:17	U	SMPL
K1396-01 - 1	23935	212	0.0160	-	7470A	PPB	08 Feb 2019 16:21:23	U	SMPL
K1401-02 - 1	RBR-200050	235	0.0216	-	7470A	PPB	08 Feb 2019 16:23:30	U	SMPL
K1401-04 - 1	RBR-200028	181	0.0085	-	7470A	PPB	08 Feb 2019 16:25:37	U	SMPL
K1401-06 - 1	RT-3425	181	0.0085	-	7470A	PPB	08 Feb 2019 16:27:45	U	SMPL
K1401-08 - 1	RT-3451	236	0.0218	-	7470A	PPB	08 Feb 2019 16:29:53	U	SMPL
K1401-10 - 1	RBR-200052	147	0.0002	-	7470A	PPB	08 Feb 2019 16:32:01	U	SMPL
PB116963TB - 1	PB116890TB	145	-0.0003	-	7470A	PPB	08 Feb 2019 16:34:07	U	SMPL
CCV07 - 1	CCV07	21037	5.0834	-	7470A	PPB	08 Feb 2019 16:36:14	U	SMPL
CCB07 - 1	CCB07	-80	-0.0550	-	7470A	PPB	08 Feb 2019 16:38:20	U	SMPL
PB116964TB - 1	PB116886TB	280	0.0326	-	7470A	PPB	08 Feb 2019 16:40:26	U	SMPL
K1396-02LX5 - 1		8	-0.0336	-	7470A	PPB	08 Feb 2019 16:42:32	U	SMPL
K1396-02A - 1		17045	4.1120	-	7470A	PPB	08 Feb 2019 16:44:39	U	SMPL
K1385-08LX5 - 1		13	-0.0324	-	7470A	PPB	08 Feb 2019 16:46:45	U	SMPL
K1385-08A - 1		17210	4.1521	-	7470A	PPB	08 Feb 2019 16:48:52	U	SMPL
CCV08 - 1	CCV08	20570	4.9697	-	7470A	PPB	08 Feb 2019 16:51:00	U	SMPL
CCB08 - 1	CCB08	-30	-0.0429	-	7470A	PPB	08 Feb 2019 16:53:07	U	SMPL