


LB100T68

INSTRUMENT ID : CV1

7470A

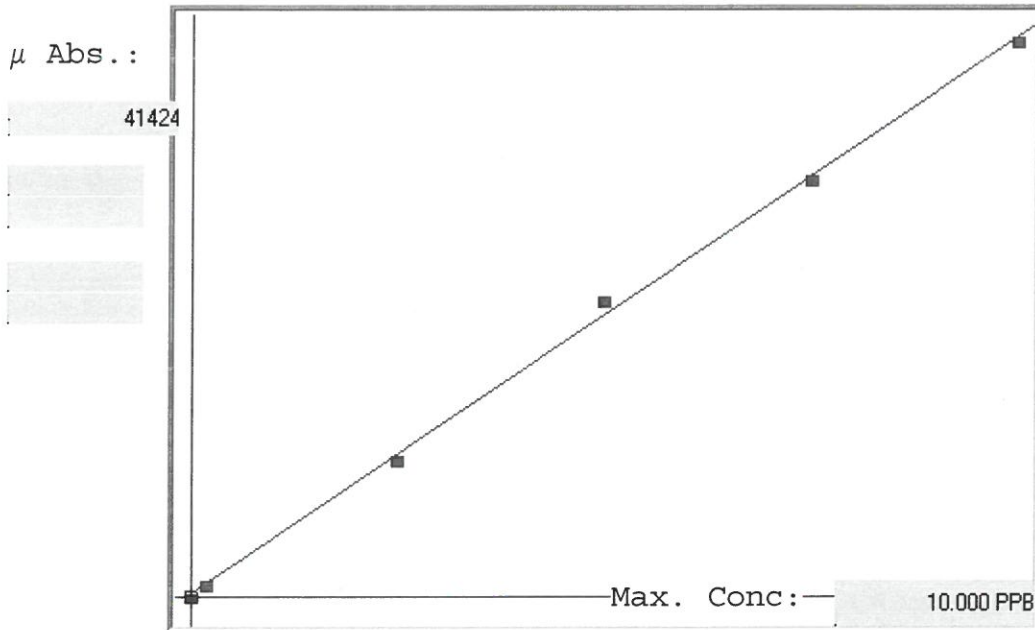

Linear

A= 0.0000e+000

B= 2.4052e-004

C= -5.0494e-002

Rho= 0.9994641

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.025	-0.025	104	0.000	104				
0.2	0.200	0.174	-0.026	933	0.0 %	933				
2.5	2.500	2.418	-0.082	10263	0.0 %	10263				
5.0	5.000	5.264	0.264	22098	0.0 %	22098				
7.5	7.500	7.456	-0.044	31211	0.0 %	31211				
10.0	10.000	9.913	-0.087	41424	0.0 %	41424				

LB100768 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 Feb 2019 12:31:14

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	104	-	0.0000	7470A	PPB	11 Feb 2019 12:34:11	S	Std
0.2 - 1	50.2	933	-	0.2000	7470A	PPB	11 Feb 2019 12:36:19	S	Std
2.5 - 1	52.5	10263	-	2.5000	7470A	PPB	11 Feb 2019 12:38:27	S	Std
5.0 - 1	55.0	22098	-	5.0000	7470A	PPB	11 Feb 2019 12:40:35	S	Std
7.5 - 1	57.5	31211	-	7.5000	7470A	PPB	11 Feb 2019 12:42:42	S	Std
10.0 - 1	510.0	41424	-	10.0000	7470A	PPB	11 Feb 2019 12:44:49	S	Std
ICV04 - 1	ICV04	15751	3.7379	-	7470A	PPB	11 Feb 2019 12:48:22	U	SMPL
ICB04 - 1	ICB04	112	-0.0236	-	7470A	PPB	11 Feb 2019 12:50:28	U	SMPL
CCV14 - 1	CCV14	22099	5.2647	-	7470A	PPB	11 Feb 2019 12:52:34	U	SMPL
CCB14 - 1	CCB14	-51	-0.0628	-	7470A	PPB	11 Feb 2019 12:54:40	U	SMPL
CRA - 1	CRA	1012	0.1929	-	7470A	PPB	11 Feb 2019 12:56:45	U	SMPL
HighStd - 1	HighStd	40918	9.7911	-	7470A	PPB	11 Feb 2019 12:58:51	U	SMPL
ChkStd - 1	ChkStd	28061	6.6987	-	7470A	PPB	11 Feb 2019 13:00:58	U	SMPL
PB117009BL - 1	PBW	-10	-0.0529	-	7470A	PPB	11 Feb 2019 13:03:05	U	SMPL
PB117009BS - 1	LCSW	15434	3.6617	-	7470A	PPB	11 Feb 2019 13:05:13	U	SMPL
K1348-02 - 1	OK-01-020719	9	-0.0483	-	7470A	PPB	11 Feb 2019 13:07:20	U	SMPL
K1348-02DUP - 1	OK-01-020719DUP	42	-0.0404	-	7470A	PPB	11 Feb 2019 13:09:28	U	SMPL
K1348-02MS - 1	OK-01-020719MS	17055	4.0516	-	7470A	PPB	11 Feb 2019 13:11:36	U	SMPL
K1348-02MSD - 1	OK-01-020719MSD	16864	4.0056	-	7470A	PPB	11 Feb 2019 13:13:44	U	SMPL
K1349-02 - 1	OR-03-020719-A	17	-0.0464	-	7470A	PPB	11 Feb 2019 13:15:50	U	SMPL
CCV15 - 1	CCV15	21187	5.0454	-	7470A	PPB	11 Feb 2019 13:17:56	U	SMPL
CCB15 - 1	CCB15	35	-0.0421	-	7470A	PPB	11 Feb 2019 13:20:02	U	SMPL
K1349-04 - 1	OR-03-020719-B	71	-0.0334	-	7470A	PPB	11 Feb 2019 13:22:08	U	SMPL
K1405-02 - 1	26-WARD-SOLID	98	-0.0269	-	7470A	PPB	11 Feb 2019 13:24:14	U	SMPL
K1406-02 - 1	N.RIVER-UNK-SOLID	55	-0.0373	-	7470A	PPB	11 Feb 2019 13:26:21	U	SMPL
K1411-01 - 1	EIGI-RO-294	29	-0.0435	-	7470A	PPB	11 Feb 2019 13:28:27	U	SMPL
K1422-04 - 1	TEST-PIT-1	48	-0.0389	-	7470A	PPB	11 Feb 2019 13:30:34	U	SMPL
PB117009TB - 1	PB116933TB	42	-0.0404	-	7470A	PPB	11 Feb 2019 13:32:41	U	SMPL
K1348-02LX5 - 1		80	-0.0313	-	7470A	PPB	11 Feb 2019 13:34:49	U	SMPL
K1348-02A - 1		17508	4.1605	-	7470A	PPB	11 Feb 2019 13:36:57	U	SMPL
CCV16 - 1	CCV16	20914	4.9797	-	7470A	PPB	11 Feb 2019 13:39:05	U	SMPL
CCB16 - 1	CCB16	-22	-0.0558	-	7470A	PPB	11 Feb 2019 13:41:11	U	SMPL