


LB101041

INSTRUMENT ID : CU1

245.1

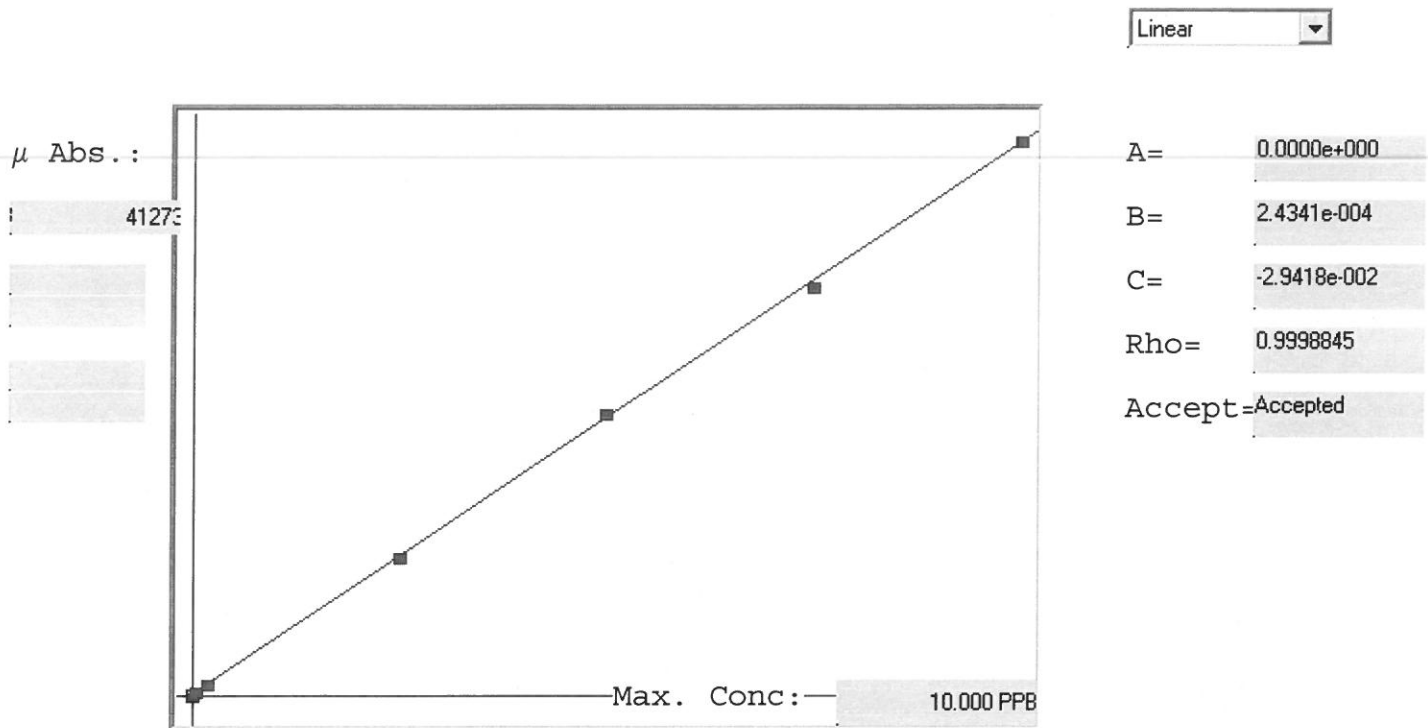

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.013	-0.013	67	0.000	67				
0.05	0.050	0.052	0.002	333	0.0 %	333				
0.2	0.200	0.196	-0.004	925	0.0 %	925				
2.5	2.500	2.480	-0.020	10310	0.0 %	10310				
5.0	5.000	5.112	0.112	21124	0.0 %	21124				
7.5	7.500	7.406	-0.094	30548	0.0 %	30548				
10.0	10.000	10.017	0.017	41273	0.0 %	41273				

LB101041 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 27 Feb 2019 10:51:29

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	67	-	0.0000	245.1	PPB	27 Feb 2019 10:52:10	S	Std
0.05 - 1	50-05	333	-	0.0500	245.1	PPB	27 Feb 2019 10:54:27	S	Std
0.2 - 1	50-2	925	-	0.2000	245.1	PPB	27 Feb 2019 10:56:45	S	Std
2.5 - 1	52-5	10310	-	2.5000	245.1	PPB	27 Feb 2019 10:59:02	S	Std
5.0 - 1	55-0	21124	-	5.0000	245.1	PPB	27 Feb 2019 11:01:19	S	Std
7.5 - 1	57-5	30548	-	7.5000	245.1	PPB	27 Feb 2019 11:03:35	S	Std
10.0 - 1	510-0	41273	-	10.0000	245.1	PPB	27 Feb 2019 11:05:51	S	Std
ICV27 - 1	ICV27	16503	3.9876	-245.1		PPB	27 Feb 2019 11:09:16	U	SMPL
ICB27 - 1	ICB27	72	-0.0119	-245.1		PPB	27 Feb 2019 11:11:31	U	SMPL
CCV32 - 1	CCV32	21147	5.1180	-245.1		PPB	27 Feb 2019 11:13:46	U	SMPL
CCB32 - 1	CCB32	-46	-0.0406	-245.1		PPB	27 Feb 2019 11:16:01	U	SMPL
CRA - 1	CRA	317	0.0477	-245.1		PPB	27 Feb 2019 11:18:17	U	SMPL
HighStd - 1	HighStd	41944	10.1802	-245.1		PPB	27 Feb 2019 11:20:32	U	SMPL
ChkStd - 1	ChkStd	28572	6.9253	-245.1		PPB	27 Feb 2019 11:22:47	U	SMPL
PB117382BL - 1	PBW	43	-0.0190	-245.1		PPB	27 Feb 2019 11:25:04	U	SMPL
PB117382BS - 1	LCSW	17811	4.3060	-245.1		PPB	27 Feb 2019 11:27:22	U	SMPL
K1570-01 - 1	50-50	233	0.0273	-245.1		PPB	27 Feb 2019 11:29:38	U	SMPL
K1570-02 - 1	50-25	462	0.0830	-245.1		PPB	27 Feb 2019 11:31:54	U	SMPL
K1570-03 - 1	25-25	260	0.0339	-245.1		PPB	27 Feb 2019 11:34:12	U	SMPL
K1570-04 - 1	25-10	45	-0.0185	-245.1		PPB	27 Feb 2019 11:36:28	U	SMPL
K1570-05 - 1	10-10	31	-0.0219	-245.1		PPB	27 Feb 2019 11:38:44	U	SMPL
CCV33 - 1	CCV33	20829	5.0406	-245.1		PPB	27 Feb 2019 11:40:59	U	SMPL
CCB33 - 1	CCB33	-34	-0.0377	-245.1		PPB	27 Feb 2019 11:43:15	U	SMPL
K1587-01 - 1	TP-MH-C02	164	0.0105	-245.1		PPB	27 Feb 2019 12:19:42	U	SMPL
K1587-01DUP - 1	TP-MH-C02DUP	145	0.0059	-245.1		PPB	27 Feb 2019 12:21:57	U	SMPL
K1587-01MS - 1	TP-MH-C02MS	17697	4.2782	-245.1		PPB	27 Feb 2019 12:24:12	U	SMPL
K1587-01MSD - 1	TP-MH-C02MSD	16905	4.0854	-245.1		PPB	27 Feb 2019 12:26:28	U	SMPL
K1611-03 - 1	HP-627	196	0.0183	-245.1		PPB	27 Feb 2019 12:28:44	U	SMPL
K1614-03 - 1	TI-633	103	-0.0043	-245.1		PPB	27 Feb 2019 12:31:00	U	SMPL
K1616-05 - 1	TI-658	179	0.0142	-245.1		PPB	27 Feb 2019 12:33:16	U	SMPL
K1587-01LX5 - 1		29	-0.0224	-245.1		PPB	27 Feb 2019 12:35:34	U	SMPL
K1587-01A - 1		16845	4.0708	-245.1		PPB	27 Feb 2019 12:37:51	U	SMPL
CCV34 - 1	CCV34	21010	5.0846	-245.1		PPB	27 Feb 2019 12:40:07	U	SMPL
CCB34 - 1	CCB34	91	-0.0073	-245.1		PPB	27 Feb 2019 12:42:22	U	SMPL