


LB101046

7470A

INSTRUMENT ID: CV1

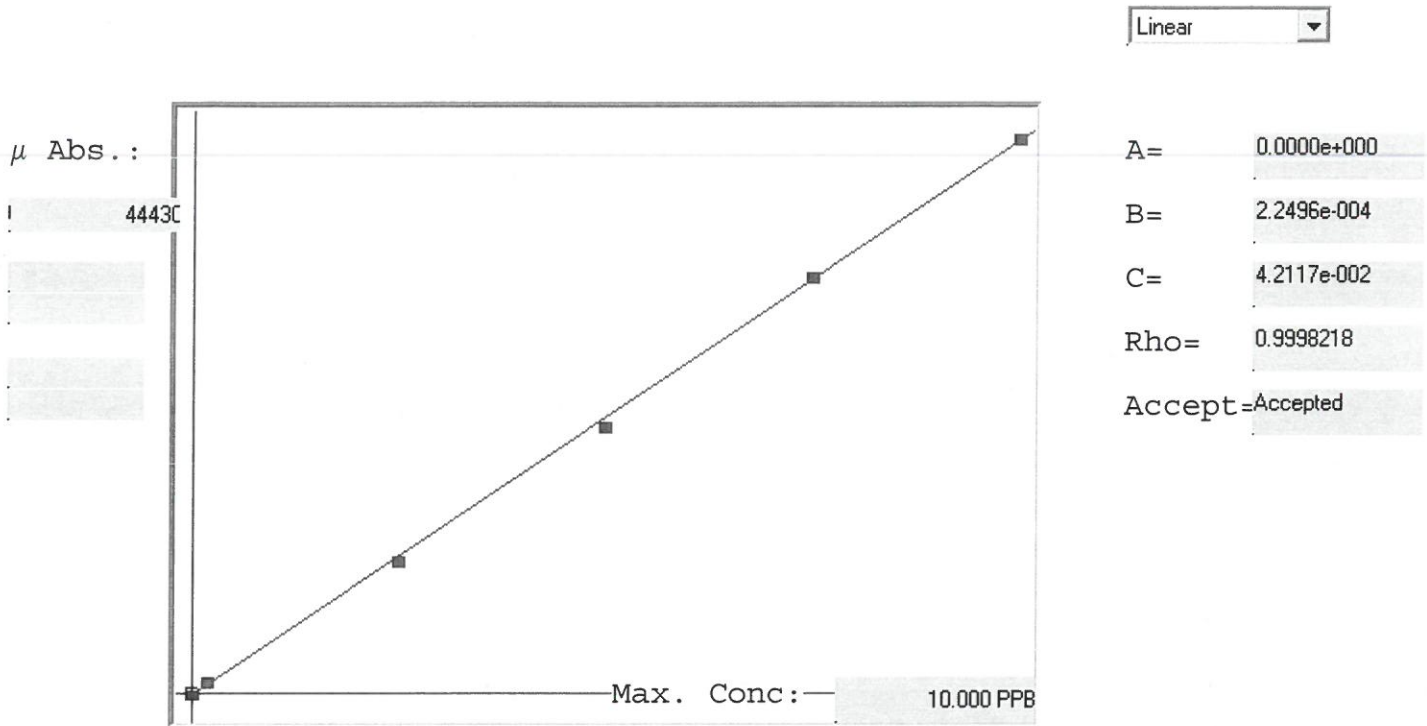

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.050	0.050	34	0.000	34				
0.2	0.200	0.250	0.050	925	0.0 %	925				
2.5	2.500	2.441	-0.059	10663	0.0 %	10663				
5.0	5.000	4.871	-0.129	21466	0.0 %	21466				
7.5	7.500	7.551	0.051	33380	0.0 %	33380				
10.0	10.000	10.037	0.037	44430	0.0 %	44430				

LB101046 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 27 Feb 2019 13:51:55

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50.0	34	-	0.0000	7470A	PPB	27 Feb 2019 13:54:00	S	Std
0.2 - 1	50.2	925	-	0.2000	7470A	PPB	27 Feb 2019 13:56:08	S	Std
2.5 - 1	52.5	10663	-	2.5000	7470A	PPB	27 Feb 2019 13:58:16	S	Std
5.0 - 1	55.0	21466	-	5.0000	7470A	PPB	27 Feb 2019 14:00:24	S	Std
7.5 - 1	57.5	33380	-	7.5000	7470A	PPB	27 Feb 2019 14:02:31	S	Std
10.0 - 1	510.0	44430	-	10.0000	7470A	PPB	27 Feb 2019 14:04:37	S	Std
ICV28 - 1	ICV28	16976	3.8610	-	7470A	PPB	27 Feb 2019 14:08:05	U	SMPL
ICB28 - 1	ICB28	8	0.0439	-	7470A	PPB	27 Feb 2019 14:10:11	U	SMPL
CCV35 - 1	CCV35	21594	4.8998	-	7470A	PPB	27 Feb 2019 14:12:17	U	SMPL
CCB35 - 1	CCB35	26	0.0480	-	7470A	PPB	27 Feb 2019 14:14:23	U	SMPL
CRA - 1	CRA	879	0.2399	-	7470A	PPB	27 Feb 2019 14:20:27	U	SMPL
HighStd - 1	HighStd	43995	9.9391	-	7470A	PPB	27 Feb 2019 14:22:33	U	SMPL
ChkStd - 1	ChkStd	30844	6.9807	-	7470A	PPB	27 Feb 2019 14:24:39	U	SMPL
PB117403BL - 1	PBW	-10	0.0399	-	7470A	PPB	27 Feb 2019 14:26:47	U	SMPL
PB117403BS - 1	LCSW	16963	3.8581	-	7470A	PPB	27 Feb 2019 14:28:54	U	SMPL
K1348-08 - 1	OK-02-022519	57	0.0549	-	7470A	PPB	27 Feb 2019 14:31:01	U	SMPL
K1348-08DUP - 1	OK-02-022519DUP	94	0.0633	-	7470A	PPB	27 Feb 2019 14:33:09	U	SMPL
K1348-08MS - 1	OK-02-022519MS	16798	3.8209	-	7470A	PPB	27 Feb 2019 14:39:26	U	SMPL
K1348-08MSD - 1	OK-02-022519MSD	16386	3.7283	-	7470A	PPB	27 Feb 2019 14:41:34	U	SMPL
K1608-01 - 1	OIL-WATER-SEPERATOR-1	28	0.0484	-	7470A	PPB	27 Feb 2019 14:43:40	U	SMPL
CCV36 - 1	CCV36	21868	4.9615	-	7470A	PPB	27 Feb 2019 14:45:46	U	SMPL
CCB36 - 1	CCB36	-31	0.0351	-	7470A	PPB	27 Feb 2019 14:47:52	U	SMPL
K1610-02 - 1	WV-A	64	0.0565	-	7470A	PPB	27 Feb 2019 14:49:58	U	SMPL
K1610-04 - 1	WV-B	45	0.0522	-	7470A	PPB	27 Feb 2019 14:52:04	U	SMPL
K1610-06 - 1	WV-C	43	0.0518	-	7470A	PPB	27 Feb 2019 14:54:11	U	SMPL
K1610-08 - 1	WV-D	51	0.0536	-	7470A	PPB	27 Feb 2019 14:56:17	U	SMPL
K1610-10 - 1	WV-E	56	0.0547	-	7470A	PPB	27 Feb 2019 14:58:24	U	SMPL
PB117435BL - 1	PBW	24	0.0475	-	7470A	PPB	27 Feb 2019 15:03:12	U	SMPL
PB117435BS - 1	LCSW	17572	3.9951	-	7470A	PPB	27 Feb 2019 15:08:01	U	SMPL
K1605-02 - 1	N48966	29	0.0486	-	7470A	PPB	27 Feb 2019 15:10:08	U	SMPL
K1605-02DUP - 1	N48966DUP	66	0.0570	-	7470A	PPB	27 Feb 2019 15:12:16	U	SMPL
K1605-02MS - 1	N48966MS	17344	3.9438	-	7470A	PPB	27 Feb 2019 15:14:22	U	SMPL
CCV37 - 1	CCV37	21873	4.9626	-	7470A	PPB	27 Feb 2019 15:16:29	U	SMPL
CCB37 - 1	CCB37	-25	0.0365	-	7470A	PPB	27 Feb 2019 15:18:36	U	SMPL
K1605-02MSD - 1	N48966MSD	17303	3.9346	-	7470A	PPB	27 Feb 2019 15:20:42	U	SMPL
PB117403TB - 1	PB117374TB	66	0.0570	-	7470A	PPB	27 Feb 2019 15:22:49	U	SMPL
PB117435TB - 1	PB117376TB	61	0.0558	-	7470A	PPB	27 Feb 2019 15:24:55	U	SMPL
K1348-08LX5 - 1		13	0.0450	-	7470A	PPB	27 Feb 2019 15:27:01	U	SMPL
K1348-08A - 1		16562	3.7679	-	7470A	PPB	27 Feb 2019 15:29:08	U	SMPL
K1605-02LX5 - 1		-17	0.0383	-	7470A	PPB	27 Feb 2019 15:31:16	U	SMPL
K1605-02A - 1		17388	3.9537	-	7470A	PPB	27 Feb 2019 15:33:23	U	SMPL
CCV38 - 1	CCV38	21360	4.8472	-	7470A	PPB	27 Feb 2019 15:35:31	U	SMPL
CCB38 - 1	CCB38	-26	0.0363	-	7470A	PPB	27 Feb 2019 15:37:39	U	SMPL