


LB101071

7470A

INSTRUMENT ID : CV1

 μ Abs.:

42376

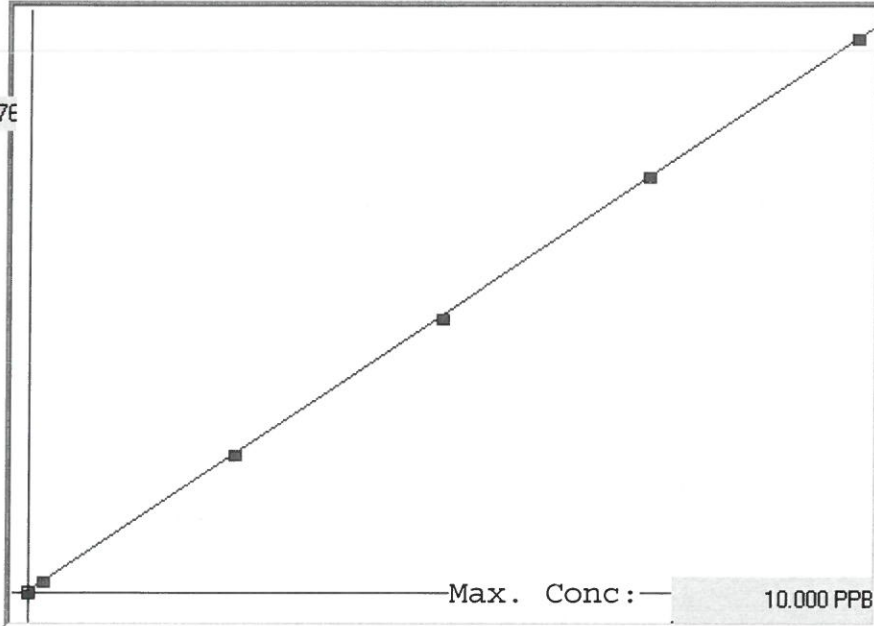

Linear

A= 0.0000e+000

B= 2.3638e-004

C= -1.3354e-002

Rho= 0.9999951

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.001	-0.001	52	0.000	52				
0.2	0.200	0.204	0.004	921	0.0 %	921				
2.5	2.500	2.510	0.010	10673	0.0 %	10673				
5.0	5.000	4.975	-0.025	21104	0.0 %	21104				
7.5	7.500	7.508	0.008	31819	0.0 %	31819				
10.0	10.000	10.004	0.004	42376	0.0 %	42376				

LB101071 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 28 Feb 2019 11:01:04

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	500	52	-	0.0000	7470A	PPB	28 Feb 2019 11:35:40	S	Std
0.2 - 1	502	921	-	0.2000	7470A	PPB	28 Feb 2019 11:37:48	S	Std
2.5 - 1	525	10673	-	2.5000	7470A	PPB	28 Feb 2019 11:39:57	S	Std
5.0 - 1	550	21104	-	5.0000	7470A	PPB	28 Feb 2019 11:42:04	S	Std
7.5 - 1	575	31819	-	7.5000	7470A	PPB	28 Feb 2019 11:44:12	S	Std
10.0 - 1	5100	42376	-	10.0000	7470A	PPB	28 Feb 2019 11:46:18	S	Std
ICV30 - 1	ICV30	15887	3.7421	-	7470A	PPB	28 Feb 2019 11:48:59	U	SMPL
ICB30 - 1	ICB30	91	0.0082	-	7470A	PPB	28 Feb 2019 11:51:05	U	SMPL
CCV45 - 1	CCV45	21244	5.0084	-	7470A	PPB	28 Feb 2019 11:53:12	U	SMPL
CCB45 - 1	CCB45	-12	-0.0162	-	7470A	PPB	28 Feb 2019 11:55:18	U	SMPL
CRA - 1	CRA	889	0.1968	-	7470A	PPB	28 Feb 2019 11:57:24	U	SMPL
HighStd - 1	HighStd	41880	9.8864	-	7470A	PPB	28 Feb 2019 11:59:30	U	SMPL
ChkStd - 1	ChkStd	29862	7.0456	-	7470A	PPB	28 Feb 2019 12:01:36	U	SMPL
PB117474BL - 1	PBW	13	-0.0103	-	7470A	PPB	28 Feb 2019 12:03:44	U	SMPL
PB117474BS - 1	LCSW	13808	3.2506	-	7470A	PPB	28 Feb 2019 12:05:51	U	SMPL
K1350-12 - 1	EO-01-022619-A	28	-0.0067	-	7470A	PPB	28 Feb 2019 12:07:58	U	SMPL
K1350-12DUP - 1	EO-01-022619-ADUP	61	0.0011	-	7470A	PPB	28 Feb 2019 12:10:05	U	SMPL
K1350-12MS - 1	EO-01-022619-AMS	16339	3.8489	-	7470A	PPB	28 Feb 2019 12:12:13	U	SMPL
K1350-12MSD - 1	EO-01-022619-AMSD	16126	3.7986	-	7470A	PPB	28 Feb 2019 12:14:21	U	SMPL
K1350-14 - 1	EO-01-022619-B	11	-0.0108	-	7470A	PPB	28 Feb 2019 12:16:27	U	SMPL
CCV46 - 1	CCV46	21126	4.9805	-	7470A	PPB	28 Feb 2019 12:18:34	U	SMPL
CCB46 - 1	CCB46	87	0.0072	-	7470A	PPB	28 Feb 2019 12:20:40	U	SMPL
K1350-16 - 1	EO-01-022619-C	85	0.0067	-	7470A	PPB	28 Feb 2019 12:22:46	U	SMPL
K1353-02 - 1	PL-02-022619-A	43	-0.0032	-	7470A	PPB	28 Feb 2019 12:24:52	U	SMPL
K1353-04 - 1	PL-02-022619-B	19	-0.0089	-	7470A	PPB	28 Feb 2019 12:26:59	U	SMPL
K1353-06 - 1	PL-02-022619-C	74	0.0041	-	7470A	PPB	28 Feb 2019 12:29:05	U	SMPL
K1353-08 - 1	PL-02-022619-D	67	0.0025	-	7470A	PPB	28 Feb 2019 12:31:12	U	SMPL
K1619-01 - 1	OIL-WATER-SEPERATOR-2	69	0.0030	-	7470A	PPB	28 Feb 2019 12:33:18	U	SMPL
K1632-01 - 1	50153	66	0.0022	-	7470A	PPB	28 Feb 2019 12:35:25	U	SMPL
K1633-04 - 1	SR-11-S	102	0.0108	-	7470A	PPB	28 Feb 2019 12:37:33	U	SMPL
K1633-08 - 1	SR-11-D	27	-0.0070	-	7470A	PPB	28 Feb 2019 12:39:41	U	SMPL
PB117475BL - 1	PBW	61	0.0011	-	7470A	PPB	28 Feb 2019 12:41:47	U	SMPL
CCV47 - 1	CCV47	21107	4.9760	-	7470A	PPB	28 Feb 2019 12:43:54	U	SMPL
CCB47 - 1	CCB47	110	0.0126	-	7470A	PPB	28 Feb 2019 12:46:01	U	SMPL
PB117475BS - 1	LCSW	16474	3.8808	-	7470A	PPB	28 Feb 2019 12:48:07	U	SMPL
K1631-14 - 1	Z31W	53	-0.0008	-	7470A	PPB	28 Feb 2019 12:50:14	U	SMPL
K1631-14DUP - 1	Z31WDUP	85	0.0067	-	7470A	PPB	28 Feb 2019 12:52:20	U	SMPL
K1631-14MS - 1	Z31WMS	15848	3.7329	-	7470A	PPB	28 Feb 2019 12:54:27	U	SMPL
K1631-14MSD - 1	Z31WMSD	15582	3.6700	-	7470A	PPB	28 Feb 2019 12:56:34	U	SMPL
K1632-02 - 1	30236	39	-0.0041	-	7470A	PPB	28 Feb 2019 12:58:41	U	SMPL
K1632-03 - 1	30238	94	0.0089	-	7470A	PPB	28 Feb 2019 13:00:49	U	SMPL
PB117477BL - 1	PBW	3	-0.0126	-	7470A	PPB	28 Feb 2019 13:02:56	U	SMPL
PB117477BS - 1	LCSW	16879	3.9766	-	7470A	PPB	28 Feb 2019 13:05:04	U	SMPL
K1631-13 - 1	Z31W	451	0.0933	-	7470A	PPB	28 Feb 2019 13:07:11	U	SMPL
CCV48 - 1	CCV48	21143	4.9845	-	7470A	PPB	28 Feb 2019 13:09:18	U	SMPL
CCB48 - 1	CCB48	32	-0.0058	-	7470A	PPB	28 Feb 2019 13:11:24	U	SMPL
K1631-13DUP - 1	Z31WDUP	476	0.0992	-	7470A	PPB	28 Feb 2019 13:13:30	U	SMPL
K1631-13MS - 1	Z31WMS	17853	4.2068	-	7470A	PPB	28 Feb 2019 13:15:37	U	SMPL
K1631-13MSD - 1	Z31WMSD	17855	4.2073	-	7470A	PPB	28 Feb 2019 13:17:43	U	SMPL
K1650-18 - 1	TWP-1	3	-0.0126	-	7470A	PPB	28 Feb 2019 13:19:50	U	SMPL
K1650-19 - 1	TWP-6	116	0.0141	-	7470A	PPB	28 Feb 2019 13:21:57	U	SMPL
PB117474TB - 1	PB117433TB	57	0.0001	-	7470A	PPB	28 Feb 2019 13:24:04	U	SMPL
PB117475TB - 1	PB117425TB	57	0.0001	-	7470A	PPB	28 Feb 2019 13:26:11	U	SMPL
K1350-12LX5 - 1		2	-0.0129	-	7470A	PPB	28 Feb 2019 13:28:19	U	SMPL
K1350-12A - 1		16325	3.8456	-	7470A	PPB	28 Feb 2019 13:30:27	U	SMPL
K1631-14LX5 - 1		-21	-0.0183	-	7470A	PPB	28 Feb 2019 13:32:33	U	SMPL
CCV49 - 1	CCV49	20964	4.9422	-	7470A	PPB	28 Feb 2019 13:34:40	U	SMPL
CCB49 - 1	CCB49	-27	-0.0197	-	7470A	PPB	28 Feb 2019 13:36:47	U	SMPL
K1631-14A - 1		16051	3.7809	-	7470A	PPB	28 Feb 2019 13:38:53	U	SMPL
K1631-13LX5 - 1		43	-0.0032	-	7470A	PPB	28 Feb 2019 13:41:00	U	SMPL
K1631-13A - 1		17669	4.1633	-	7470A	PPB	28 Feb 2019 13:43:07	U	SMPL
CCV50 - 1	CCV50	21762	5.1308	-	7470A	PPB	28 Feb 2019 13:45:58	U	SMPL
CCB50 - 1	CCB50	20	-0.0086	-	7470A	PPB	28 Feb 2019 13:48:04	U	SMPL