


LB101079

INSTRUMENT ID: CV1

7471B

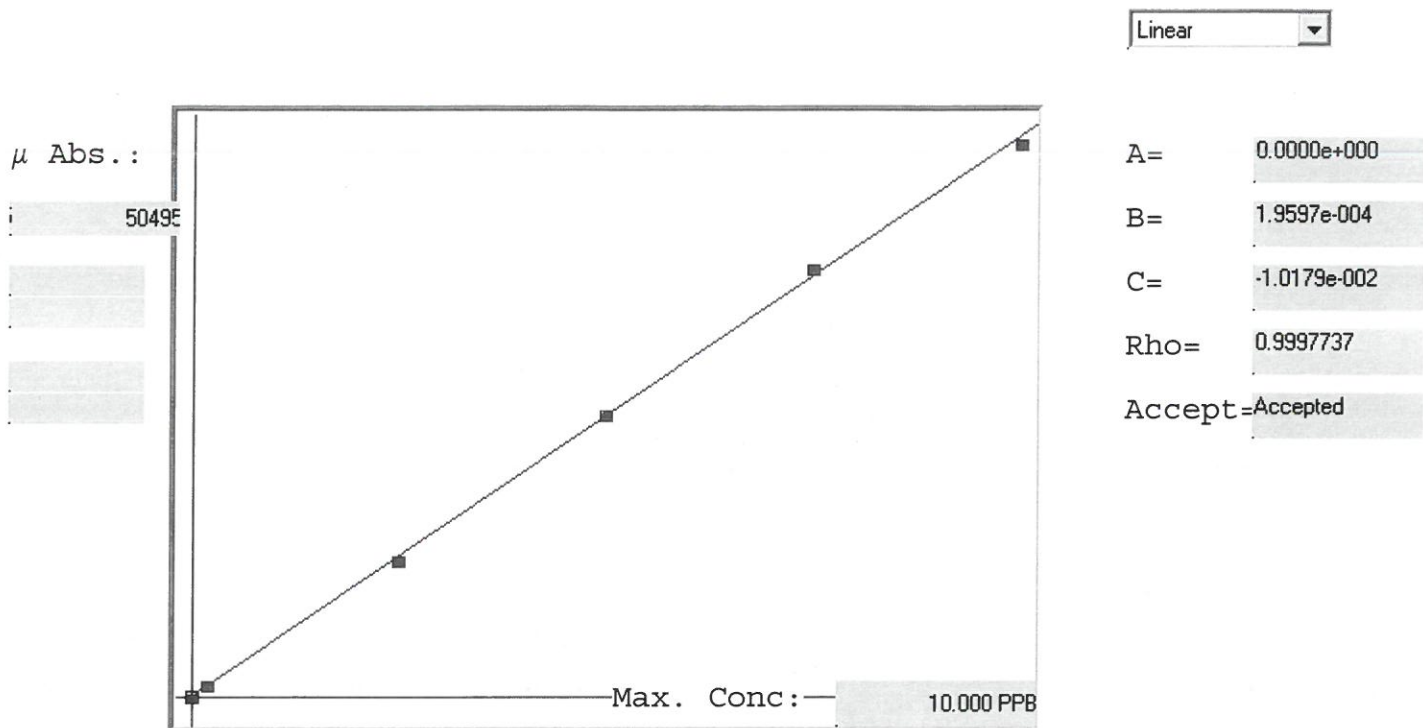

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.010	-0.010	-1	0.000	-1				
0.2	0.200	0.198	-0.002	1064	0.0 %	1064				
2.5	2.500	2.453	-0.047	12570	0.0 %	12570				
5.0	5.000	5.030	0.030	25718	0.0 %	25718				
7.5	7.500	7.644	0.144	39056	0.0 %	39056				
10.0	10.000	9.885	-0.115	50495	0.0 %	50495				

LB101079 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 28 Feb 2019 14:53:17

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50-0	-1	-	0.0000	7471B	PPB	28 Feb 2019 15:52:11	S	Std
0.2 - 1	50-2	1064	-	0.2000	7471B	PPB	28 Feb 2019 15:54:28	S	Std
2.5 - 1	52-5	12570	-	2.5000	7471B	PPB	28 Feb 2019 15:56:45	S	Std
5.0 - 1	55-0	25718	-	5.0000	7471B	PPB	28 Feb 2019 15:59:03	S	Std
7.5 - 1	57-5	39056	-	7.5000	7471B	PPB	28 Feb 2019 16:01:19	S	Std
10.0 - 1	510-0	50495	-	10.0000	7471B	PPB	28 Feb 2019 16:03:37	S	Std
ICV31 - 1	ICV31	20972	4.0997	-	7471B	PPB	28 Feb 2019 16:09:25	U	SMPL
ICB31 - 1	ICB31	-15	-0.0131	-	7471B	PPB	28 Feb 2019 16:11:41	U	SMPL
CCV51 - 1	CCV51	27767	5.4314	-	7471B	PPB	28 Feb 2019 16:13:58	U	SMPL
CCB51 - 1	CCB51	-50	-0.0200	-	7471B	PPB	28 Feb 2019 16:16:13	U	SMPL
CRA - 1	CRA	1100	0.2054	-	7471B	PPB	28 Feb 2019 16:18:29	U	SMPL
HighStd - 1	HighStd	54496	10.6695	-	7471B	PPB	28 Feb 2019 16:24:14	U	SMPL
ChkStd - 1	ChkStd	35762	6.9981	-	7471B	PPB	28 Feb 2019 16:29:53	U	SMPL
PB117478BL - 1	PBS	-69	-0.0237	-	7471B	PPB	28 Feb 2019 16:32:09	U	SMPL
PB117478BS - 1	LCSS	21829	4.2677	-	7471B	PPB	28 Feb 2019 16:34:27	U	SMPL
K1340-01 - 1	BU-03-022719	1519	0.2875	-	7471B	PPB	28 Feb 2019 16:36:43	U	SMPL
K1340-01DUP - 1	BU-03-022719DUP	1547	0.2930	-	7471B	PPB	28 Feb 2019 16:39:00	U	SMPL
K1340-01MS - 1	BU-03-022719MS	23292	4.5544	-	7471B	PPB	28 Feb 2019 16:51:48	U	SMPL
K1340-01MSD - 1	BU-03-022719MSD	23138	4.5242	-	7471B	PPB	28 Feb 2019 16:54:04	U	SMPL
K1341-07 - 1	HR-06-022719-A	1434	0.2708	-	7471B	PPB	28 Feb 2019 16:56:21	U	SMPL
CCV52 - 1	CCV52	26659	5.2142	-	7471B	PPB	28 Feb 2019 16:58:38	U	SMPL
CCB52 - 1	CCB52	34	-0.0035	-	7471B	PPB	28 Feb 2019 17:00:53	U	SMPL
K1341-09 - 1	HR-06-022719-B	4264	0.8254	-	7471B	PPB	28 Feb 2019 17:03:10	U	SMPL
K1349-13 - 1	OR-03-022719-A	1852	0.3528	-	7471B	PPB	28 Feb 2019 17:05:25	U	SMPL
K1349-15 - 1	OR-03-022719-B	2556	0.4907	-	7471B	PPB	28 Feb 2019 17:07:40	U	SMPL
K1643-01 - 1	INTERIOR-WALL	678	0.1227	-	7471B	PPB	28 Feb 2019 17:09:56	U	SMPL
K1643-03 - 1	FLOOR-SLAB	1116	0.2085	-	7471B	PPB	28 Feb 2019 17:12:12	U	SMPL
K1647-03 - 1	44766	4619	0.8950	-	7471B	PPB	28 Feb 2019 17:14:30	U	SMPL
K1649-01 - 1	TRE-INTERIOR-WALL	437	0.0755	-	7471B	PPB	28 Feb 2019 17:16:47	U	SMPL
K1649-02 - 1	TRE-FLOOR-SLAB	1625	0.3083	-	7471B	PPB	28 Feb 2019 17:19:05	U	SMPL
K1654-01 - 1	SOIL-PILE	2698	0.5186	-	7471B	PPB	28 Feb 2019 17:21:22	U	SMPL
PB117479BL - 1	PBS	49	-0.0006	-	7471B	PPB	28 Feb 2019 17:23:38	U	SMPL
CCV53 - 1	CCV53	26094	5.1035	-	7471B	PPB	28 Feb 2019 17:25:54	U	SMPL
CCB53 - 1	CCB53	-82	-0.0262	-	7471B	PPB	28 Feb 2019 17:28:10	U	SMPL
PB117479BS - 1	LCSS	21753	4.2528	-	7471B	PPB	28 Feb 2019 17:30:27	U	SMPL
K1358-05 - 1	TR-05-022719	5614	1.0900	-	7471B	PPB	28 Feb 2019 17:32:43	U	SMPL
K1358-05DUP - 1	TR-05-022719DUP	5670	1.1010	-	7471B	PPB	28 Feb 2019 17:34:59	U	SMPL
K1358-05MS - 1	TR-05-022719MS	29822	5.8341	-	7471B	PPB	28 Feb 2019 17:37:15	U	SMPL
K1358-05MSD - 1	TR-05-022719MSD	30036	5.8760	-	7471B	PPB	28 Feb 2019 17:39:31	U	SMPL
K1645-03 - 1	SR-10	5805	1.1274	-	7471B	PPB	28 Feb 2019 17:41:48	U	SMPL
K1645-07 - 1	SR-9-S	448	0.0776	-	7471B	PPB	28 Feb 2019 17:44:06	U	SMPL
K1645-11 - 1	SR-9-D	291	0.0468	-	7471B	PPB	28 Feb 2019 17:46:23	U	SMPL
K1650-01 - 1	B-1(1.5-2.5)	11459	2.2355	-	7471B	PPB	28 Feb 2019 17:48:40	U	SMPL
K1650-02 - 1	B-1(17-18)	209	0.0308	-	7471B	PPB	28 Feb 2019 17:50:56	U	SMPL
CCV54 - 1	CCV54	26312	5.1462	-	7471B	PPB	28 Feb 2019 17:53:12	U	SMPL
CCB54 - 1	CCB54	-20	-0.0141	-	7471B	PPB	28 Feb 2019 17:55:28	U	SMPL
K1650-03 - 1	B-1(24-25)	297	0.0480	-	7471B	PPB	28 Feb 2019 17:57:45	U	SMPL
K1650-05 - 1	B-2(9-10)	208	0.0306	-	7471B	PPB	28 Feb 2019 18:00:01	U	SMPL
K1650-06 - 1	B-3(2.5-3.5)	127611	24.9979	-	7471B	PPB	28 Feb 2019 18:02:17	U	SMPL
K1650-07 - 1	B-3(9-10)	-119	-0.0335	-	7471B	PPB	28 Feb 2019 18:04:33	U	SMPL
K1650-08 - 1	B-4(4-5)	57286	11.2162	-	7471B	PPB	28 Feb 2019 18:06:51	U	SMPL
K1650-11 - 1	B-5(9-10)	206	0.0302	-	7471B	PPB	28 Feb 2019 18:09:08	U	SMPL
K1650-12 - 1	B-6(4-5)	64020	12.5359	-	7471B	PPB	28 Feb 2019 18:11:26	U	SMPL
K1650-13 - 1	B-6(9-10)	192	0.0274	-	7471B	PPB	28 Feb 2019 18:13:43	U	SMPL
K1650-14 - 1	B-7(3.5-4.5)	34401	6.7314	-	7471B	PPB	28 Feb 2019 18:16:02	U	SMPL
K1650-15 - 1	B-7(9-10)	126	0.0145	-	7471B	PPB	28 Feb 2019 18:18:18	U	SMPL
CCV55 - 1	CCV55	27987	5.4745	-	7471B	PPB	28 Feb 2019 18:31:43	U	SMPL
CCB55 - 1	CCB55	-73	-0.0245	-	7471B	PPB	28 Feb 2019 18:33:59	U	SMPL
K1650-16 - 1	B-8(3.5-4.5)	46475	9.0976	-	7471B	PPB	28 Feb 2019 18:36:16	U	SMPL
K1651-01 - 1	351-281	1507	0.2851	-	7471B	PPB	28 Feb 2019 18:38:32	U	SMPL
K1652-10 - 1	COMP-DAY-1	4290	0.8305	-	7471B	PPB	28 Feb 2019 18:40:49	U	SMPL
K1652-12 - 1	COMP-DAY-2	68022	13.3202	-	7471B	PPB	28 Feb 2019 18:43:05	U	SMPL
K1340-01LX5 - 1		132	0.0157	-	7471B	PPB	28 Feb 2019 18:45:21	U	SMPL
K1340-01A - 1		25607	5.0081	-	7471B	PPB	28 Feb 2019 18:47:40	U	SMPL
K1358-05LX5 - 1		1095	0.2044	-	7471B	PPB	28 Feb 2019 18:49:56	U	SMPL
K1358-05A - 1		30558	5.9783	-	7471B	PPB	28 Feb 2019 18:52:14	U	SMPL
K1650-06DLX5 - 1		25263	4.9406	-	7471B	PPB	28 Feb 2019 18:54:31	U	SMPL
K1650-08DLX2 - 1		28020	5.4809	-	7471B	PPB	28 Feb 2019 18:56:49	U	SMPL
CCV56 - 1	CCV56	24339	4.7596	-	7471B	PPB	28 Feb 2019 18:59:07	U	SMPL
CCB56 - 1	CCB56	-68	-0.0235	-	7471B	PPB	28 Feb 2019 19:01:24	U	SMPL
K1650-12DLX2 - 1		31783	6.2184	-	7471B	PPB	28 Feb 2019 19:03:41	U	SMPL
K1652-12DLX2 - 1		32763	6.4104	-	7471B	PPB	28 Feb 2019 19:05:58	U	SMPL
CCV57 - 1	CCV57	23649	4.6243	-	7471B	PPB	28 Feb 2019 19:08:15	U	SMPL
CCB57 - 1	CCB57	-24	-0.0149	-	7471B	PPB	28 Feb 2019 19:10:33	U	SMPL