

LB101098


ISM02.4

INSTRUMENT ID: CV1

Linear

 $\mu$  Abs.:

48703

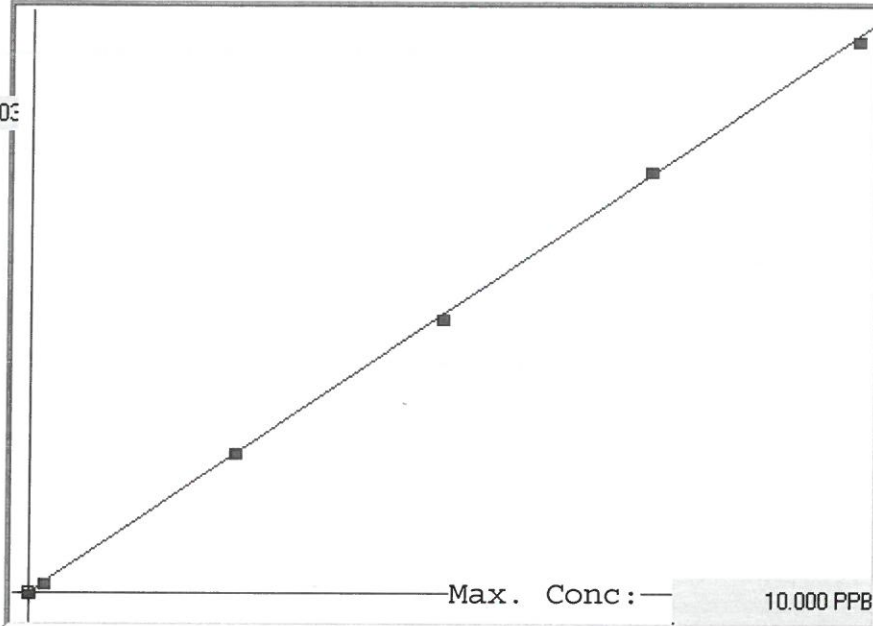

A= 0.0000e+000

B= 2.0393e-004

C= 1.5430e-003

Rho= 0.9998869

Accept=Accepted

slope  
y-intercept

| Std ID | Conc.  | Calc.  | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 | %D |
|--------|--------|--------|--------|-------|------------|-------|-------|-------|-------|-------|----|
| 0.00   | 0.000  | -0.018 | -0.018 | -98   | 0.000      | -98   |       |       |       |       | 1  |
| 0.2    | 0.200  | 0.200  | 0.000  | 974   | 0.0 %      | 974   |       |       |       |       | 0  |
| 2.5    | 2.500  | 2.519  | 0.019  | 12343 | 0.0 %      | 12343 |       |       |       |       | 1  |
| 5.0    | 5.000  | 4.958  | -0.042 | 24307 | 0.0 %      | 24307 |       |       |       |       | 1  |
| 7.5    | 7.500  | 7.608  | 0.108  | 37299 | 0.0 %      | 37299 |       |       |       |       | 1  |
| 10     | 10.000 | 9.933  | -0.067 | 48703 | 0.0 %      | 48703 |       |       |       |       | 1  |

LB101098

INSTRUMENT ID : CV1

| Sample ID  | Extended ID | $\mu$ Abs. | Conc.     | Std Conc | Method      | Units | Date           | Type |
|------------|-------------|------------|-----------|----------|-------------|-------|----------------|------|
|            | 0 S0.0      | -98        | -         |          | 0 ISM02.4   | PPB   | 3/1/2019 10:24 | Std  |
|            | 0.2 S0.2    | 974        | -         |          | 0.2 ISM02.4 | PPB   | 3/1/2019 10:27 | Std  |
|            | 2.5 S2.5    | 12343      | -         |          | 2.5 ISM02.4 | PPB   | 3/1/2019 10:29 | Std  |
|            | 5 S5.0      | 24307      | -         |          | 5 ISM02.4   | PPB   | 3/1/2019 10:31 | Std  |
|            | 7.5 S7.5    | 37299      | -         |          | 7.5 ISM02.4 | PPB   | 3/1/2019 10:33 | Std  |
|            | 10 S10.0    | 48703      | -         |          | 10 ISM02.4  | PPB   | 3/1/2019 10:36 | Std  |
| ICV        | ICV         | 19647      | 4.0081 -  |          | ISM02.4     | PPB   | 3/1/2019 10:44 | SMPL |
| ICB        | ICB         | -31        | -0.0048 - |          | ISM02.4     | PPB   | 3/1/2019 10:47 | SMPL |
| CCV060     | CCV060      | 23423      | 4.7781 -  |          | ISM02.4     | PPB   | 3/1/2019 10:49 | SMPL |
| CCB060     | CCB060      | 7          | 0.003 -   |          | ISM02.4     | PPB   | 3/1/2019 10:51 | SMPL |
| PB117485BL | PBS485      | 151        | 0.0323 -  |          | ISM02.4     | PPB   | 3/1/2019 10:53 | SMPL |
| K1554-19   | MX2G13      | 24141      | 4.9246 -  |          | ISM02.4     | PPB   | 3/1/2019 10:56 | SMPL |
| K1554-20   | MX2G13D     | 24469      | 4.9914 -  |          | ISM02.4     | PPB   | 3/1/2019 11:00 | SMPL |
| K1554-21   | MX2G13S     | 39372      | 8.0306 -  |          | ISM02.4     | PPB   | 3/1/2019 11:02 | SMPL |
| CCV061     | CCV061      | 24244      | 4.9456 -  |          | ISM02.4     | PPB   | 3/1/2019 11:09 | SMPL |
| CCB061     | CCB061      | -35        | -0.0056 - |          | ISM02.4     | PPB   | 3/1/2019 11:11 | SMPL |