


LB1D1102
INSTRUMENT ID: CV1

7470A

Linear

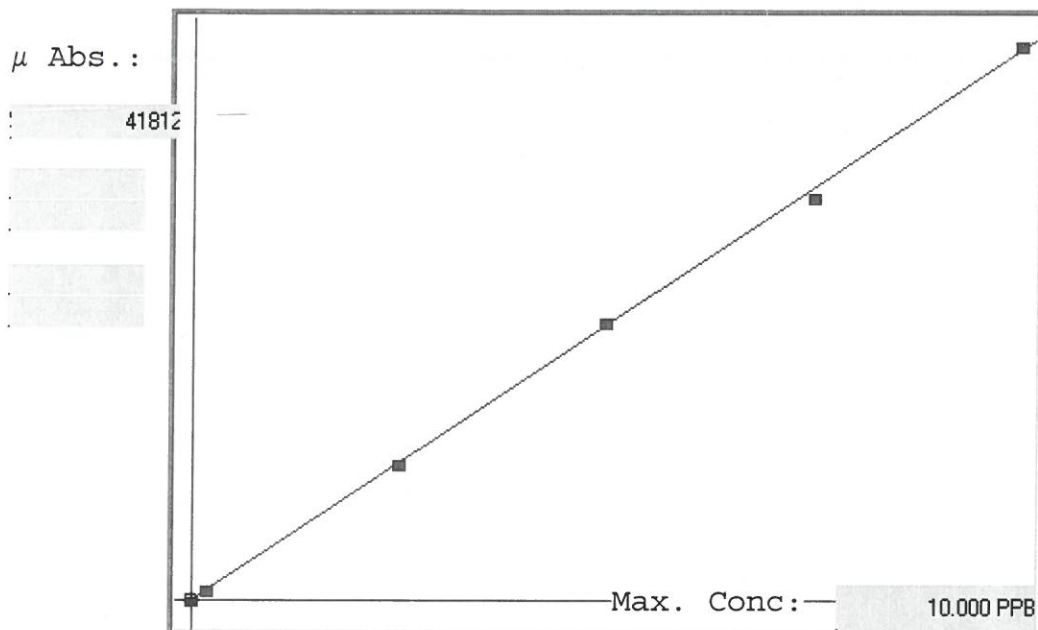

A= 0.0000e+000

B= 2.4095e-004

C= 9.3613e-004

Rho= 0.9998182

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.013	0.013	51	0.000	51				
0.2	0.200	0.193	-0.007	796	0.0 %	796				
2.5	2.500	2.507	0.007	10399	0.0 %	10399				
5.0	5.000	5.056	0.056	20979	0.0 %	20979				
7.5	7.500	7.356	-0.144	30527	0.0 %	30527				
10.0	10.000	10.075	0.075	41812	0.0 %	41812				

LB101102 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 01 Mar 2019 11:49:00

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc/Method	Units	Date	Type	Type
0.0 - 1	50.0	51	-	0.00007470A	PPB	01 Mar 2019 11:53:25	S	Std
0.2 - 1	50.2	796	-	0.20007470A	PPB	01 Mar 2019 11:55:33	S	Std
2.5 - 1	52.5	10399	-	2.50007470A	PPB	01 Mar 2019 11:57:41	S	Std
5.0 - 1	55.0	20979	-	5.00007470A	PPB	01 Mar 2019 11:59:49	S	Std
7.5 - 1	57.5	30527	-	7.50007470A	PPB	01 Mar 2019 12:01:56	S	Std
10.0 - 1	510.0	41812	-	10.00007470A	PPB	01 Mar 2019 12:06:34	S	Std
ICV35 - 1	ICV35	16061	3.8708	-7470A	PPB	01 Mar 2019 12:09:25	U	SMPL
ICB35 - 1	ICB35	-26	-0.0053	-7470A	PPB	01 Mar 2019 12:11:32	U	SMPL
CCV62 - 1	CCV62	21193	5.1073	-7470A	PPB	01 Mar 2019 12:13:39	U	SMPL
CCB62 - 1	CCB62	-30	-0.0063	-7470A	PPB	01 Mar 2019 12:15:44	U	SMPL
CRA - 1	CRA	769	0.1862	-7470A	PPB	01 Mar 2019 12:17:50	U	SMPL
HighStd - 1	HighStd	41916	10.1005	-7470A	PPB	01 Mar 2019 12:19:56	U	SMPL
ChkStd - 1	ChkStd	28372	6.8371	-7470A	PPB	01 Mar 2019 12:22:02	U	SMPL
PB117519BL - 1	PBW	-43	-0.0094	-7470A	PPB	01 Mar 2019 12:24:10	U	SMPL
PB117519BS - 1	LCSW	17342	4.1794	-7470A	PPB	01 Mar 2019 12:26:17	U	SMPL
K1340-02 - 1	BU-03-022719	-33	-0.0070	-7470A	PPB	01 Mar 2019 12:28:25	U	SMPL
K1340-02DUP - 1	BU-03-022719DUP	7	0.0026	-7470A	PPB	01 Mar 2019 12:30:32	U	SMPL
K1340-02MS - 1	BU-03-022719MS	16372	3.9457	-7470A	PPB	01 Mar 2019 12:32:40	U	SMPL
K1340-02MSD - 1	BU-03-022719MSD	16448	3.9640	-7470A	PPB	01 Mar 2019 12:34:48	U	SMPL
K1341-08 - 1	HR-06-022719-A	-8	-0.0010	-7470A	PPB	01 Mar 2019 12:36:54	U	SMPL
CCV63 - 1	CCV63	20901	5.0370	-7470A	PPB	01 Mar 2019 12:39:02	U	SMPL
CCB63 - 1	CCB63	-46	-0.0101	-7470A	PPB	01 Mar 2019 12:41:08	U	SMPL
K1341-10 - 1	HR-06-022719-B	32	0.0086	-7470A	PPB	01 Mar 2019 12:43:14	U	SMPL
K1349-14 - 1	OR-03-022719-A	20	0.0058	-7470A	PPB	01 Mar 2019 12:45:20	U	SMPL
K1349-16 - 1	OR-03-022719-B	12	0.0038	-7470A	PPB	01 Mar 2019 12:47:27	U	SMPL
K1358-06 - 1	TR-05-022719	22	0.0062	-7470A	PPB	01 Mar 2019 12:49:33	U	SMPL
K1643-02 - 1	INTERIOR-WALL	38	0.0101	-7470A	PPB	01 Mar 2019 12:51:40	U	SMPL
K1643-04 - 1	FLOOR-SLAB	21	0.0060	-7470A	PPB	01 Mar 2019 12:53:48	U	SMPL
K1645-04 - 1	SR-10	49	0.0127	-7470A	PPB	01 Mar 2019 12:55:55	U	SMPL
K1645-08 - 1	SR-9-S	40	0.0106	-7470A	PPB	01 Mar 2019 12:58:03	U	SMPL
K1645-12 - 1	SR-9-D	33	0.0089	-7470A	PPB	01 Mar 2019 13:00:11	U	SMPL
K1647-05 - 1	44766	39	0.0103	-7470A	PPB	01 Mar 2019 13:02:18	U	SMPL
CCV64 - 1	CCV64	20463	4.9314	-7470A	PPB	01 Mar 2019 13:04:24	U	SMPL
CCB64 - 1	CCB64	-40	-0.0087	-7470A	PPB	01 Mar 2019 13:06:31	U	SMPL
K1651-03 - 1	351-281	44	0.0115	-7470A	PPB	01 Mar 2019 13:08:37	U	SMPL
K1652-11 - 1	COMP-DAY-1	76	0.0192	-7470A	PPB	01 Mar 2019 13:10:44	U	SMPL
K1652-13 - 1	COMP-DAY-2	106	0.0265	-7470A	PPB	01 Mar 2019 13:12:50	U	SMPL
K1654-03 - 1	SOIL-PILE	65	0.0166	-7470A	PPB	01 Mar 2019 13:14:57	U	SMPL
PB117519TB - 1	PB117453TB	48	0.0125	-7470A	PPB	01 Mar 2019 13:17:04	U	SMPL
K1340-02LX5 - 1		3	0.0017	-7470A	PPB	01 Mar 2019 13:19:11	U	SMPL
K1340-02A - 1		16604	4.0016	-7470A	PPB	01 Mar 2019 13:21:18	U	SMPL
CCV65 - 1	CCV65	21440	5.1668	-7470A	PPB	01 Mar 2019 13:23:26	U	SMPL
CCB65 - 1	CCB65	-37	-0.0080	-7470A	PPB	01 Mar 2019 13:25:34	U	SMPL