


LB101252

7471B

INSTRUMENT ID: CV1

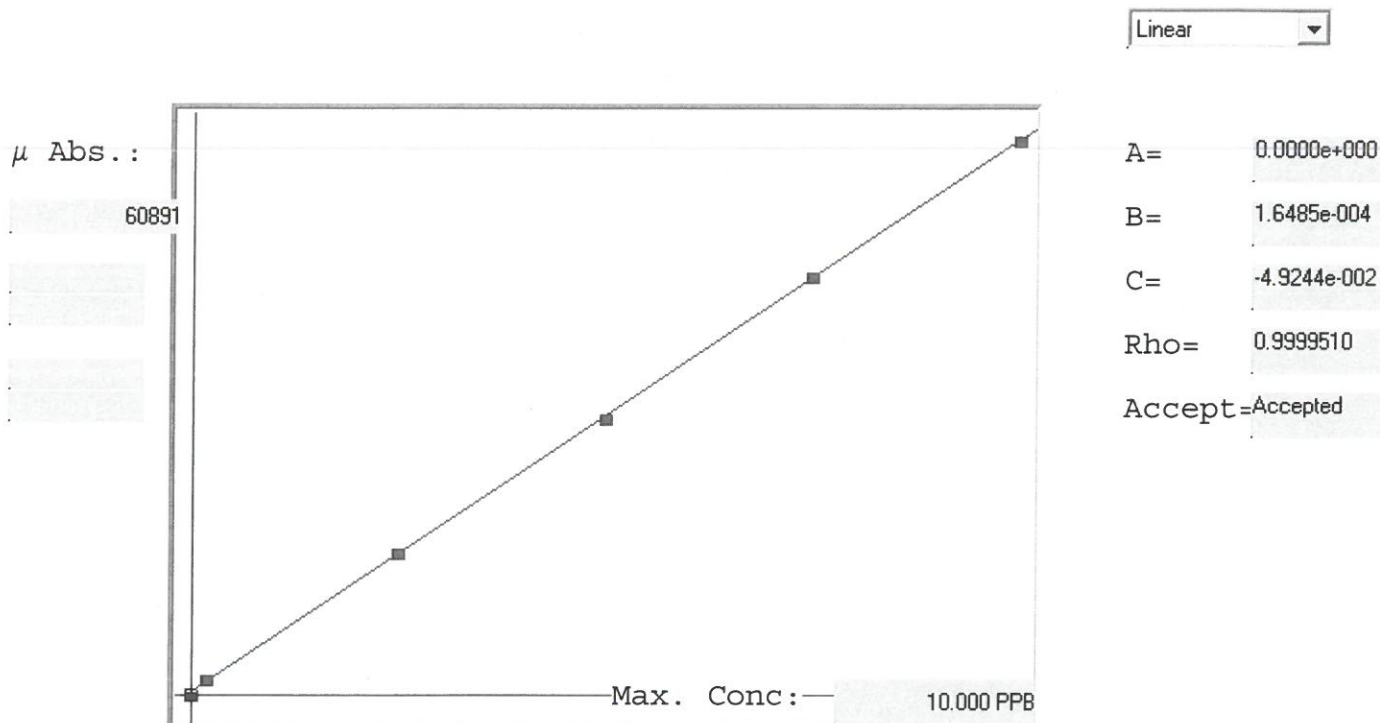

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.047	-0.047	12	0.000	12				
0.2	0.200	0.229	0.029	1687	0.0 %	1687				
2.5	2.500	2.546	0.046	15746	0.0 %	15746				
5.0	5.000	4.956	-0.044	30365	0.0 %	30365				
7.5	7.500	7.527	0.027	45961	0.0 %	45961				
10.0	10.000	9.988	-0.012	60891	0.0 %	60891				

LB101252 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 Mar 2019 10:13:15

Sample ID	Extended ID	μ Abs	Conc.	Std Cond	Method	Units	Date	Type	Type
0.0 - 1	50.0	12	-	0.0000	7471B	PPB	08 Mar 2019 10:15:21	S	Std
0.2 - 1	50.2	1687	-	0.2000	7471B	PPB	08 Mar 2019 10:17:38	S	Std
2.5 - 1	52.5	15746	-	2.5000	7471B	PPB	08 Mar 2019 10:19:56	S	Std
5.0 - 1	55.0	30365	-	5.0000	7471B	PPB	08 Mar 2019 10:22:13	S	Std
7.5 - 1	57.5	45961	-	7.5000	7471B	PPB	08 Mar 2019 10:24:30	S	Std
10.0 - 1	510.0	60891	-	10.0000	7471B	PPB	08 Mar 2019 10:26:47	S	Std
ICV47 - 1	ICV47	24592	4.0047	-	7471B	PPB	08 Mar 2019 10:30:23	U	SMPL
ICB47 - 1	ICB47	436	0.0226	-	7471B	PPB	08 Mar 2019 10:32:37	U	SMPL
CCV15 - 1	CCV15	30164	4.9232	-	7471B	PPB	08 Mar 2019 10:34:53	U	SMPL
CCB15 - 1	CCB15	-40	-0.0558	-	7471B	PPB	08 Mar 2019 10:37:09	U	SMPL
CRA - 1	CRA	1702	0.2313	-	7471B	PPB	08 Mar 2019 10:39:25	U	SMPL
HighStd - 1	HighStd	61319	10.0590	-	7471B	PPB	08 Mar 2019 10:41:40	U	SMPL
ChkStd - 1	ChkStd	43161	7.0657	-	7471B	PPB	08 Mar 2019 10:43:56	U	SMPL
PB117740BL - 1	PBS	-32	-0.0545	-	7471B	PPB	08 Mar 2019 10:46:14	U	SMPL
PB117740BS - 1	LCSS	22202	3.6107	-	7471B	PPB	08 Mar 2019 10:48:32	U	SMPL
K1807-01 - 1	TP-1	2049	0.2885	-	7471B	PPB	08 Mar 2019 10:50:48	U	SMPL
K1807-01DUP - 1	TP-1DUP	2088	0.2950	-	7471B	PPB	08 Mar 2019 10:53:05	U	SMPL
K1807-01MS - 1	TP-1MS	23769	3.8690	-	7471B	PPB	08 Mar 2019 10:55:22	U	SMPL
K1807-01MSD - 1	TP-1MSD	23803	3.8746	-	7471B	PPB	08 Mar 2019 10:57:39	U	SMPL
K1807-03 - 1	TP-2	8124	1.2900	-	7471B	PPB	08 Mar 2019 10:59:55	U	SMPL
CCV16 - 1	CCV16	30445	4.9695	-	7471B	PPB	08 Mar 2019 11:02:11	U	SMPL
CCB16 - 1	CCB16	149	-0.0247	-	7471B	PPB	08 Mar 2019 11:04:26	U	SMPL
K1807-05 - 1	TP-3	4869	0.7534	-	7471B	PPB	08 Mar 2019 11:06:44	U	SMPL
K1807-07 - 1	TP-4	1968	0.2752	-	7471B	PPB	08 Mar 2019 11:09:00	U	SMPL
K1807-09 - 1	TP-5	3777	0.5734	-	7471B	PPB	08 Mar 2019 11:11:16	U	SMPL
K1807-11 - 1	TP-6	2044	0.2877	-	7471B	PPB	08 Mar 2019 11:13:32	U	SMPL
K1807-13 - 1	TP-7	2227	0.3179	-	7471B	PPB	08 Mar 2019 11:15:48	U	SMPL
K1807-15 - 1	TP-8	1229	0.1534	-	7471B	PPB	08 Mar 2019 11:18:05	U	SMPL
K1807-17 - 1	TP-9	2452	0.3550	-	7471B	PPB	08 Mar 2019 11:20:22	U	SMPL
K1807-19 - 1	TP-10	1939	0.2704	-	7471B	PPB	08 Mar 2019 11:22:39	U	SMPL
K1807-21 - 1	TP-18	1198	0.1482	-	7471B	PPB	08 Mar 2019 11:24:56	U	SMPL
K1807-23 - 1	TP-17	8987	1.4322	-	7471B	PPB	08 Mar 2019 11:27:11	U	SMPL
CCV17 - 1	CCV17	30558	4.9881	-	7471B	PPB	08 Mar 2019 11:29:27	U	SMPL
CCB17 - 1	CCB17	-87	-0.0636	-	7471B	PPB	08 Mar 2019 11:31:43	U	SMPL
K1807-25 - 1	TP-16	1539	0.2045	-	7471B	PPB	08 Mar 2019 11:34:00	U	SMPL
K1807-27 - 1	TP-15	2074	0.2926	-	7471B	PPB	08 Mar 2019 11:36:15	U	SMPL
K1807-29 - 1	TP-14	2576	0.3754	-	7471B	PPB	08 Mar 2019 11:38:31	U	SMPL
K1807-31 - 1	TP-13	3117	0.4646	-	7471B	PPB	08 Mar 2019 11:40:47	U	SMPL
K1807-33 - 1	TP-12	2241	0.3202	-	7471B	PPB	08 Mar 2019 11:43:03	U	SMPL
K1807-35 - 1	TP-11	5616	0.8765	-	7471B	PPB	08 Mar 2019 11:45:20	U	SMPL
K1807-37 - 1	TP-19	2229	0.3182	-	7471B	PPB	08 Mar 2019 11:47:36	U	SMPL
K1807-39 - 1	TP-20	4887	0.7564	-	7471B	PPB	08 Mar 2019 11:49:53	U	SMPL
K1807-41 - 1	TP-21	1707	0.2321	-	7471B	PPB	08 Mar 2019 11:52:11	U	SMPL
K1807-43 - 1	TP-22	1417	0.1843	-	7471B	PPB	08 Mar 2019 11:54:27	U	SMPL
CCV18 - 1	CCV18	31080	5.0742	-	7471B	PPB	08 Mar 2019 11:56:43	U	SMPL
CCB18 - 1	CCB18	157	-0.0234	-	7471B	PPB	08 Mar 2019 11:58:58	U	SMPL
K1807-45 - 1	TP-23	5339	0.8309	-	7471B	PPB	08 Mar 2019 12:01:15	U	SMPL
PB117741BL - 1	PBS	61	-0.0392	-	7471B	PPB	08 Mar 2019 12:03:30	U	SMPL
PB117741BS - 1	LCSS	21719	3.5311	-	7471B	PPB	08 Mar 2019 12:05:46	U	SMPL
K1693-01 - 1	OR-01-030719-A	13875	2.2380	-	7471B	PPB	08 Mar 2019 12:08:01	U	SMPL
K1693-01DUP - 1	OR-01-030719-ADUP	13778	2.2220	-	7471B	PPB	08 Mar 2019 12:10:19	U	SMPL
K1693-01MS - 1	OR-01-030719-AMS	39335	6.4350	-	7471B	PPB	08 Mar 2019 12:24:41	U	SMPL
K1693-01MSD - 1	OR-01-030719-AMSD	39647	6.4864	-	7471B	PPB	08 Mar 2019 12:26:57	U	SMPL
K1693-03 - 1	OR-01-030719-B	1592	0.2132	-	7471B	PPB	08 Mar 2019 12:29:16	U	SMPL
K1787-01 - 1	SP-1	1223	0.1524	-	7471B	PPB	08 Mar 2019 12:31:34	U	SMPL
K1808-01 - 1	FK-BPM-01-AA0-BB0-AA0A-BB0A	1330	0.1700	-	7471B	PPB	08 Mar 2019 12:33:50	U	SMPL
CCV19 - 1	CCV19	31045	5.0684	-	7471B	PPB	08 Mar 2019 12:36:06	U	SMPL
CCB19 - 1	CCB19	91	-0.0342	-	7471B	PPB	08 Mar 2019 12:38:21	U	SMPL
K1809-01 - 1	FK-BPM-01-A0-B0-A0A-A0B	1073	0.1276	-	7471B	PPB	08 Mar 2019 12:40:38	U	SMPL
K1807-01LX5 - 1		363	0.0106	-	7471B	PPB	08 Mar 2019 12:42:54	U	SMPL
K1807-01A - 1		23419	3.8113	-	7471B	PPB	08 Mar 2019 12:45:10	U	SMPL
K1693-01LX5 - 1		2625	0.3835	-	7471B	PPB	08 Mar 2019 12:47:26	U	SMPL
K1693-01A - 1		38499	6.2972	-	7471B	PPB	08 Mar 2019 12:49:42	U	SMPL
CCV20 - 1	CCV20	30633	5.0005	-	7471B	PPB	08 Mar 2019 12:51:58	U	SMPL
CCB20 - 1	CCB20	18	-0.0463	-	7471B	PPB	08 Mar 2019 12:54:16	U	SMPL