


LB101309

7470A

INSTRUMENT ID : CV1

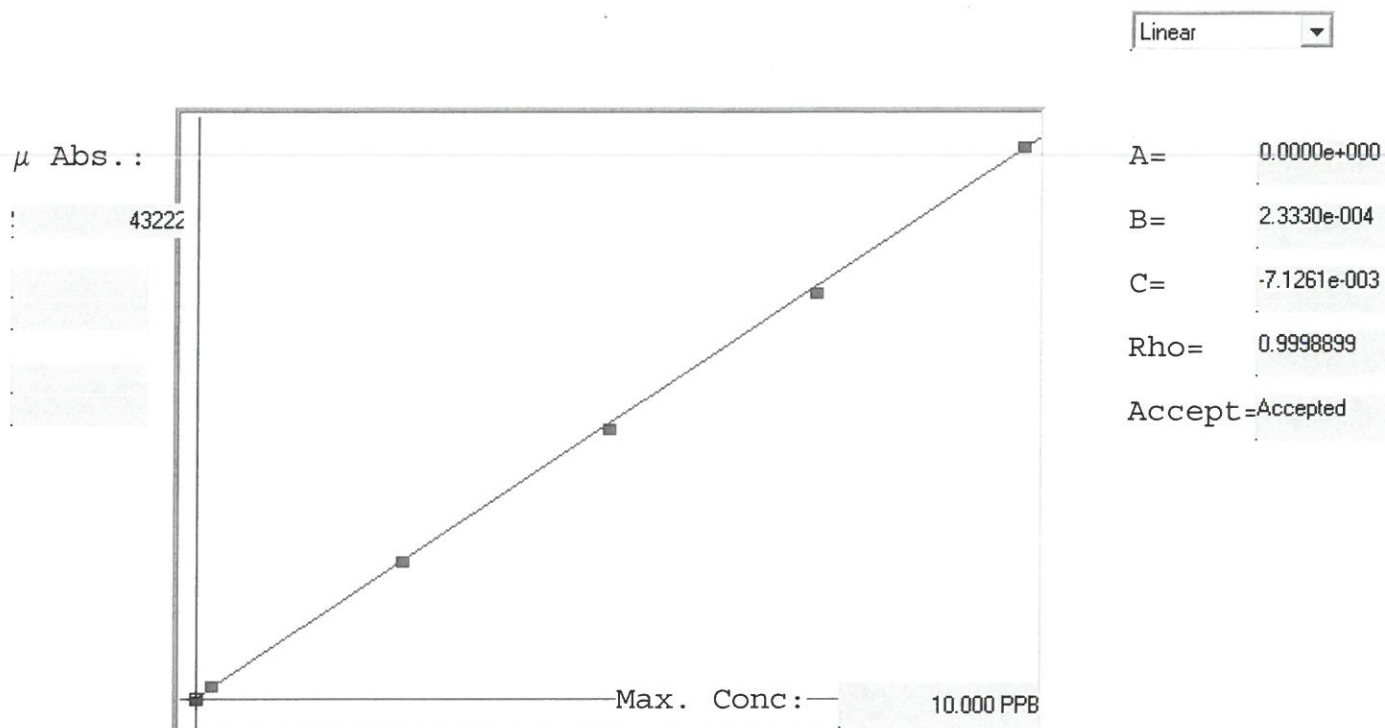

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.014	-0.014	-30	0.000	-30				
0.2	0.200	0.250	0.050	1101	0.0 %	1101				
2.5	2.500	2.521	0.021	10837	0.0 %	10837				
5.0	5.000	4.939	-0.061	21199	0.0 %	21199				
7.5	7.500	7.428	-0.072	31868	0.0 %	31868				
10.0	10.000	10.077	0.077	43222	0.0 %	43222				

LB101309 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 12 Mar 2019 14:54:35

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	S0-0	-30	-	0.00007470A	PPB		12 Mar 2019 15:13:10	S	Std
0.2 - 1	S0-2	1101	-	0.20007470A	PPB		12 Mar 2019 15:15:18	S	Std
2.5 - 1	S2-5	10837	-	2.50007470A	PPB		12 Mar 2019 15:17:26	S	Std
5.0 - 1	S5-0	21199	-	5.00007470A	PPB		12 Mar 2019 15:19:34	S	Std
7.5 - 1	S7-5	31868	-	7.50007470A	PPB		12 Mar 2019 15:21:41	S	Std
10.0 - 1	S10-0	43222	-	10.00007470A	PPB		12 Mar 2019 15:23:48	S	Std
ICV51 - 1	ICV51	17746	4.1331	-7470A	PPB		12 Mar 2019 15:30:34	U	SMPL
ICB51 - 1	ICB51	-1	-0.0074	-7470A	PPB		12 Mar 2019 15:35:40	U	SMPL
CCV41 - 1	CCV41	21328	4.9688	-7470A	PPB		12 Mar 2019 15:37:46	U	SMPL
CCB41 - 1	CCB41	-37	-0.0158	-7470A	PPB		12 Mar 2019 15:39:52	U	SMPL
CRA - 1	CRA	1078	0.2444	-7470A	PPB		12 Mar 2019 15:41:58	U	SMPL
HighStd - 1	HighStd	43173	10.0653	-7470A	PPB		12 Mar 2019 15:44:03	U	SMPL
ChkStd - 1	ChkStd	29824	6.9509	-7470A	PPB		12 Mar 2019 15:46:09	U	SMPL
PB117808BL - 1	PBW	124	0.0218	-7470A	PPB		12 Mar 2019 15:48:16	U	SMPL
PB117808BS - 1	LCSW	17697	4.1216	-7470A	PPB		12 Mar 2019 15:50:23	U	SMPL
K1834-18 - 1	COMP-2-AU	183	0.0356	-7470A	PPB		12 Mar 2019 15:52:30	U	SMPL
K1834-18DUP - 1	COMP-2-AUDUP	233	0.0472	-7470A	PPB		12 Mar 2019 15:54:38	U	SMPL
K1834-18MS - 1	COMP-2-AUMS	17336	4.0374	-7470A	PPB		12 Mar 2019 15:56:45	U	SMPL
K1834-18MSD - 1	COMP-2-AUMSD	17305	4.0302	-7470A	PPB		12 Mar 2019 15:58:53	U	SMPL
PB117809BL - 1	PBW	44	0.0031	-7470A	PPB		12 Mar 2019 16:01:00	U	SMPL
CCV42 - 1	CCV42	21319	4.9667	-7470A	PPB		12 Mar 2019 16:03:06	U	SMPL
CCB42 - 1	CCB42	40	0.0022	-7470A	PPB		12 Mar 2019 16:05:12	U	SMPL
PB117809BS - 1	LCSW	18257	4.2523	-7470A	PPB		12 Mar 2019 16:07:18	U	SMPL
K1689-02 - 1	NB-07-030819	210	0.0419	-7470A	PPB		12 Mar 2019 16:09:24	U	SMPL
K1689-02DUP - 1	NB-07-030819DUP	248	0.0507	-7470A	PPB		12 Mar 2019 16:11:31	U	SMPL
K1689-02MS - 1	NB-07-030819MS	17594	4.0976	-7470A	PPB		12 Mar 2019 16:13:37	U	SMPL
K1689-02MSD - 1	NB-07-030819MSD	17397	4.0517	-7470A	PPB		12 Mar 2019 16:15:44	U	SMPL
K1691-02 - 1	CL-02-030819-A	291	0.0608	-7470A	PPB		12 Mar 2019 16:17:51	U	SMPL
K1691-04 - 1	CL-02-030819-B	497	0.1088	-7470A	PPB		12 Mar 2019 16:19:59	U	SMPL
K1691-06 - 1	CL-02-030819-C	155	0.0290	-7470A	PPB		12 Mar 2019 16:22:08	U	SMPL
K1691-08 - 1	CL-02-030819-D	300	0.0629	-7470A	PPB		12 Mar 2019 16:24:16	U	SMPL
K1692-02 - 1	OK-01-030819	362	0.0773	-7470A	PPB		12 Mar 2019 16:26:22	U	SMPL
CCV43 - 1	CCV43	22334	5.2035	-7470A	PPB		12 Mar 2019 16:28:28	U	SMPL
CCB43 - 1	CCB43	52	0.0050	-7470A	PPB		12 Mar 2019 16:30:35	U	SMPL
K1822-03 - 1	3-8-BOD	297	0.0622	-7470A	PPB		12 Mar 2019 16:32:42	U	SMPL
K1834-21 - 1	COMP-1-AU	326	0.0689	-7470A	PPB		12 Mar 2019 16:34:48	U	SMPL
K1835-04 - 1	TP-3	384	0.0825	-7470A	PPB		12 Mar 2019 16:36:54	U	SMPL
K1836-01 - 1	OILY-DEBRIS	350	0.0745	-7470A	PPB		12 Mar 2019 16:39:01	U	SMPL
PB117810BL - 1	PBW	371	0.0794	-7470A	PPB		12 Mar 2019 16:41:08	U	SMPL
PB117810BS - 1	LCSW	18135	4.2238	-7470A	PPB		12 Mar 2019 16:43:15	U	SMPL
K1837-02 - 1	MR-MH-11-COMP	137	0.0248	-7470A	PPB		12 Mar 2019 16:45:22	U	SMPL
K1837-04 - 1	MR-MH-10-COMP	199	0.0393	-7470A	PPB		12 Mar 2019 16:47:30	U	SMPL
K1837-06 - 1	MR-MH-09-COMP	208	0.0414	-7470A	PPB		12 Mar 2019 16:49:39	U	SMPL
K1837-08 - 1	MR-MH-08-COMP	202	0.0400	-7470A	PPB		12 Mar 2019 16:51:45	U	SMPL
CCV44 - 1	CCV44	21721	5.0605	-7470A	PPB		12 Mar 2019 16:53:52	U	SMPL
CCB44 - 1	CCB44	53	0.0052	-7470A	PPB		12 Mar 2019 16:55:58	U	SMPL
K1837-10 - 1	MR-MH-07-COMP	261	0.0538	-7470A	PPB		12 Mar 2019 16:58:05	U	SMPL
K1837-12 - 1	MR-MH-06-COMP	205	0.0407	-7470A	PPB		12 Mar 2019 17:00:11	U	SMPL
K1837-14 - 1	MR-MH-05-COMP	200	0.0395	-7470A	PPB		12 Mar 2019 17:02:18	U	SMPL
K1837-14DUP - 1	MR-MH-05-COMPDUP	204	0.0405	-7470A	PPB		12 Mar 2019 17:04:24	U	SMPL
K1837-14MS - 1	MR-MH-05-COMPMS	17585	4.0955	-7470A	PPB		12 Mar 2019 17:06:31	U	SMPL
K1837-14MSD - 1	MR-MH-05-COMPMSD	17351	4.0409	-7470A	PPB		12 Mar 2019 17:08:38	U	SMPL
PB117822BL - 1	PBW	-3	-0.0078	-7470A	PPB		12 Mar 2019 17:10:46	U	SMPL
PB117822BS - 1	LCSW	18269	4.2551	-7470A	PPB		12 Mar 2019 17:12:54	U	SMPL
K1844-02 - 1	DRUM-1-4	610	0.1352	-7470A	PPB		12 Mar 2019 17:15:02	U	SMPL
K1844-02DUP - 1	DRUM-1-4DUP	648	0.1441	-7470A	PPB		12 Mar 2019 17:17:08	U	SMPL
CCV45 - 1	CCV45	21425	4.9914	-7470A	PPB		12 Mar 2019 17:19:15	U	SMPL
CCB45 - 1	CCB45	41	0.0024	-7470A	PPB		12 Mar 2019 17:21:21	U	SMPL
K1844-02MS - 1	DRUM-1-4MS	19855	4.6251	-7470A	PPB		12 Mar 2019 17:23:28	U	SMPL
K1844-02MSD - 1	DRUM-1-4MSD	19958	4.6491	-7470A	PPB		12 Mar 2019 17:25:34	U	SMPL
PB117808TB - 1	PB117775TB	132	0.0237	-7470A	PPB		12 Mar 2019 17:27:41	U	SMPL
PB117809TB - 1	PB117769TB	165	0.0314	-7470A	PPB		12 Mar 2019 17:29:48	U	SMPL
PB117810TB - 1	PB117774TB	180	0.0349	-7470A	PPB		12 Mar 2019 17:31:54	U	SMPL
K1834-18LX5 - 1		10	-0.0048	-7470A	PPB		12 Mar 2019 17:34:02	U	SMPL
K1834-18A - 1		17309	4.0311	-7470A	PPB		12 Mar 2019 17:36:09	U	SMPL
K1689-02LX5 - 1		-5	-0.0083	-7470A	PPB		12 Mar 2019 17:38:17	U	SMPL
K1689-02A - 1		17733	4.1300	-7470A	PPB		12 Mar 2019 17:40:25	U	SMPL
K1837-14LX5 - 1		-4	-0.0081	-7470A	PPB		12 Mar 2019 17:42:31	U	SMPL
CCV46 - 1	CCV46	22075	5.1431	-7470A	PPB		12 Mar 2019 17:44:38	U	SMPL
CCB46 - 1	CCB46	5	-0.0060	-7470A	PPB		12 Mar 2019 17:46:45	U	SMPL
K1837-14A - 1		17408	4.0542	-7470A	PPB		12 Mar 2019 17:48:52	U	SMPL
K1844-02LX5 - 1		69	0.0090	-7470A	PPB		12 Mar 2019 17:50:59	U	SMPL
K1844-02A - 1		20009	4.6610	-7470A	PPB		12 Mar 2019 17:53:06	U	SMPL
CCV47 - 1	CCV47	21993	5.1239	-7470A	PPB		12 Mar 2019 17:55:13	U	SMPL
CCB47 - 1	CCB47	-8	-0.0090	-7470A	PPB		12 Mar 2019 17:57:20	U	SMPL